
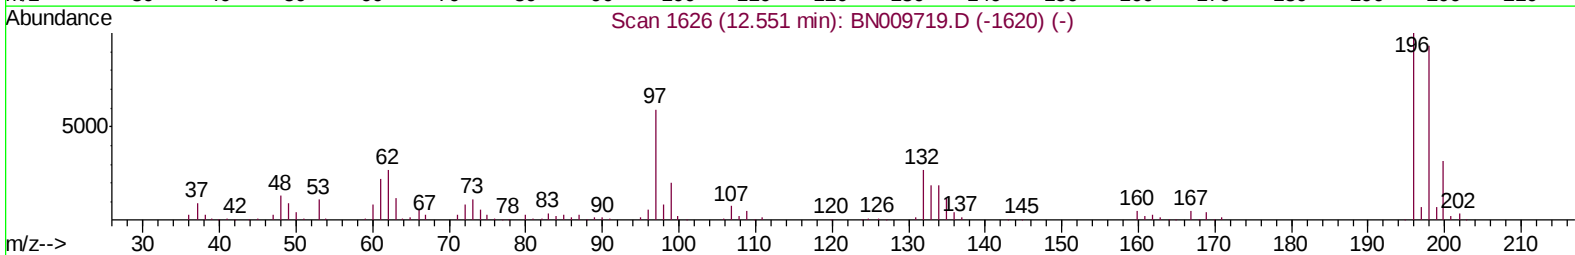
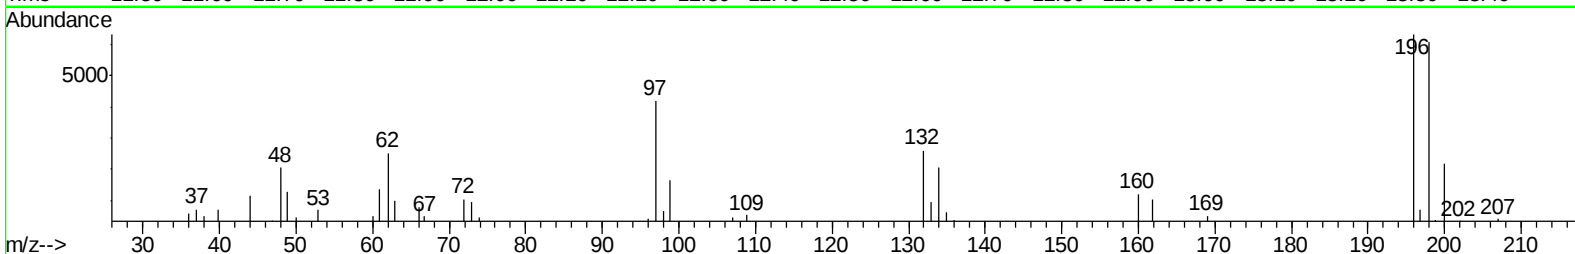


Data File : BN009726.D
Acq On : 14 Feb 2020 15:25
Operator : CG/JU
Sample : K5695-13
Misc : MDL-WATER-06
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Feb 17 00:53:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 17 00:47:25 2020
Response via : Initial Calibration

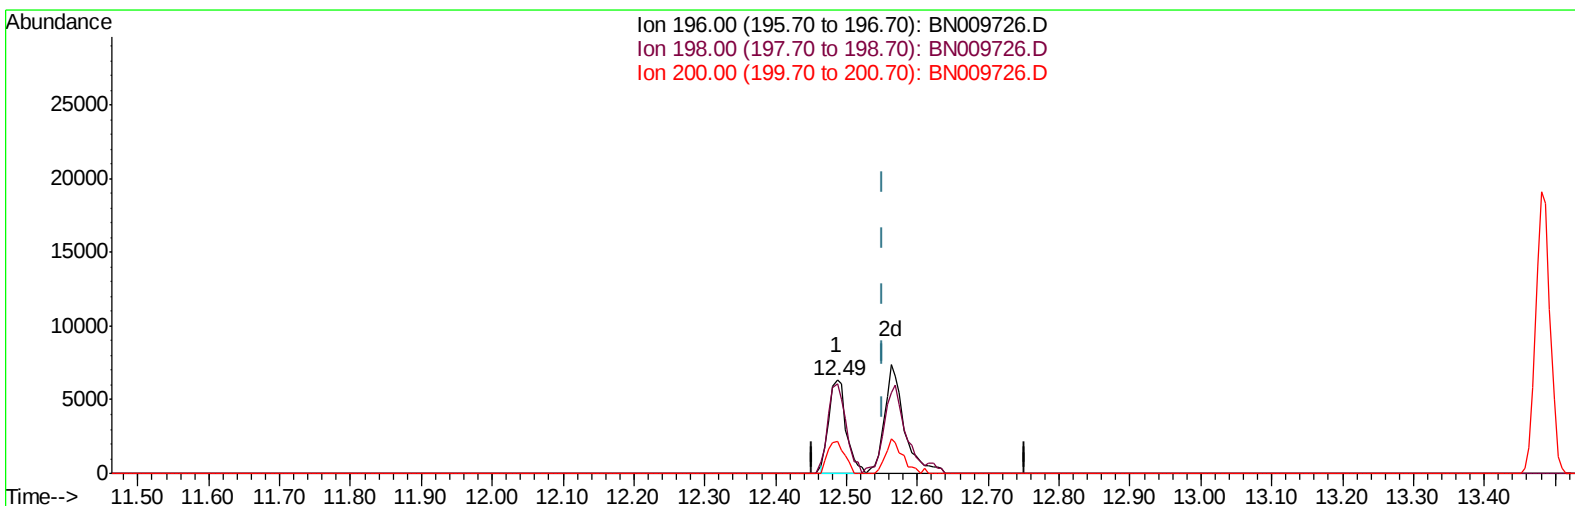

TIC: BN009726.D

(40) 2,4,5-Trichlorophenol
12.487min (-0.065) 1.87ng/ul
response 10781

Ion	Exp%	Act%
196.00	100	100
198.00	93.80	96.08
200.00	30.30	34.38
0.00	0.00	0.00