
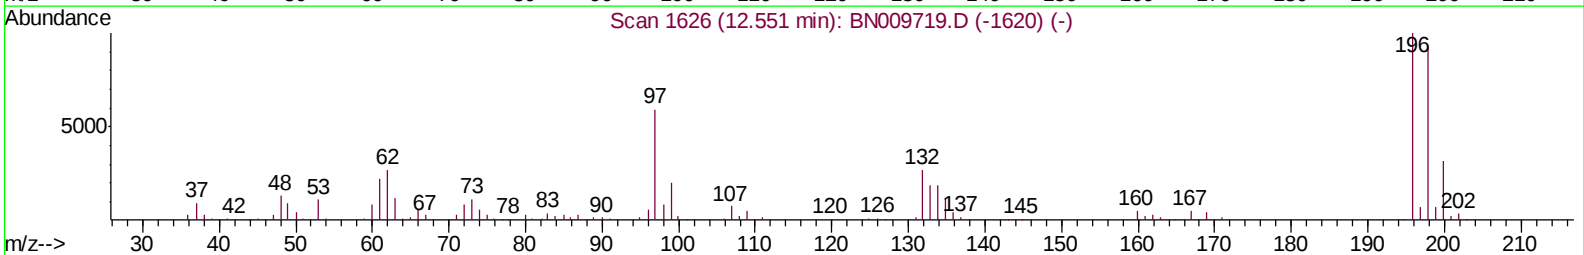
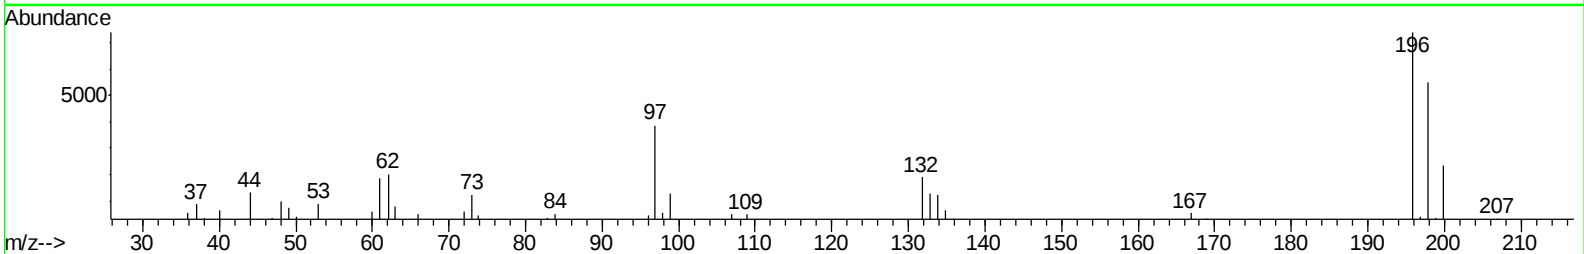


Data File : BN009726.D
Acq On : 14 Feb 2020 15:25
Operator : CG/JU
Sample : K5695-13
Misc : MDL-WATER-06
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Feb 17 00:53:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 17 00:47:25 2020
Response via : Initial Calibration

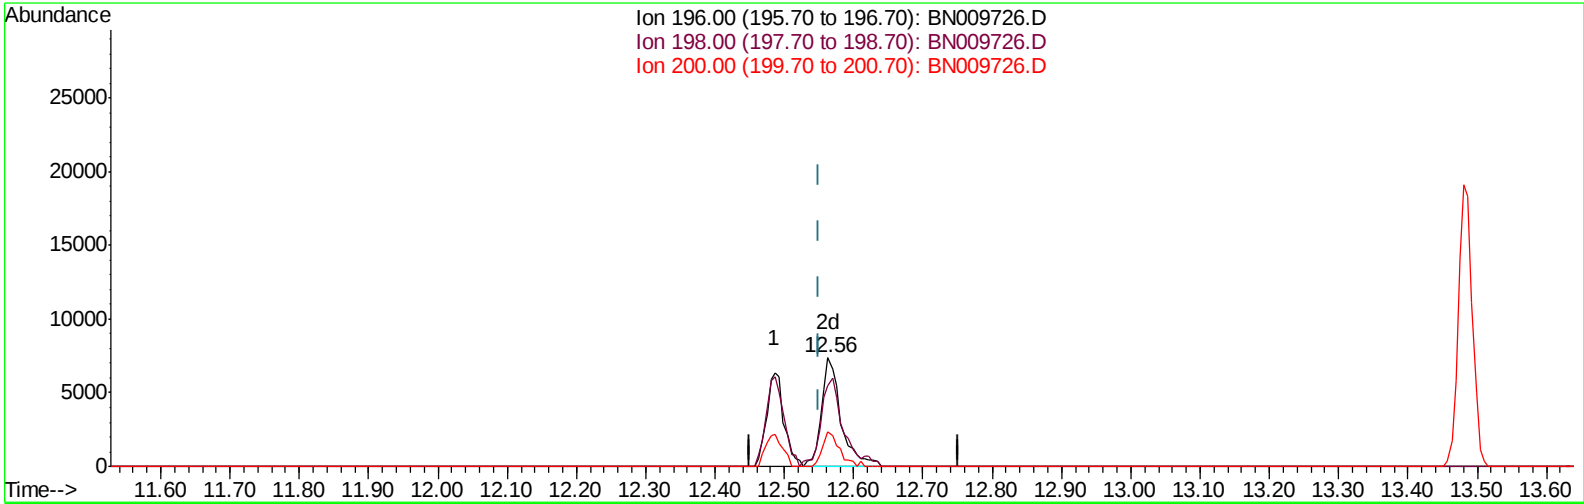

TIC: BN009726.D

(40) 2,4,5-Trichlorophenol

12.563min (+0.012) 2.48ng/ul m

response 14311

Ion	Exp%	Act%
196.00	100	100
198.00	93.80	74.74#
200.00	30.30	32.06
0.00	0.00	0.00