

Data File : BN009726.D

Acq On : 14 Feb 2020 15:25

Operator : CG/JU

Sample : K5695-13

Misc : MDL-WATER-06

ALS Vial : 9 Sample Multiplier: 1




Quant Time: Feb 17 00:53:14 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon Feb 17 00:47:25 2020

Response via : Initial Calibration

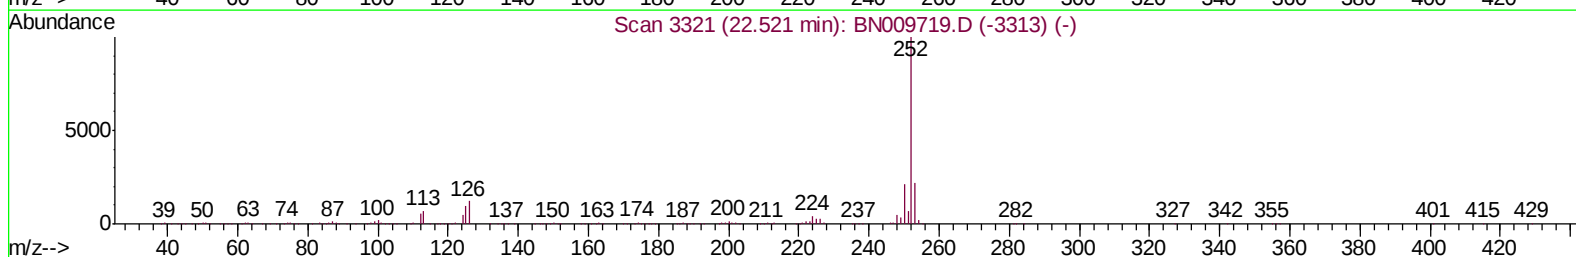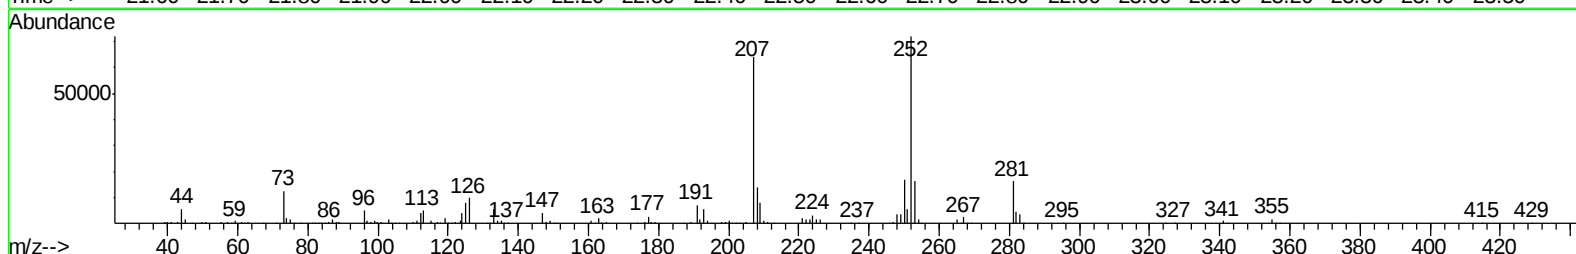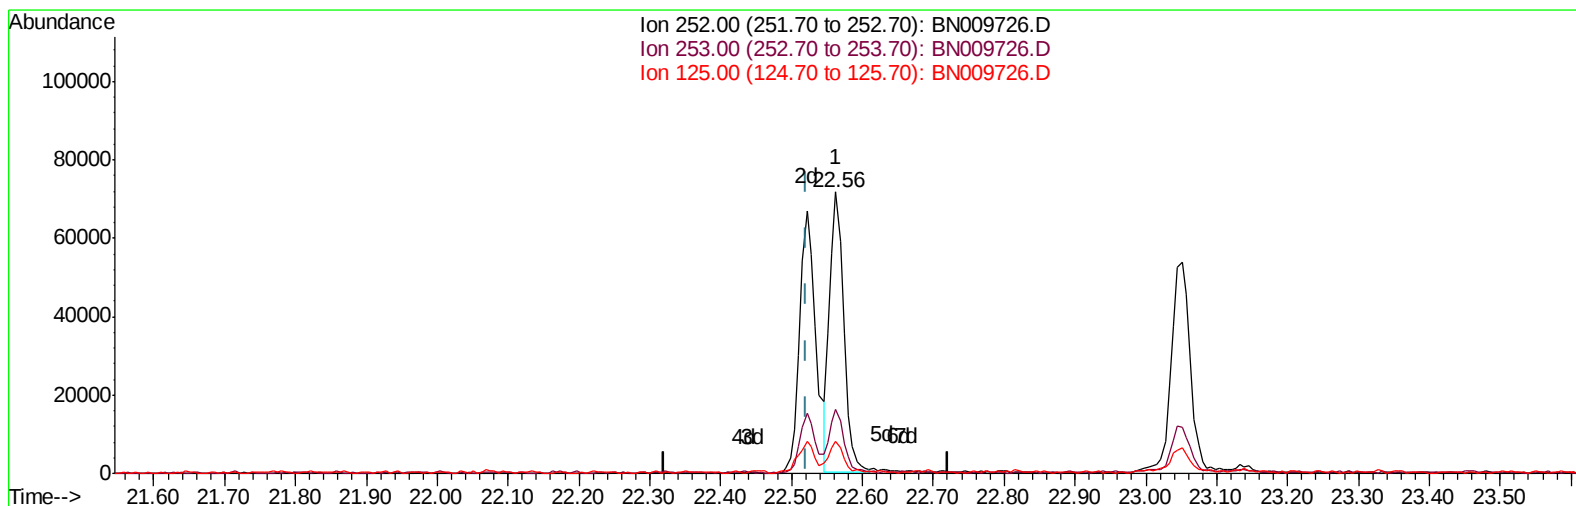

TIC: BN009726.D

(88) Benzo(b)fluoranthene

22.563min (+0.041) 2.60ng/ul

response 100381

Ion	Exp%	Act%
252.00	100	100
253.00	21.20	22.65
125.00	10.00	11.60
0.00	0.00	0.00