
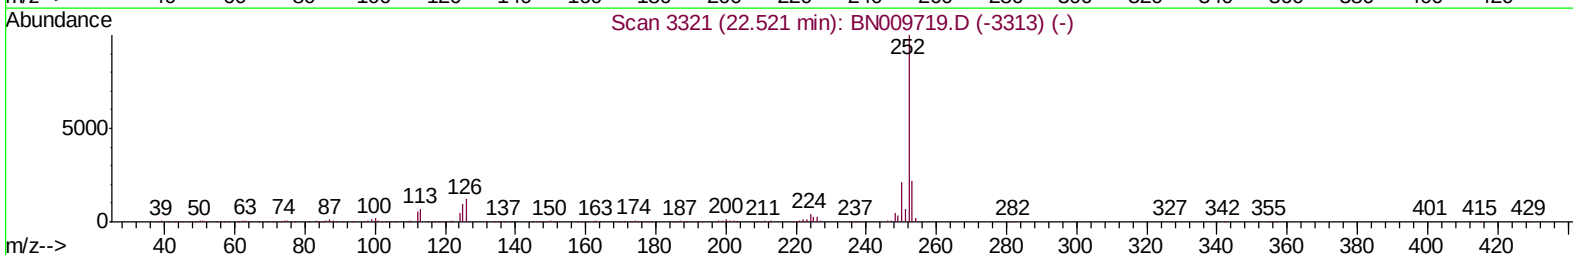
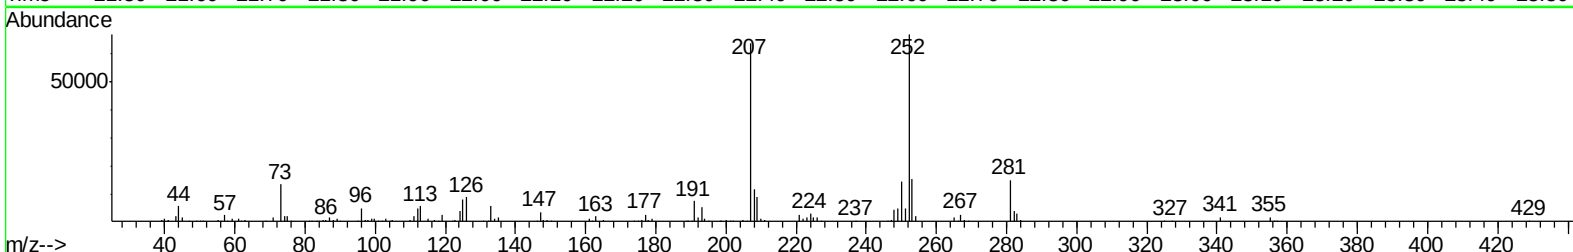


Data File : BN009726.D
Acq On : 14 Feb 2020 15:25
Operator : CG/JU
Sample : K5695-13
Misc : MDL-WATER-06
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Feb 17 00:53:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 17 00:47:25 2020
Response via : Initial Calibration

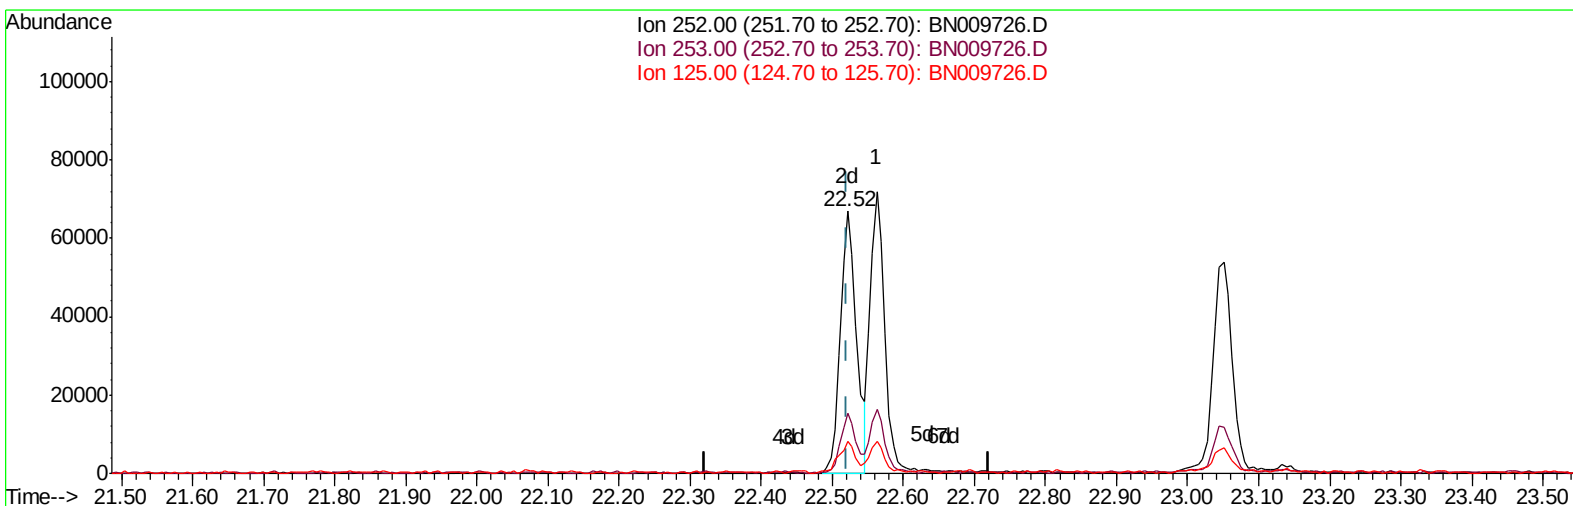

TIC: BN009726.D

(88) Benzo(b)fluoranthene

22.521min (-0.000) 2.73ng/ul m

response 105579

Ion	Exp%	Act%
252.00	100	100
253.00	21.20	22.77
125.00	10.00	12.15#
0.00	0.00	0.00