
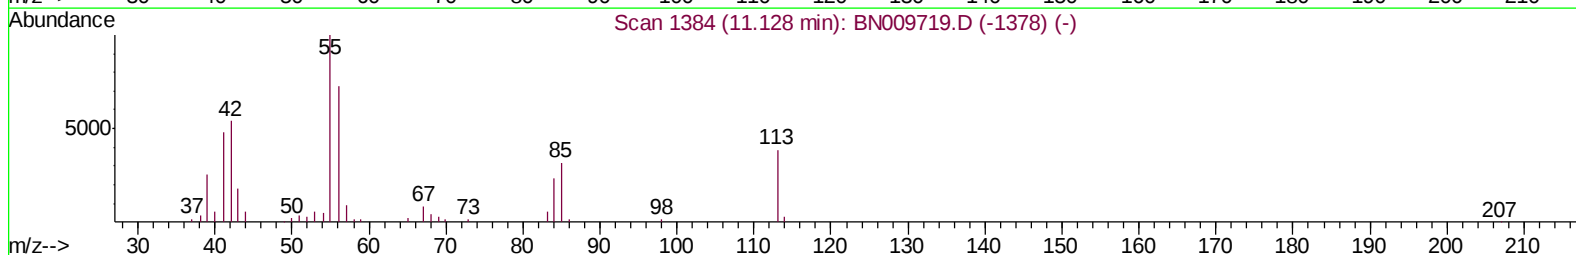
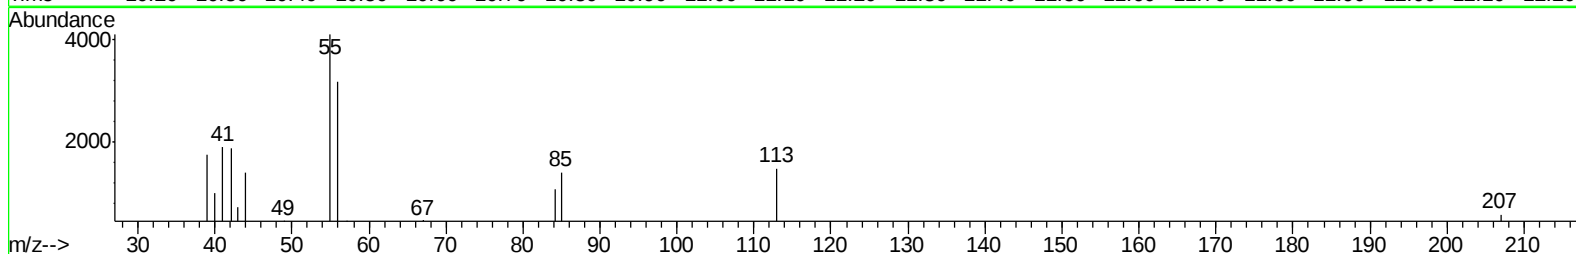


Data File : BN009727.D
Acq On : 14 Feb 2020 16:01
Operator : CG/JU
Sample : K5695-14
Misc : MDL-WATER-07
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Feb 17 00:53:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 17 00:47:25 2020
Response via : Initial Calibration

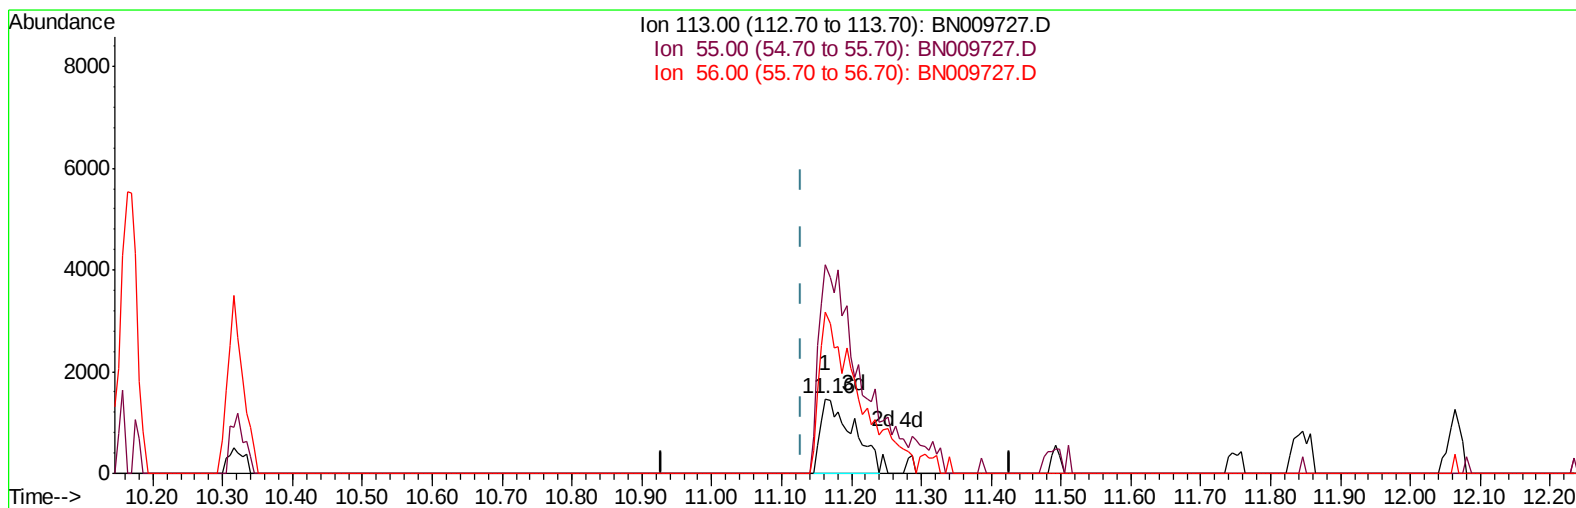

TIC: BN009727.D

(32) Caprolactam

11.163min (+0.035) 1.91ng/ul m

response 4689

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	279.28
56.00	202.00	216.17
0.00	0.00	0.00