

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN021420\
 Data File : BN009726.D
 Acq On : 14 Feb 2020 15:25
 Operator : CG/JU
 Sample : K5695-13
 Misc : MDL-WATER-06
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleID :
 MDL-WATER-06

Manual Integrations
 APPROVED

mohammad
 2/17/2020 3:50:13 PM

Quant Time: Feb 17 01:55:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 17 00:47:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	108811	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	447014	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	286057	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	613799	20.00	ng/ul	0.00
78) Chrysene-d12	21.03	240	599942	20.00	ng/ul	0.00
86) Perylene-d12	23.14	264	595728	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.06	96	11579	4.38	ng/uL	0.00
5) Phenol-d5	6.62	99	262971	28.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	190107	29.76	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	208232	29.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.13	113	207491	28.18	ng/ul	0.00
19) Nitrobenzene-d5	8.56	128	100414	30.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	109433	30.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	196539	28.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.32	131	278540	36.05	ng/ul	0.00
44) Dimethylphthalate-d6	13.48	166	653688	30.59	ng/ul	0.00
47) Acenaphthylene-d8	13.75	160	784133	31.16	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	93512	23.96	ng/ul	0.00
58) Fluorene-d10	15.06	176	561912	30.46	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.22	200	91422	23.98	ng/ul	0.00
71) Anthracene-d10	16.91	188	859459	30.55	ng/ul	0.00
79) Pyrene-d10	19.22	212	928437	29.61	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	906767	30.48	ng/ul	0.00

Target Compounds

					Qvalue
2) 1,4-Dioxane	3.09	88	2713	0.89 ng/ul	99
4) Benzaldehyde	6.59	77	18999	3.09 ng/ul	97
6) Phenol	6.65	94	26704	2.69 ng/ul	96
8) Bis(2-Chloroethyl)ether	6.87	93	22175	2.84 ng/ul	99
10) 2-Chlorophenol	6.99	128	19542	2.66 ng/ul	95
11) 2-Methylphenol	7.88	108	16965	2.34 ng/ul	94
12) 2,2'-oxybis(1-Chloropropan	7.95	45	56591m	2.96 ng/ul	
14) Acetophenone	8.24	105	31331	2.61 ng/ul	99
15) N-Nitroso-di-n-propylamine	8.23	70	17239	2.75 ng/ul	99
16) 4-Methylphenol	8.19	108	20943	2.63 ng/ul	94
17) Hexachloroethane	8.46	117	9936	2.98 ng/ul	88
20) Nitrobenzene	8.60	77	27830	2.89 ng/ul	98
21) Isophorone	9.13	82	42683	2.52 ng/ul	96
23) 2-Nitrophenol	9.30	139	10939	2.73 ng/ul#	79
24) 2,4-Dimethylphenol	9.38	107	23557	2.71 ng/ul	93
25) Bis(2-Chloroethoxy)methane	9.62	93	28437	2.74 ng/ul	97
27) 2,4-Dichlorophenol	9.83	162	18893	2.72 ng/ul#	74
28) Naphthalene	10.22	128	69485	2.88 ng/ul	98
30) 4-Chloroaniline	10.35	127	22745	2.87 ng/ul	95
31) Hexachlorobutadiene	10.50	225	13119	2.83 ng/ul#	89
32) Caprolactam	11.18	113	3895m	1.67 ng/ul	
33) 4-Chloro-3-methylphenol	11.49	107	18042	2.27 ng/ul	94
34) 2-Methylnaphthalene	11.85	142	46758	2.79 ng/ul	96

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN021420\
 Data File : BN009726.D
 Acq On : 14 Feb 2020 15:25
 Operator : CG/JU
 Sample : K5695-13
 Misc : MDL-WATER-06
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleID :
 MDL-WATER-06

Manual Integrations
 APPROVED

mohammad
 2/17/2020 3:50:13 PM

Quant Time: Feb 17 01:55:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 17 00:47:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.06	142	48640	2.90	ng/uL	98
37) 1,2,4,5-Tetrachlorobenzene	12.23	216	24695	2.91	ng/ul	93
38) Hexachlorocyclopentadiene	12.19	237	3117	0.85	ng/ul#	74
39) 2,4,6-Trichlorophenol	12.49	196	10975	2.04	ng/ul	99
40) 2,4,5-Trichlorophenol	12.56	196	14311m	2.48	ng/ul	
41) 1,1'-Biphenyl	12.88	154	62383	2.84	ng/ul	96
42) 2-Chloronaphthalene	12.92	162	47368	2.71	ng/ul	95
43) 2-Nitroaniline	13.15	65	14041	2.20	ng/ul	89
45) Dimethylphthalate	13.53	163	65265	2.93	ng/ul	99
46) 2,6-Dinitrotoluene	13.66	165	9675	2.22	ng/ul#	82
48) Acenaphthylene	13.77	152	77577	2.85	ng/ul	98
49) 3-Nitroaniline	14.00	138	8833	2.19	ng/ul#	90
50) Acenaphthene	14.12	153	53397	2.86	ng/ul	99
51) 2,4-Dinitrophenol	14.23	184	2145	0.86	ng/ul#	89
53) 4-Nitrophenol	14.31	109	9138	2.60	ng/ul	91
54) Dibenzofuran	14.46	168	75369	2.88	ng/ul	95
55) 2,4-Dinitrotoluene	14.46	165	15877	2.45	ng/ul#	99
56) 2,3,4,6-Tetrachlorophenol	14.70	232	11802	2.38	ng/ul#	92
57) Diethylphthalate	14.92	149	61445	2.68	ng/ul	97
59) Fluorene	15.12	166	62105	2.82	ng/ul	96
60) 4-Chlorophenyl-phenylether	15.12	204	31265	2.88	ng/ul	96
61) 4-Nitroaniline	15.17	138	7384	1.50	ng/ul	90
64) 4,6-Dinitro-2-methylphenol	15.23	198	10002	2.44	ng/ul#	75
65) N-Nitrosodiphenylamine	15.34	169	49318	2.71	ng/ul	94
66) 4-Bromophenyl-phenylether	16.02	248	16864	2.75	ng/ul	98
67) Hexachlorobenzene	16.13	284	18647	2.74	ng/ul	97
68) Atrazine	16.31	200	16020	2.32	ng/ul	91
69) Pentachlorophenol	16.49	266	6049	1.54	ng/ul#	78
70) Phenanthrene	16.86	178	100162	2.86	ng/ul	98
72) Anthracene	16.95	178	102444	2.86	ng/ul	99
73) 1,2,3,4-Tetrachlorobenzene	12.85	216	27331	3.05	ng/uL	95
74) Pentachlorobenzene	14.39	250	23735	2.74	ng/uL	95
75) Carbazole	17.23	167	72674	2.30	ng/ul	98
76) Di-n-butylphthalate	17.81	149	86413	2.22	ng/ul	99
77) Fluoranthene	18.89	202	104533	2.55	ng/ul	99
80) Pyrene	19.25	202	119517	2.76	ng/ul	99
81) Butylbenzylphthalate	20.18	149	35107	1.97	ng/ul	97
82) 3,3'-Dichlorobenzidine	20.96	252	29127	2.23	ng/ul#	92
83) Benzo(a)anthracene	21.02	228	107542	2.61	ng/ul	98
84) Bis(2-ethylhexyl)phthalate	20.97	149	54998	2.03	ng/ul	98
85) Chrysene	21.07	228	111800	2.75	ng/ul	98
87) Di-n-octyl phthalate	21.82	149	88852	1.97	ng/ul	100
88) Benzo(b)fluoranthene	22.52	252	105579m	2.73	ng/ul	
89) Benzo(k)fluoranthene	22.56	252	100381	2.74	ng/ul	99
91) Benzo(a)pyrene	23.05	252	102908	2.96	ng/ul	99
92) Indeno(1,2,3-cd)pyrene	25.20	276	108852	2.64	ng/ul	96
93) Dibenzo(a,h)anthracene	25.20	278	94035	2.67	ng/ul	97
94) Benzo(g,h,i)perylene	25.83	276	93275	2.70	ng/ul	96

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN021420\
Data File : BN009726.D
Acq On : 14 Feb 2020 15:25
Operator : CG/JU
Sample : K5695-13
Misc : MDL-WATER-06
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-06


Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM

Quant Time: Feb 17 01:55:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 17 00:47:25 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

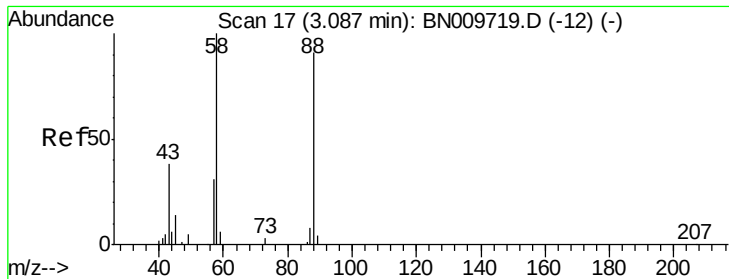

#2

1,4-Dioxane

Concen: 0.89 ng/uL

RT: 3.09 min Scan# 18

Delta R.T. 0.01 min

Lab File: BN009726.D


Acq: 14 Feb 2020 15:25

Instrument :

BNA_N

ClientSampleId :




MDL-WATER-06

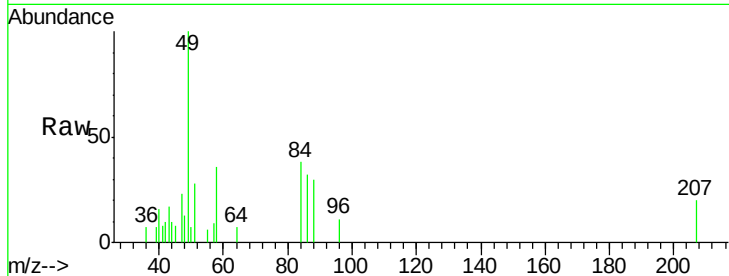

Tgt Ion:	88	Resp:	2713
Ion	Ratio	Lower	Upper
88	100		
43	57.0	44.7	67.1
58	121.8	96.2	144.2

Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM

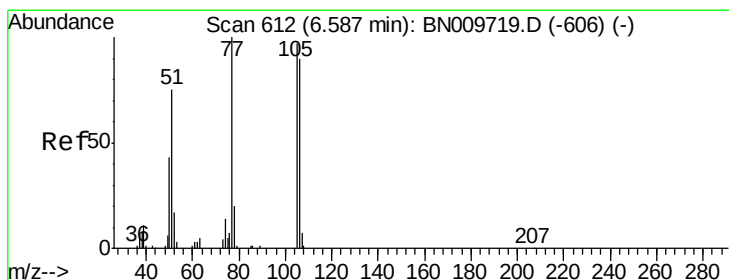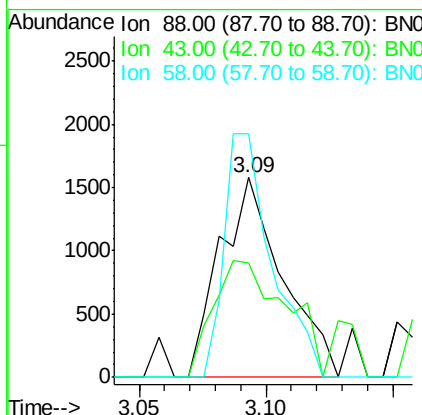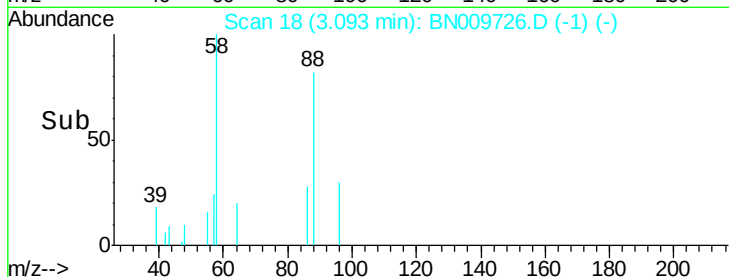

#4

Benzaldehyde


Concen: 3.09 ng/uL

RT: 6.59 min Scan# 613



Delta R.T. 0.01 min


Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

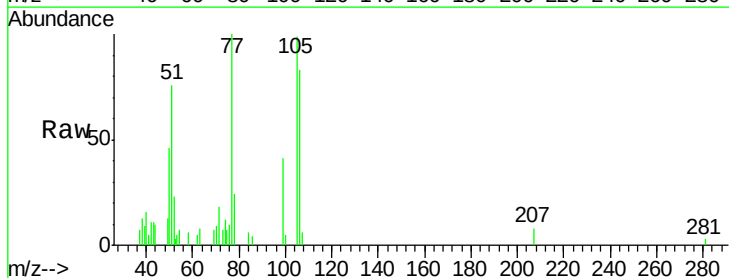

Tgt Ion:	77	Resp:	18999
Ion	Ratio	Lower	Upper
77	100		
105	99.0	78.2	117.2
106	83.3	70.9	106.3

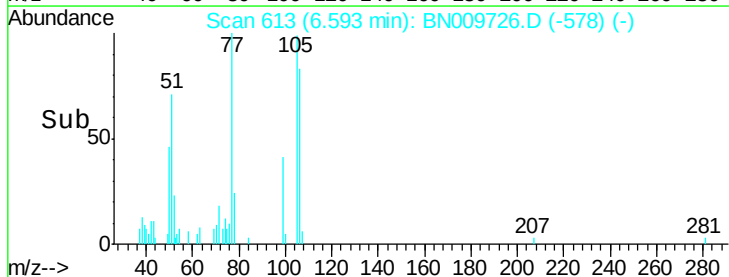



#6

Phenol

Concen: 2.69 ng/ul

RT: 6.65 min Scan# 622

Delta R.T. 0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-06

Tgt Ion:	94	Resp:	26704
Ion	Ratio	Lower	Upper
94	100		
65	36.3	27.6	41.4
66	51.7	38.5	57.7

Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM



#8

Bis(2-Chloroethyl)ether

Concen: 2.84 ng/ul




RT: 6.87 min Scan# 660


Delta R.T. 0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Tgt Ion:	93	Resp:	22175
Ion	Ratio	Lower	Upper
93	100		
63	103.6	82.7	124.1
95	30.4	26.6	40.0



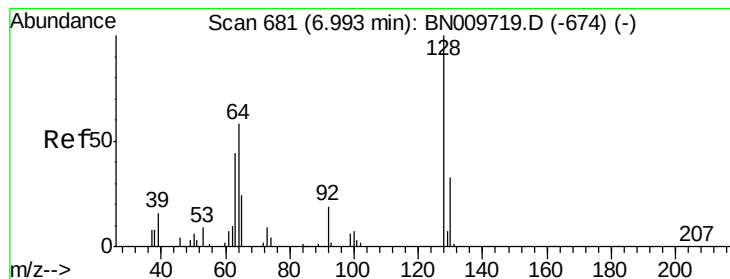





#10
2-Chlorophenol
Concen: 2.66 ng/ul
RT: 6.99 min Scan# 680
Delta R.T. -0.01 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-06

Tgt Ion	Ratio	Lower	Upper
128	100		
64	70.8	52.5	78.7
130	30.0	24.4	36.6




Manual Integrations
APPROVED


mohammad
2/17/2020 3:50:13 PM

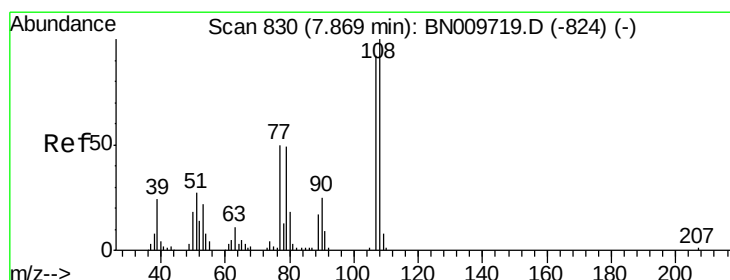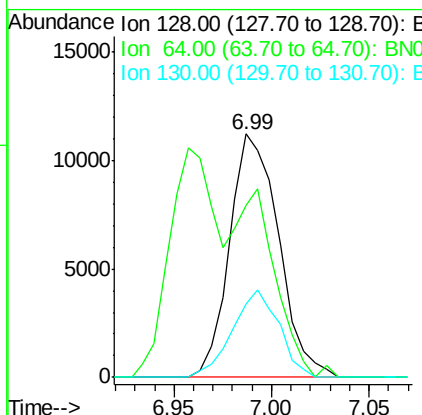

#11
2-Methylphenol
Concen: 2.34 ng/ul
RT: 7.88 min Scan# 831
Delta R.T. 0.01 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Lower	Upper
108	100		
107	95.6	72.3	108.5









#12
2,2'-oxybis(1-Chloropropane)
Concen: 2.96 ng/ul m
RT: 7.95 min Scan# 843
Delta R.T. -0.01 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-06

Tgt Ion	Ratio	Lower	Upper
45	100		
77	6.9	6.3	9.5
79	5.5	5.1	7.7




Manual Integrations
APPROVED


mohammad
2/17/2020 3:50:13 PM

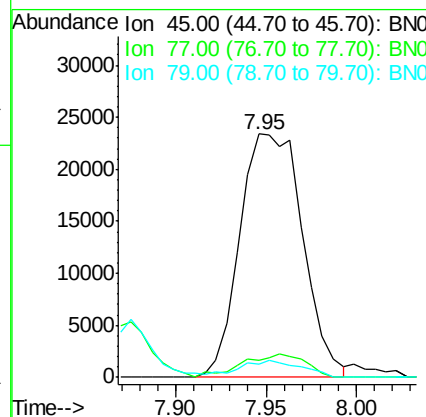

#14
Acetophenone
Concen: 2.61 ng/ul
RT: 8.24 min Scan# 893
Delta R.T. 0.01 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Lower	Upper
105	100		
77	85.2	68.9	103.3
51	44.3	35.6	53.4

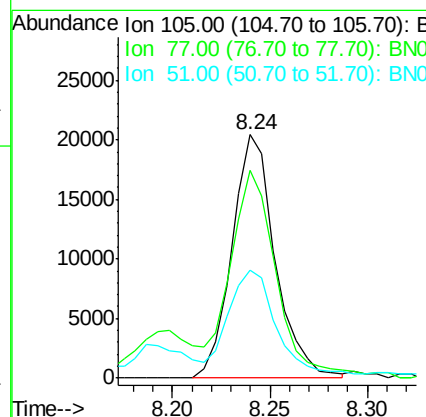



#15

N-Nitroso-di-n-propylamine

Concen: 2.75 ng/ul

RT: 8.23 min Scan# 891

Delta R.T. 0.01 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-06

Tgt Ion:	70	Resp:	17239
Ion	Ratio	Lower	Upper
70	100		
42	90.6	72.6	108.8
101	11.3	7.7	11.5
130	16.6	14.7	22.1

Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM

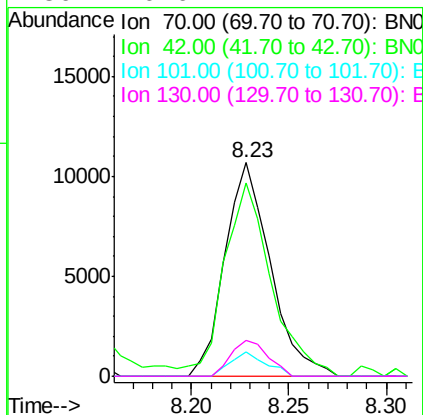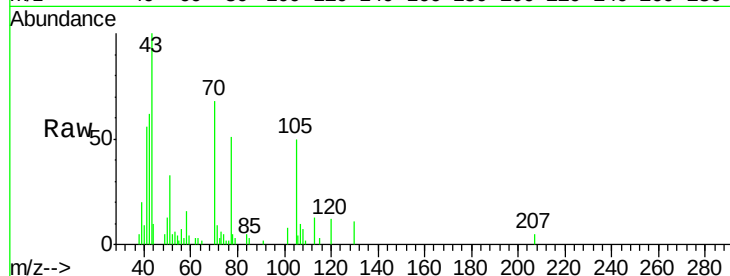

#16

4-Methylphenol

Concen: 2.63 ng/ul




RT: 8.19 min Scan# 885


Delta R.T. 0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Tgt Ion:	108	Resp:	20943
Ion	Ratio	Lower	Upper
108	100		
107	101.5	86.4	129.6

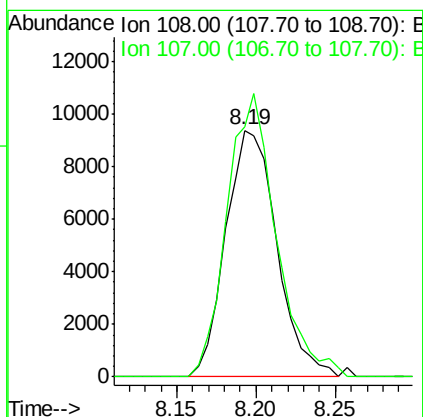



#17

Hexachloroethane

Concen: 2.98 ng/ul

RT: 8.46 min Scan# 931

Delta R.T. -0.01 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-06

Tgt Ion	Ratio	Lower	Upper
117	100		
201	86.8	76.6	115.0
199	49.5	49.1	73.7

Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM

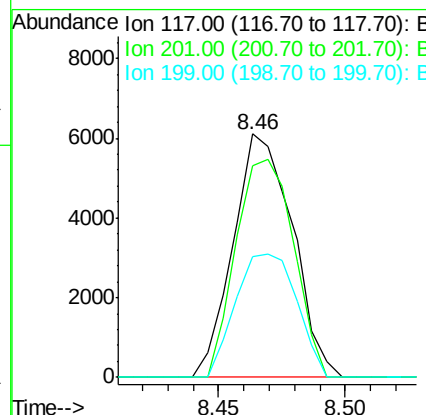

#20

Nitrobenzene

Concen: 2.89 ng/ul




RT: 8.60 min Scan# 955


Delta R.T. 0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Lower	Upper
77	100		
123	39.1	30.5	45.7
65	15.6	13.4	20.2

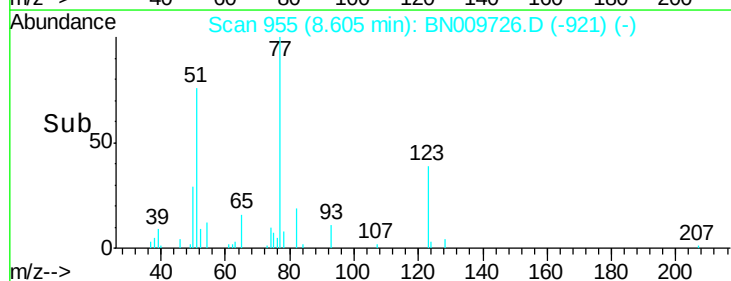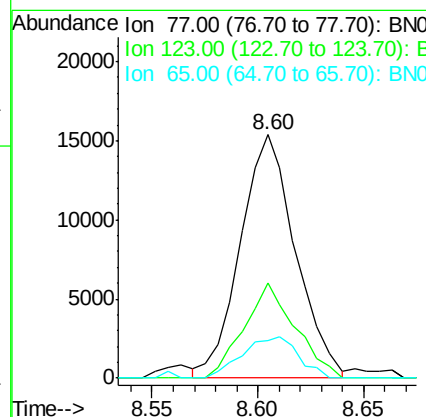



#21

Isophorone

Concen: 2.52 ng/ul

RT: 9.13 min Scan# 1044

Delta R.T. 0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-06

Tgt Ion:	82	Resp:	42683
Ion Ratio	Lower	Upper	
82	100		
95	7.9	6.0	9.0
138	18.1	12.6	19.0

Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM

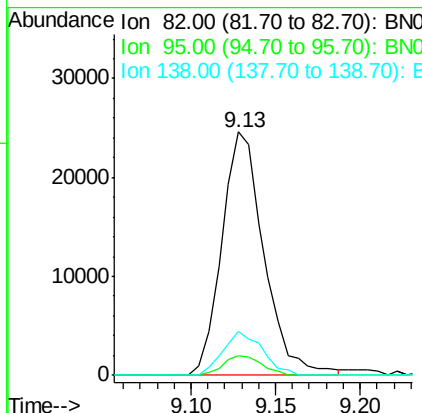

#23

2-Nitrophenol

Concen: 2.73 ng/ul




RT: 9.30 min Scan# 1074


Delta R.T. -0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Tgt Ion:	139	Resp:	10939
Ion Ratio	Lower	Upper	
139	100		
65	94.9	58.0	87.0#
109	31.2	28.8	43.2









#24
 2,4-Dimethylphenol
 Concen: 2.71 ng/ul
 RT: 9.38 min Scan# 1087
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-06

Tgt Ion	Ratio	Resp	Lower	Upper
107	100	23557		
121	40.5	38.5	57.7	
122	82.3	62.9	94.3	




Manual Integrations
 APPROVED


mohammad
 2/17/2020 3:50:13 PM

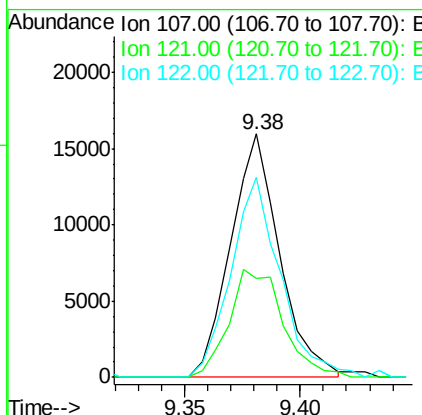

#25
 Bis(2-Chloroethoxy)methane
 Concen: 2.74 ng/ul
 RT: 9.62 min Scan# 1127
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Resp	Lower	Upper
93	100	28437		
95	29.5	25.1	37.7	
123	10.8	8.9	13.3	



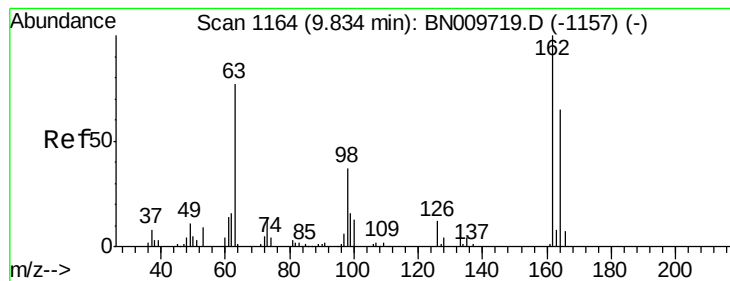





#27
 2,4-Dichlorophenol
 Concen: 2.72 ng/ul
 RT: 9.83 min Scan# 1164
 Delta R.T. 0.00 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-06

Tgt Ion	Ratio	Resp	Lower	Upper
162	100	18893		
164	82.5	50.5	75.7#	
98	51.8	28.7	43.1#	




Manual Integrations
 APPROVED


mohammad
 2/17/2020 3:50:13 PM

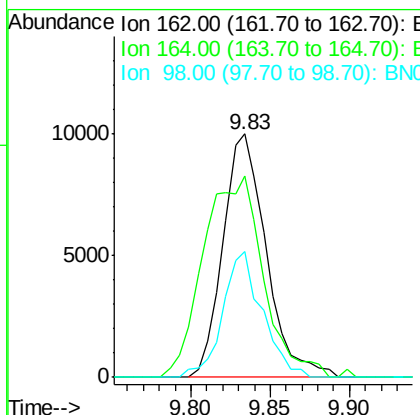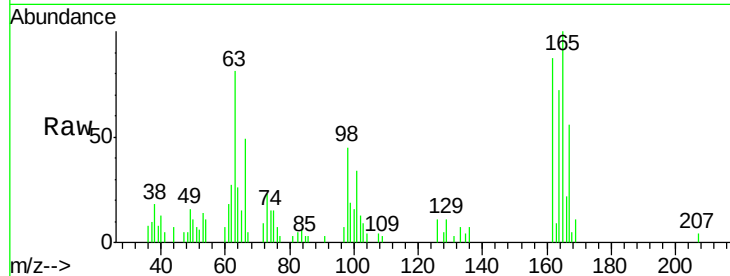

#28
 Naphthalene
 Concen: 2.88 ng/ul
 RT: 10.22 min Scan# 1229
 Delta R.T. -0.00 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Resp	Lower	Upper
128	100	69485		
129	10.2	8.6	13.0	
127	11.7	10.3	15.5	

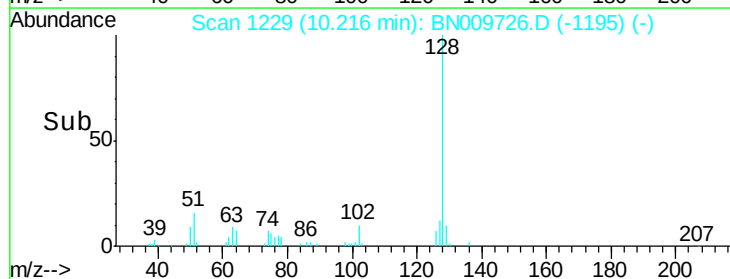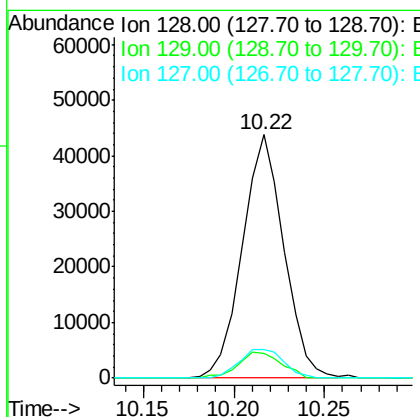







#30
4-Chloroaniline
Concen: 2.87 ng/ul
RT: 10.35 min Scan# 1251
Delta R.T. 0.00 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-06

Tgt Ion:127 Resp: 22745
Ion Ratio Lower Upper
127 100
129 33.8 24.8 37.2




Manual Integrations
APPROVED


mohammad
2/17/2020 3:50:13 PM



#31
Hexachlorobutadiene
Concen: 2.83 ng/ul
RT: 10.50 min Scan# 1278
Delta R.T. 0.00 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Tgt Ion:225 Resp: 13119
Ion Ratio Lower Upper
225 100
223 73.3 47.0 70.4#
227 67.9 57.3 85.9

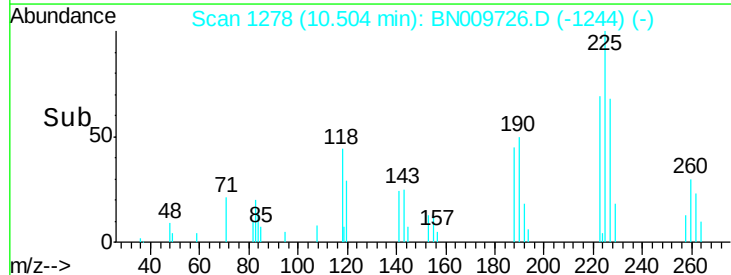







#32
 Caprolactam
 Concen: 1.67 ng/ul m
 RT: 11.18 min Scan# 1393
 Delta R.T. 0.05 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-06

Tgt Ion	Ratio	Lower	Upper
113	100		
55	268.5	209.1	313.7
56	153.4	161.6	242.4#




Manual Integrations
 APPROVED


mohammad
 2/17/2020 3:50:13 PM

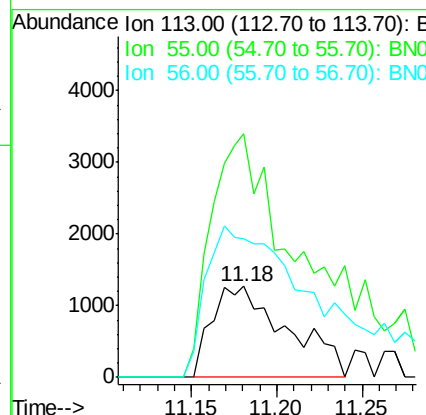

#33
 4-Chloro-3-methylphenol
 Concen: 2.27 ng/ul
 RT: 11.49 min Scan# 1445
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Lower	Upper
107	100		
144	27.0	19.3	28.9
142	69.3	59.5	89.3

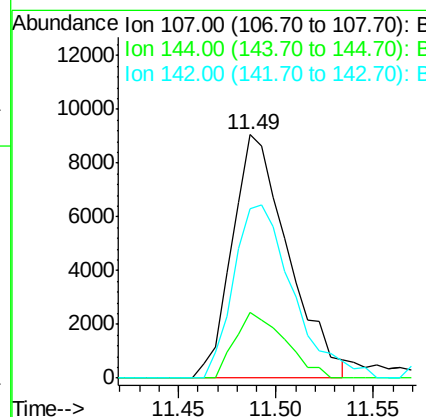

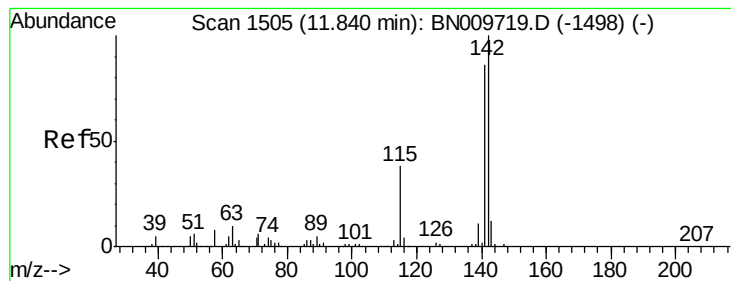

#34

2-Methylnaphthalene

Concen: 2.79 ng/uL

RT: 11.85 min Scan# 1506

Delta R.T. 0.01 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-06

Tgt Ion:142 Resp: 46758

Ion Ratio Lower Upper

142 100


141 86.6 72.1 108.1

Manual Integrations

APPROVED




mohammad

2/17/2020 3:50:13 PM



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

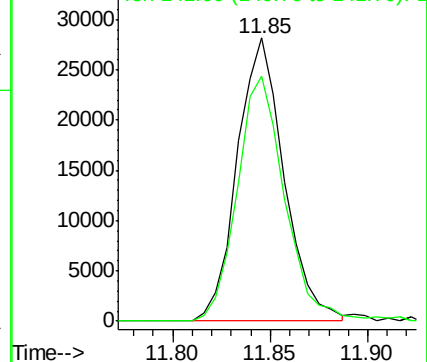

#35

1-Methylnaphthalene

Concen: 2.90 ng/uL

RT: 12.06 min Scan# 1543

Delta R.T. 0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25


Tgt Ion:142 Resp: 48640

Ion Ratio Lower Upper

142 100

141 93.3 72.8 109.2



116 3.2 3.2 4.8




Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

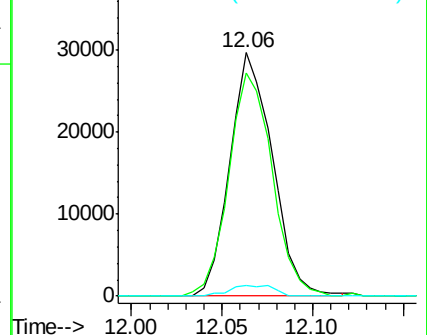







#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 2.91 ng/ul
 RT: 12.23 min Scan# 1571
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-06

Tgt Ion	Ratio	Resp	Lower	Upper
216	100	24695		
214	73.0		64.8	97.2
179	25.5		17.6	26.4
108	20.0		16.3	24.5




Manual Integrations
 APPROVED


mohammad
 2/17/2020 3:50:13 PM

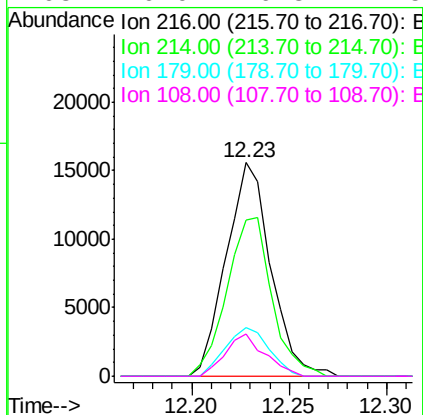

#38
 Hexachlorocyclopentadiene
 Concen: 0.85 ng/ul
 RT: 12.19 min Scan# 1565
 Delta R.T. -0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Resp	Lower	Upper
237	100	3117		
235	41.9		48.3	72.5#
272	0.0		9.6	14.4#

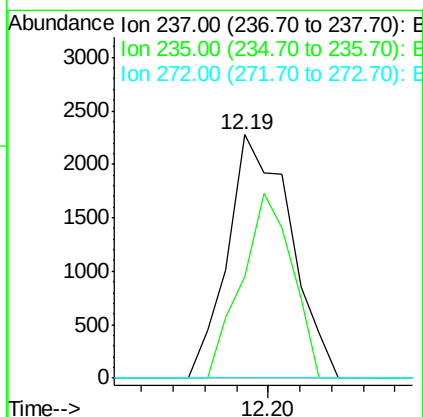







#39
 2,4,6-Trichlorophenol
 Concen: 2.04 ng/ul
 RT: 12.49 min Scan# 1615
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleID :
 MDL-WATER-06

Tgt Ion	Ratio	Resp	Lower	Upper
196	100	10975		
198	96.1	77.2	115.8	
200	34.4	26.8	40.2	




Manual Integrations
 APPROVED


mohammad
 2/17/2020 3:50:13 PM

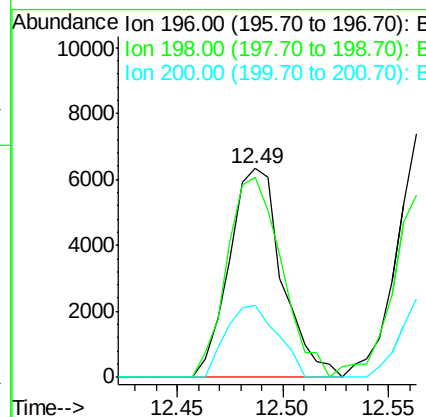

#40
 2,4,5-Trichlorophenol
 Concen: 2.48 ng/ul m
 RT: 12.56 min Scan# 1628
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Resp	Lower	Upper
196	100	14311		
198	74.7	75.0	112.6#	
200	32.1	24.2	36.4	

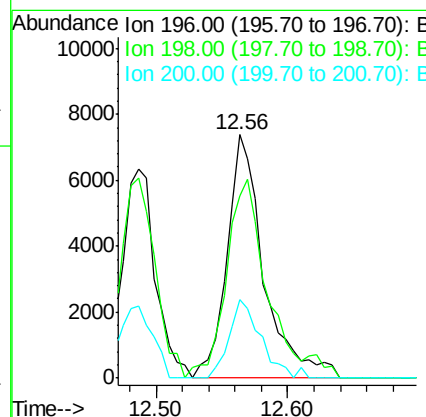







#41
 1,1'-Biphenyl
 Concen: 2.84 ng/ul
 RT: 12.88 min Scan# 1682
 Delta R.T. -0.00 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-06

Tgt Ion	Ratio	Lower	Upper
154	100		
153	39.0	33.2	49.8
76	12.4	11.0	16.4




Manual Integrations
 APPROVED


mohammad
 2/17/2020 3:50:13 PM

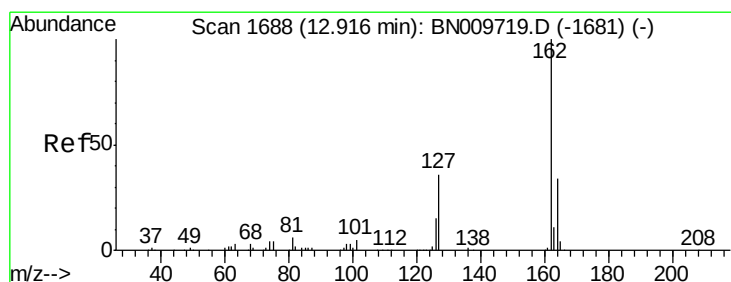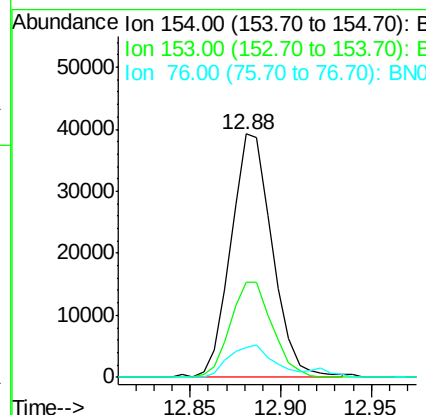

#42
 2-Chloronaphthalene
 Concen: 2.71 ng/ul
 RT: 12.92 min Scan# 1689
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Lower	Upper
162	100		
164	34.6	25.7	38.5
127	42.6	31.4	47.2

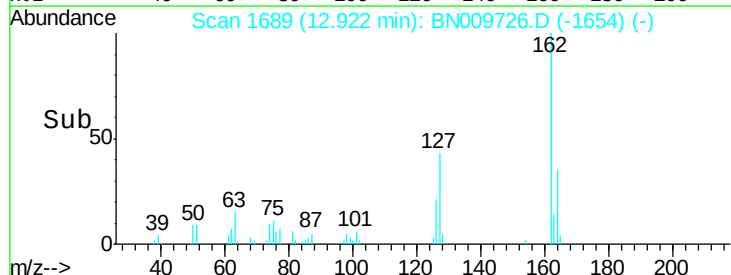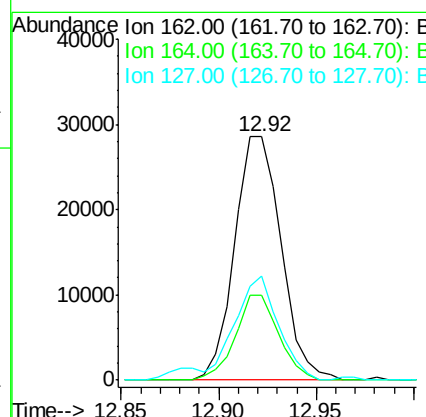







#43
2-Nitroaniline
Concen: 2.20 ng/ul
RT: 13.15 min Scan# 1728
Delta R.T. 0.01 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-06

Tgt Ion	Ratio	Lower	Upper
65	100		
92	46.3	43.6	65.4
138	68.0	61.3	91.9




Manual Integrations
APPROVED


mohammad
2/17/2020 3:50:13 PM

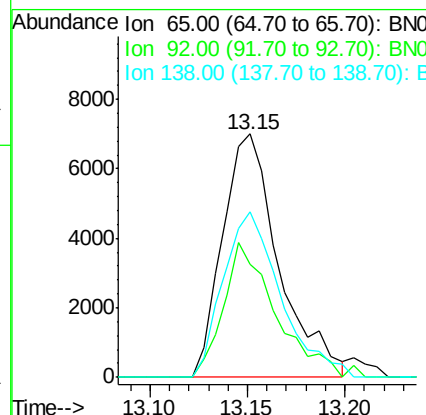

#45
Dimethylphthalate
Concen: 2.93 ng/ul
RT: 13.53 min Scan# 1793
Delta R.T. 0.01 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.7	3.4	5.0
164	10.3	8.0	12.0

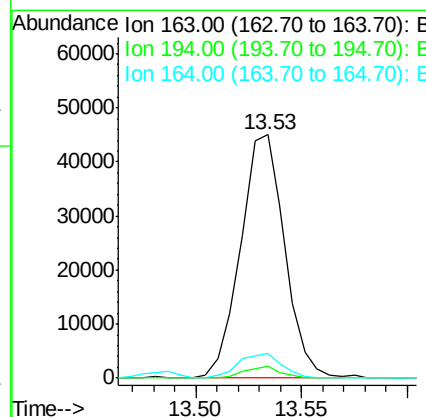



#46

2,6-Dinitrotoluene

Concen: 2.22 ng/ul

RT: 13.66 min Scan# 1814

Delta R.T. 0.01 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-06

Tgt Ion:	165	Resp:	9675
Ion Ratio	Lower	Upper	
165	100		
89	84.4	54.1	81.1#
121	26.9	18.1	27.1

Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM



#48

Acenaphthylene

Concen: 2.85 ng/ul




RT: 13.77 min Scan# 1834


Delta R.T. 0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Tgt Ion:	152	Resp:	77577
Ion Ratio	Lower	Upper	
152	100		
151	18.1	15.7	23.5
153	13.1	10.3	15.5









#49
3-Nitroaniline
Concen: 2.19 ng/ul
RT: 14.00 min Scan# 1872
Delta R.T. 0.02 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-06

Tgt Ion:138 Resp: 8833
Ion Ratio Lower Upper
138 100
108 18.4 8.9 13.3#
92 113.6 99.2 148.8




Manual Integrations
APPROVED




mohammad
2/17/2020 3:50:13 PM



#50
Acenaphthene
Concen: 2.86 ng/ul
RT: 14.12 min Scan# 1893
Delta R.T. 0.00 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Tgt Ion:153 Resp: 53397
Ion Ratio Lower Upper
153 100
152 46.5 36.6 54.8
154 88.0 70.6 106.0



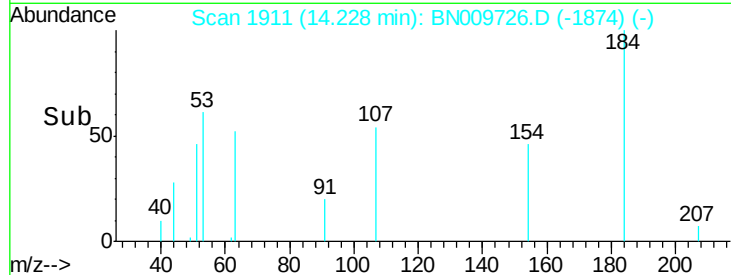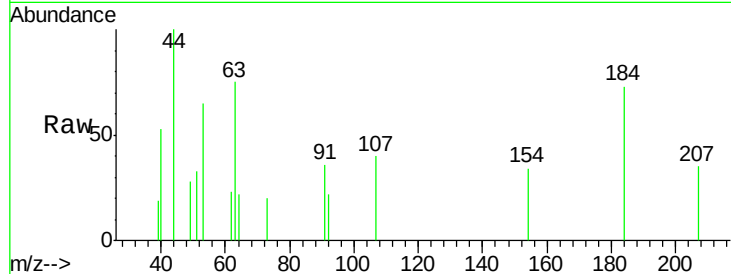





#51
2,4-Dinitrophenol
Concen: 0.86 ng/ul
RT: 14.23 min Scan# 1911
Delta R.T. 0.02 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Resp	Lower	Upper
184	100	2145		
63	102.9	83.0	124.6	
154	46.3	54.9	82.3	

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-06


Manual Integrations
APPROVED


mohammad
2/17/2020 3:50:13 PM



#53
4-Nitrophenol
Concen: 2.60 ng/ul
RT: 14.31 min Scan# 1925
Delta R.T. 0.00 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Resp	Lower	Upper
109	100	9138		
139	106.2	96.3	144.5	
65	171.3	129.9	194.9	





#54

Dibenzenofuran

Concen: 2.88 ng/ul

RT: 14.46 min Scan# 1951

Delta R.T. 0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-06

Tgt Ion:168 Resp: 75369

Ion Ratio Lower Upper

168 100





139 37.7 32.7 49.1

Manual Integrations

APPROVED

mohammad

2/17/2020 3:50:13 PM

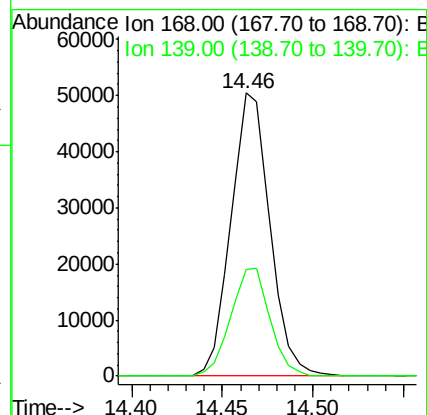

#55

2,4-Dinitrotoluene

Concen: 2.45 ng/ul

RT: 14.46 min Scan# 1951

Delta R.T. 0.01 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25




Tgt Ion:165 Resp: 15877


Ion Ratio Lower Upper

165 100

63 84.8 68.3 102.5

182 3.7 2.2 3.4#

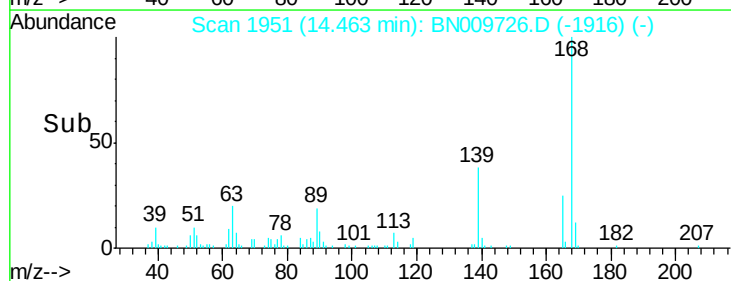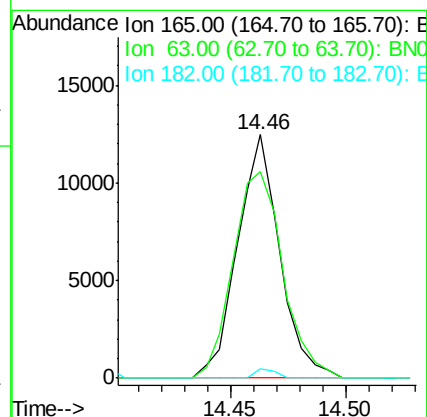




#56
 2,3,4,6-Tetrachlorophenol
 Concen: 2.38 ng/ul
 RT: 14.70 min Scan# 1992
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-06




Tgt Ion:	232	Resp:	11802
Ion Ratio	Lower	Upper	
232	100		
131	60.0	40.6	60.8
130	0.0	2.2	3.4
166	33.4	26.6	39.8

Manual Integrations
 APPROVED

mohammad
 2/17/2020 3:50:13 PM

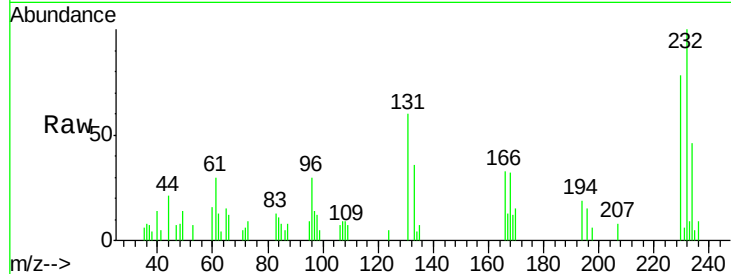


Abundance Ion 232.00 (231.70 to 232.70): E
 Ion 131.00 (130.70 to 131.70): E
 Ion 130.00 (129.70 to 130.70): E
 Ion 166.00 (165.70 to 166.70): E


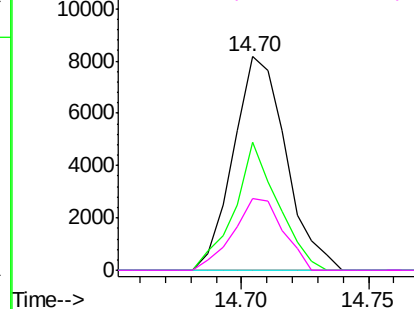



#57
 Diethylphthalate
 Concen: 2.68 ng/ul
 RT: 14.92 min Scan# 2028
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion:	149	Resp:	61445
Ion Ratio	Lower	Upper	
149	100		
177	23.4	17.8	26.6
150	14.0	9.8	14.6



Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 177.00 (176.70 to 177.70): E
 Ion 150.00 (149.70 to 150.70): E

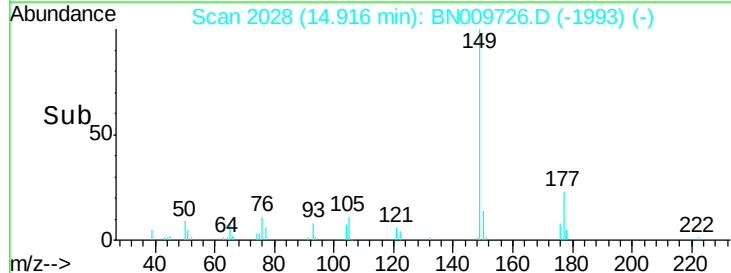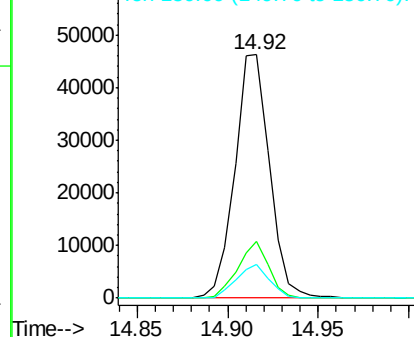

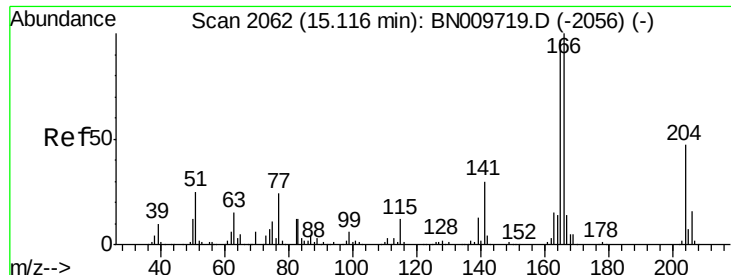





#59
Fluorene
Concen: 2.82 ng/ul
RT: 15.12 min Scan# 2063
Delta R.T. 0.01 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-06

Tgt Ion	Ratio	Lower	Upper
166	100		
165	96.1	79.8	119.8
167	11.6	10.7	16.1




Manual Integrations
APPROVED


mohammad
2/17/2020 3:50:13 PM

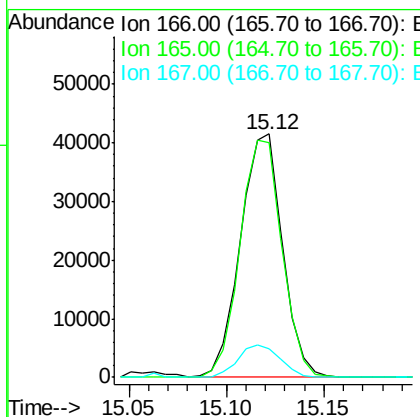

#60
4-Chlorophenyl-phenylether
Concen: 2.88 ng/ul
RT: 15.12 min Scan# 2063
Delta R.T. 0.00 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25


Tgt Ion	Ratio	Lower	Upper
204	100		
206	32.9	26.5	39.7
141	56.9	48.8	73.2

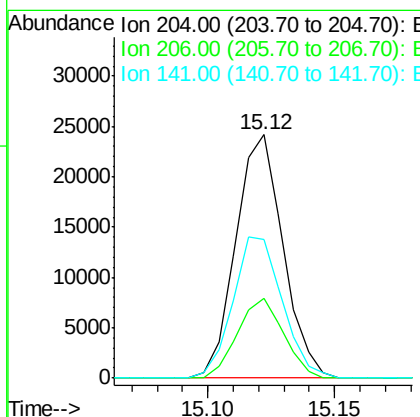



#61
4-Nitroaniline
Concen: 1.50 ng/ul
RT: 15.17 min Scan# 2071
Delta R.T. 0.02 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25




Instrument :
BNA_N
ClientSampleId :
MDL-WATER-06



Tgt Ion:138 Resp: 7384
Ion Ratio Lower Upper
138 100
92 54.5 47.8 71.6
108 78.3 72.3 108.5




Manual Integrations
APPROVED


mohammad
2/17/2020 3:50:13 PM

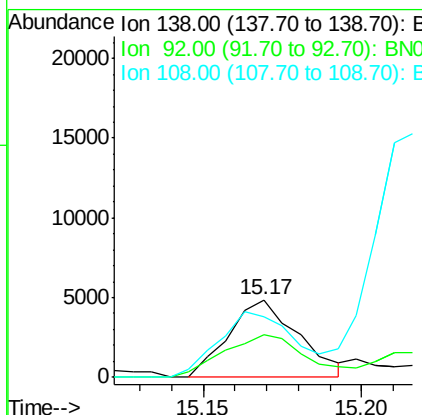

#64
4,6-Dinitro-2-methylphenol
Concen: 2.44 ng/ul
RT: 15.23 min Scan# 2082
Delta R.T. 0.01 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Tgt Ion:198 Resp: 10002
Ion Ratio Lower Upper
198 100
182 9.0 3.7 5.5#
77 46.0 25.1 37.7#





#65

N-Nitrosodiphenylamine

Concen: 2.71 ng/ul

RT: 15.34 min Scan# 2100

Delta R.T. 0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-06

Tgt Ion:	169	Resp:	49318
Ion Ratio	Lower	Upper	
169	100		
168	70.0	51.8	77.6
167	36.9	27.7	41.5

Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM

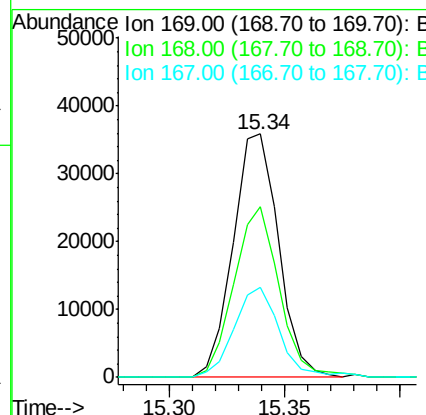

#66

4-Bromophenyl-phenylether

Concen: 2.75 ng/ul




RT: 16.02 min Scan# 2215


Delta R.T. 0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Tgt Ion:	248	Resp:	16864
Ion Ratio	Lower	Upper	
248	100		
250	98.6	81.4	122.0
141	84.0	66.9	100.3

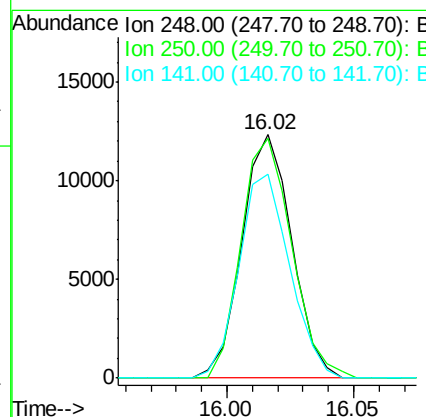



#67

Hexachlorobenzene

Concen: 2.74 ng/ul

RT: 16.13 min Scan# 2234

Delta R.T. 0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Instrument :

BNA_N


ClientSampled :

MDL-WATER-06




Tgt Ion:	284	Resp:	18647
Ion Ratio	Lower	Upper	
284	100		
142	42.4	34.4	51.6
249	40.5	29.7	44.5

Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM

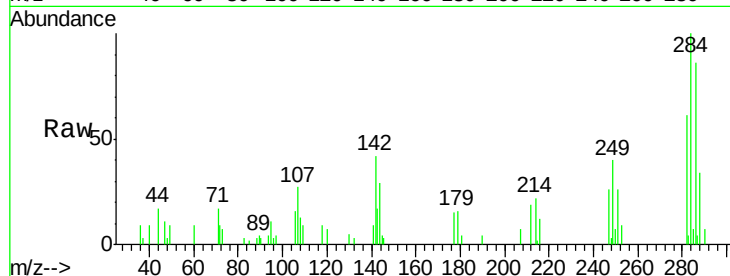

Abundance Ion 284.00 (283.70 to 284.70): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E

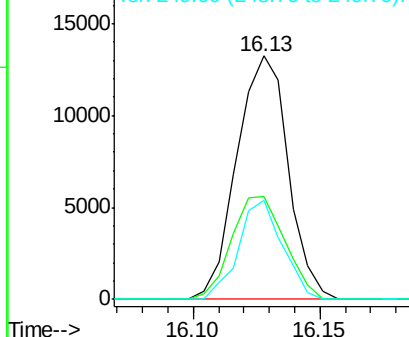

#68

Atrazine

Concen: 2.32 ng/ul


RT: 16.31 min Scan# 2265

Delta R.T. 0.01 min



Lab File: BN009726.D


Acq: 14 Feb 2020 15:25

Tgt Ion:	200	Resp:	16020
Ion Ratio	Lower	Upper	
200	100		
173	25.4	22.1	33.1
215	43.4	41.6	62.4



Abundance Ion 200.00 (199.70 to 200.70): E
Ion 173.00 (172.70 to 173.70): E
Ion 215.00 (214.70 to 215.70): E

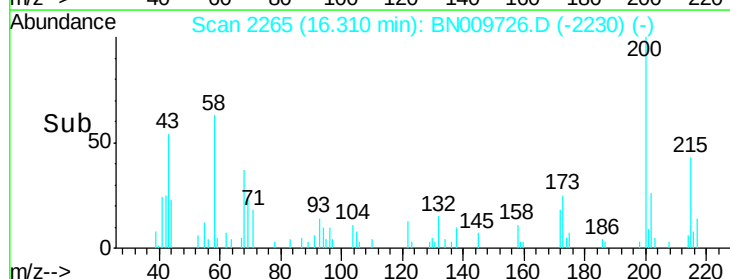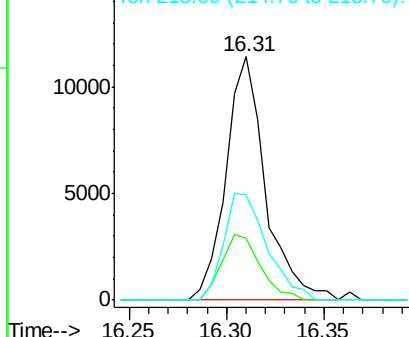




#69
 Pentachlorophenol
 Concen: 1.54 ng/ul
 RT: 16.49 min Scan# 2296
 Delta R.T. 0.02 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-06




Tgt Ion	Ratio	Resp	Lower	Upper
266	100	6049		
264	49.6	52.9	79.3#	
268	46.7	52.5	78.7#	

Manual Integrations
 APPROVED

mohammad
 2/17/2020 3:50:13 PM




Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E


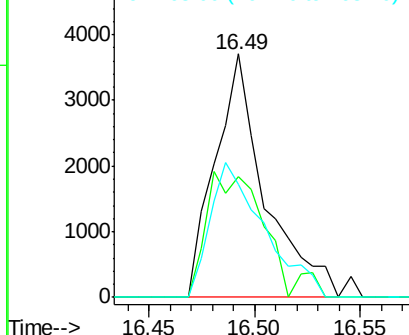



#70
 Phenanthrene
 Concen: 2.86 ng/ul
 RT: 16.86 min Scan# 2358
 Delta R.T. 0.00 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	100162		
179	14.4	12.5	18.7	
176	17.7	14.6	22.0	



Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 176.00 (175.70 to 176.70): E

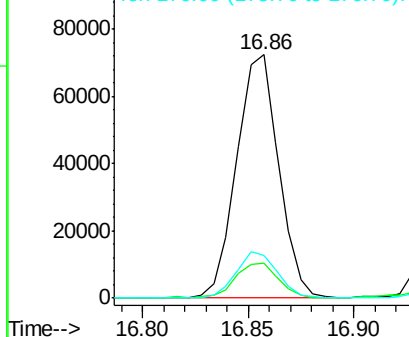



#72

Anthracene

Concen: 2.86 ng/uL

RT: 16.95 min Scan# 2373

Delta R.T. 0.00 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-06

Tgt Ion:	178	Resp:	102444
Ion Ratio	Lower	Upper	
178	100		
179	14.7	12.2	18.2
176	17.6	14.6	21.8

Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM

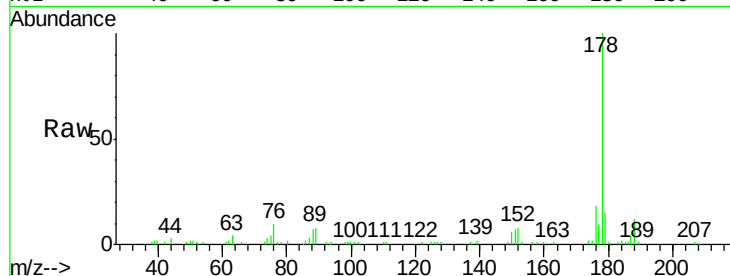

#73

1,2,3,4-Tetrachlorobenzene

Concen: 3.05 ng/uL




RT: 12.85 min Scan# 1676


Delta R.T. 0.01 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Tgt Ion:	216	Resp:	27331
Ion Ratio	Lower	Upper	
216	100		
214	80.0	66.8	100.2
218	44.9	39.1	58.7









#74
 Pentachlorobenzene
 Concen: 2.74 ng/uL
 RT: 14.39 min Scan# 1938
 Delta R.T. 0.00 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-06

Tgt Ion	Ratio	Resp	Lower	Upper
250	100	23735		
248	65.5	49.4	74.0	
252	61.4	51.8	77.6	




Manual Integrations
 APPROVED


mohammad
 2/17/2020 3:50:13 PM



#75
 Carbazole
 Concen: 2.30 ng/uL
 RT: 17.23 min Scan# 2422
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Resp	Lower	Upper
167	100	72674		
166	21.6	16.6	24.8	
139	11.4	9.9	14.9	





#76

Di-n-butylphthalate

Concen: 2.22 ng/ul

RT: 17.81 min Scan# 2520

Delta R.T. 0.01 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-06

Tgt Ion:	149	Resp:	86413
Ion Ratio	Lower	Upper	
149	100		
150	9.0	7.0	10.6
104	5.7	4.3	6.5

Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM



#77

Fluoranthene

Concen: 2.55 ng/ul




RT: 18.89 min Scan# 2703


Delta R.T. 0.01 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Tgt Ion:	202	Resp:	104533
Ion Ratio	Lower	Upper	
202	100		
101	11.3	9.4	14.2
100	9.3	7.2	10.8









#80
 Pyrene
 Concen: 2.76 ng/ul
 RT: 19.25 min Scan# 2765
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-06

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	13.4	11.3	16.9
100	11.6	9.0	13.6




Manual Integrations
 APPROVED


mohammad
 2/17/2020 3:50:13 PM

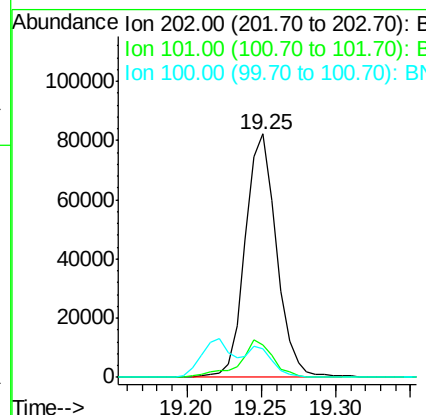

#81
 Butylbenzylphthalate
 Concen: 1.97 ng/ul
 RT: 20.18 min Scan# 2923
 Delta R.T. -0.00 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Resp Lower	Resp Upper
149	100		
91	84.4	65.5	98.3
206	22.0	15.9	23.9

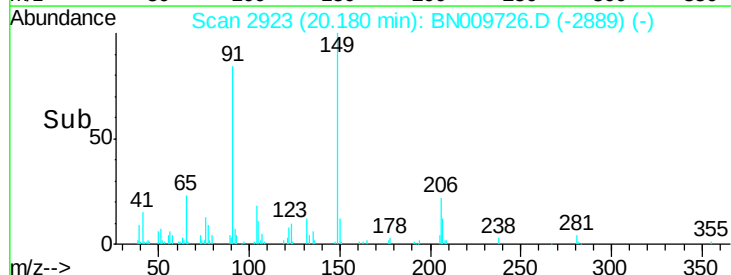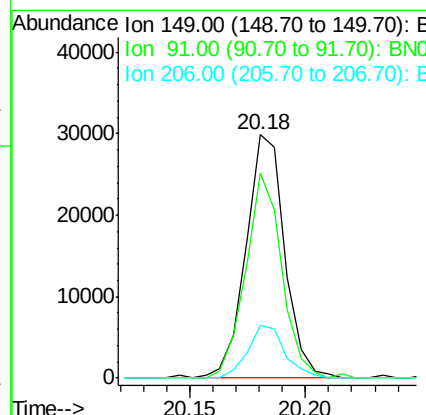







#82
 3,3'-Dichlorobenzidine
 Concen: 2.23 ng/ul
 RT: 20.96 min Scan# 3055
 Delta R.T. 0.00 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-06

Tgt Ion	Ratio	Lower	Upper
252	100		
254	67.7	49.3	73.9
126	13.7	8.8	13.2




Manual Integrations
 APPROVED


mohammad
 2/17/2020 3:50:13 PM

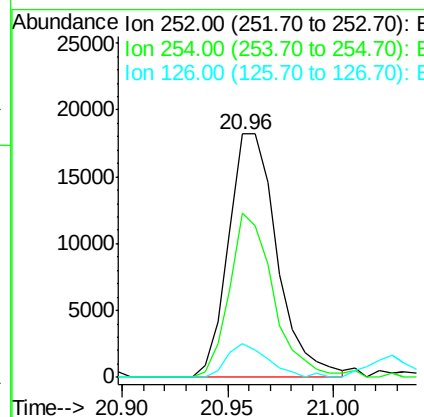

#83
 Benzo(a)anthracene
 Concen: 2.61 ng/ul
 RT: 21.02 min Scan# 3065
 Delta R.T. -0.00 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Lower	Upper
228	100		
229	19.9	15.0	22.4
226	25.7	21.4	32.2

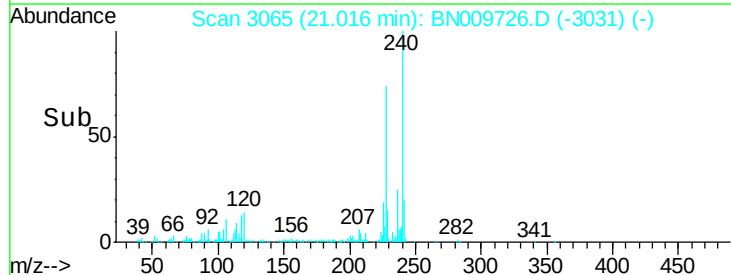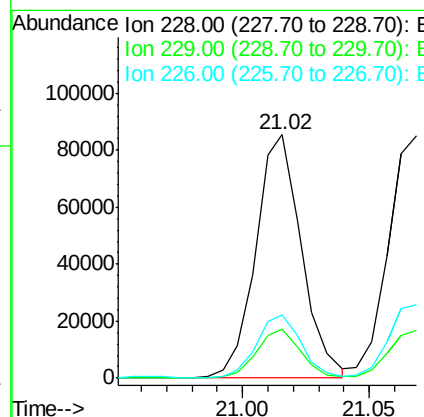







#84
 Bis(2-ethylhexyl)phthalate
 Concen: 2.03 ng/ul
 RT: 20.97 min Scan# 3058
 Delta R.T. 0.00 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-06

Tgt Ion	Ratio	Resp	Lower	Upper
149	100	54998		
167	25.2		21.0	31.6
279	3.5		3.0	4.6




Manual Integrations
 APPROVED


mohammad
 2/17/2020 3:50:13 PM

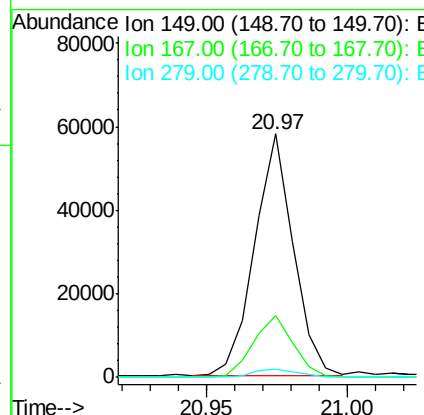

#85
 Chrysene
 Concen: 2.75 ng/ul
 RT: 21.07 min Scan# 3074
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	111800		
226	30.1		23.4	35.2
229	19.8		15.0	22.4

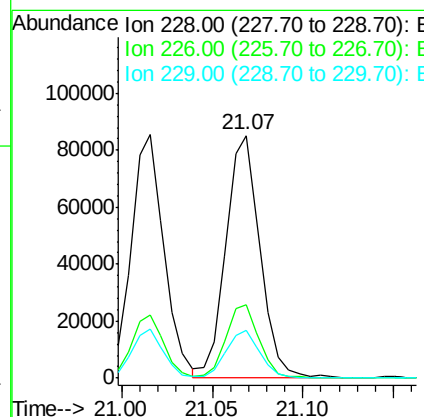







#87
Di-n-octyl phthalate
Concen: 1.97 ng/ul
RT: 21.82 min Scan# 3202
Delta R.T. 0.00 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-06

Tgt Ion:149 Resp: 88852




Manual Integrations
APPROVED


mohammad
2/17/2020 3:50:13 PM

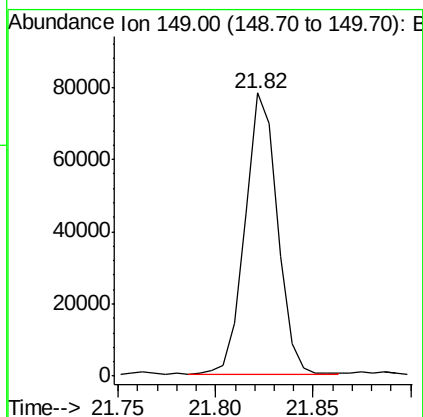

#88
Benzo(b)fluoranthene
Concen: 2.73 ng/ul m
RT: 22.52 min Scan# 3321
Delta R.T. -0.00 min
Lab File: BN009726.D
Acq: 14 Feb 2020 15:25

Tgt Ion:252 Resp: 105579
Ion Ratio Lower Upper
252 100
253 22.8 17.0 25.4
125 12.1 8.0 12.0#

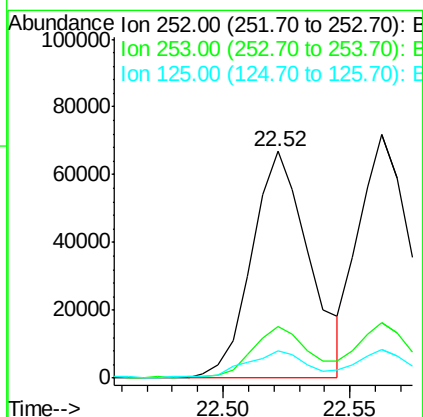



#89

Benzo(k)fluoranthene

Concen: 2.74 ng/ul

RT: 22.56 min Scan# 3328

Delta R.T. 0.01 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-06

Tgt Ion:	252	Resp:	100381
Ion Ratio	Lower	Upper	
252	100		
253	22.7	18.0	27.0
125	11.6	8.2	12.2

Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM

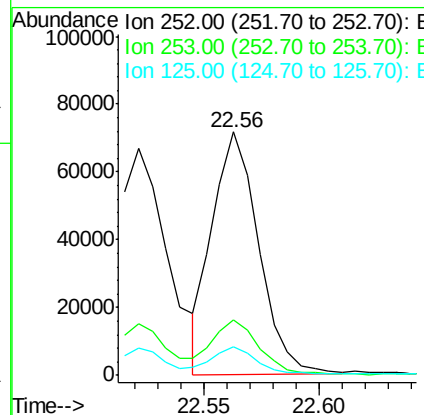

#91

Benzo(a)pyrene

Concen: 2.96 ng/ul




RT: 23.05 min Scan# 3411


Delta R.T. 0.01 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Tgt Ion:	252	Resp:	102908
Ion Ratio	Lower	Upper	
252	100		
253	21.7	17.4	26.0
125	12.1	9.0	13.6

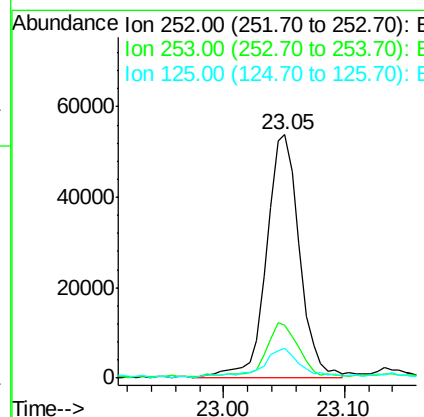







#92
 Indeno(1,2,3-cd)pyrene
 Concen: 2.64 ng/ul
 RT: 25.20 min Scan# 3777
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-06

Tgt Ion	Ratio	Resp Lower	Resp Upper
276	100		
138	23.3	20.9	31.3
277	23.5	18.2	27.4




Manual Integrations
 APPROVED




mohammad
 2/17/2020 3:50:13 PM

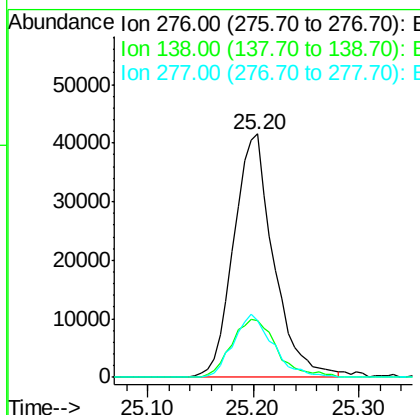

#93
 Dibenzo(a,h)anthracene
 Concen: 2.67 ng/ul
 RT: 25.20 min Scan# 3777
 Delta R.T. 0.01 min
 Lab File: BN009726.D
 Acq: 14 Feb 2020 15:25

Tgt Ion	Ratio	Resp Lower	Resp Upper
278	100		
139	17.5	13.0	19.4
279	23.3	17.5	26.3

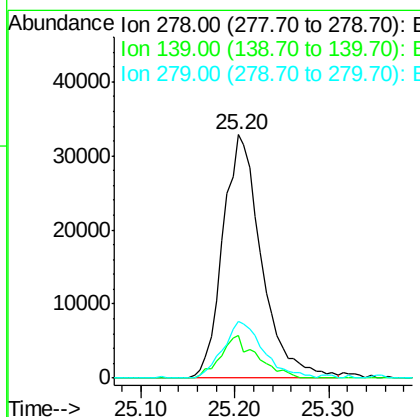



#94

Benzo(g,h,i)perylene

Concen: 2.70 ng/ul

RT: 25.83 min Scan# 3883

Delta R.T. 0.01 min

Lab File: BN009726.D

Acq: 14 Feb 2020 15:25

Tgt Ion:	276	Resp:	93275
Ion Ratio	Lower	Upper	
276	100		
138	23.6	17.5	26.3
277	25.1	18.1	27.1

Instrument :

BNA_N

ClientSampleId :

MDL-WATER-06

Manual Integrations
APPROVED

mohammad
2/17/2020 3:50:13 PM

