

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021723\
 Data File : BN024060.D
 Acq On : 17 Feb 2023 10:56
 Operator : CG/JU
 Sample : PB150872BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK872

Quant Time: Feb 17 21:35:21 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 14:45:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	6215	0.400	ng/ul	0.00
4) Naphthalene-d8	10.634	136	16828	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.484	164	9851	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.230	188	22293	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.424	240	18320	0.400	ng/ul	0.00
23) Perylene-d12	23.797	264	16605	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.231	96	34870	5.234	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	7091	0.269	ng/ul	0.00
18) Fluoranthene-d10	19.263	212	17757	0.361	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.479	166	2581	0.064	ng/ul#	14
20) Pyrene	19.630	202	2753	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.651	252	5695	0.093	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021723\
Data File : BN024060.D
Acq On : 17 Feb 2023 10:56
Operator : CG/JU
Sample : PB150872BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK872

Quant Time: Feb 17 21:35:21 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 14:45:13 2023
Response via : Initial Calibration




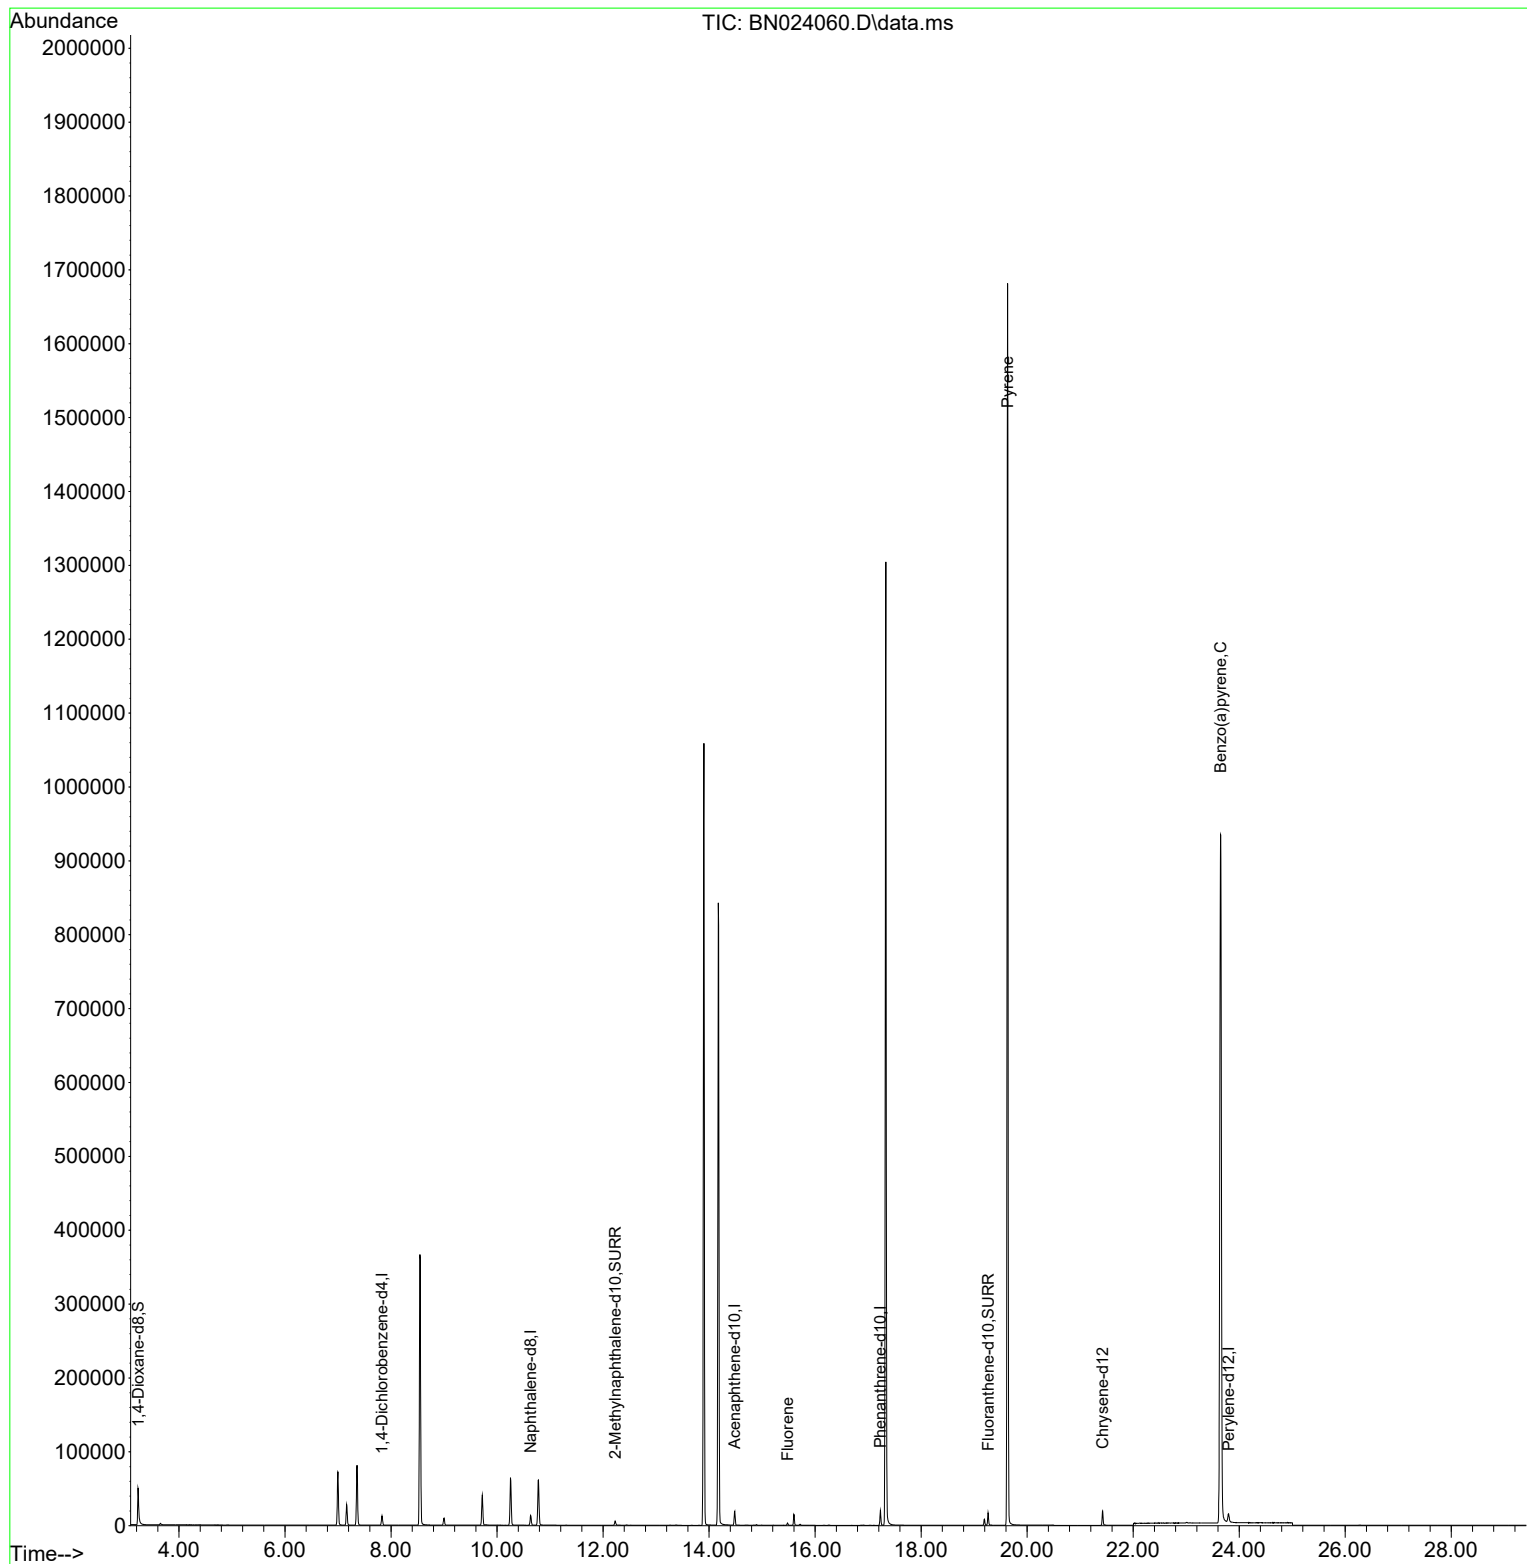


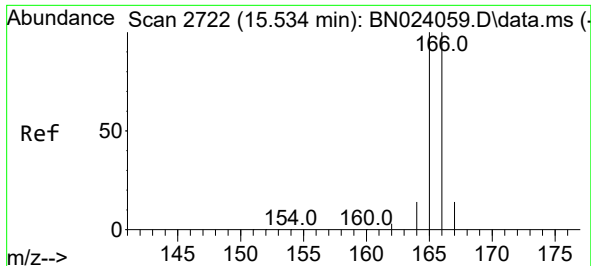

#12
Fluorene
Concen: 0.064 ng/ul
RT: 15.479 min Scan# 21
Delta R.T. -0.059 min
Lab File: BN024060.D
Acq: 17 Feb 2023 10:56




Instrument :
BNA_N
ClientSampleId :
SBLK872


Tgt Ion:166 Resp: 2581
Ion Ratio Lower Upper
166 100
165 6.8 77.4 116.2#
167 33.8 11.4 17.0#

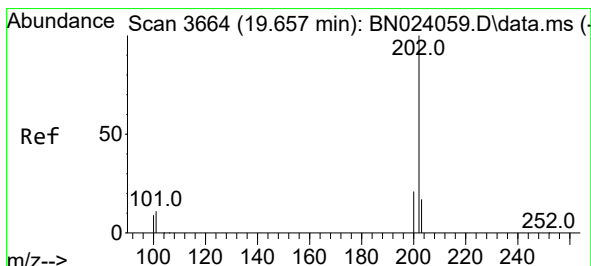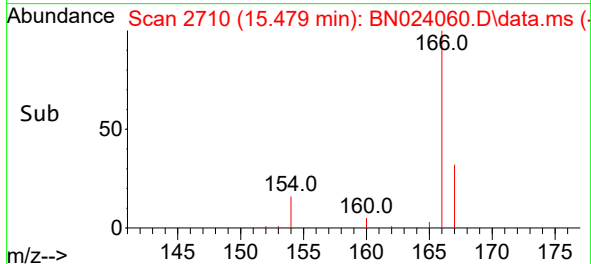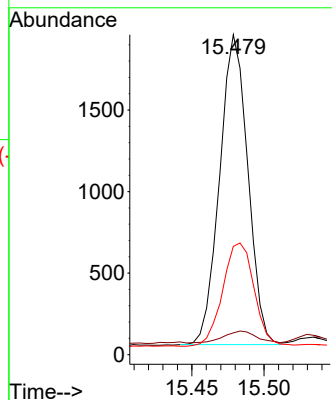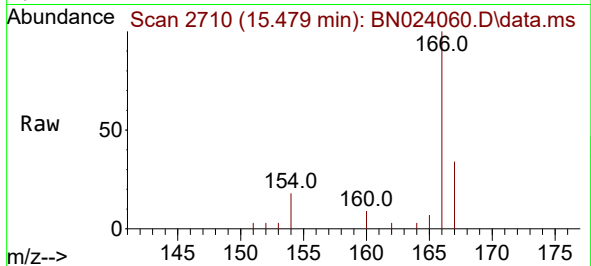

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.630 min Scan# 3658
Delta R.T. -0.032 min
Lab File: BN024060.D
Acq: 17 Feb 2023 10:56


Tgt Ion:202 Resp: 2753
Ion Ratio Lower Upper
202 100
101 166.5 8.1 12.1#
100 1301.0 6.2 9.4#

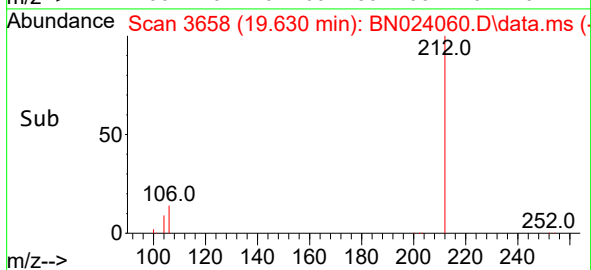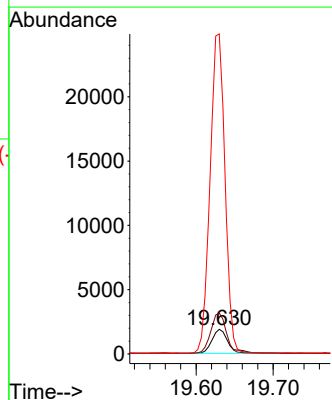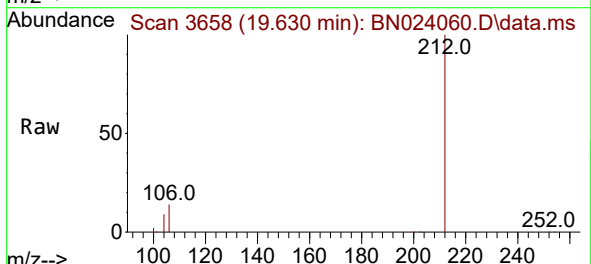

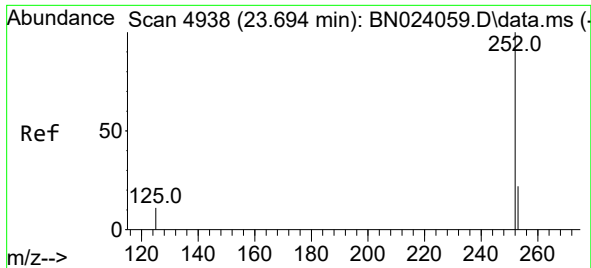

#26
Benzo(a)pyrene
Concen: 0.093 ng/ul
RT: 23.651 min Scan# 49
Delta R.T. -0.055 min
Lab File: BN024060.D
Acq: 17 Feb 2023 10:56

Instrument :
BNA_N
ClientSampleId :
SBLK872

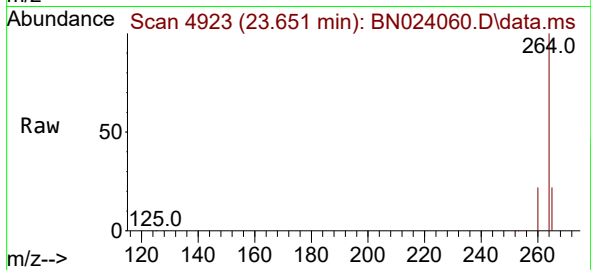

Tgt Ion:252 Resp: 5695
Ion Ratio Lower Upper
252 100
253 45.3 21.5 32.3#
125 33.2 11.2 16.8#

