

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021723\
 Data File : BN024061.D
 Acq On : 17 Feb 2023 11:33
 Operator : CG/JU
 Sample : PB150879BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK879

Quant Time: Feb 17 21:35:27 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 14:45:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	5291	0.400	ng/ul	0.00
4) Naphthalene-d8	10.634	136	14198	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.483	164	8153	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.234	188	17814	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.430	240	12981	0.400	ng/ul	0.00
23) Perylene-d12	23.819	264	10639	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.226	96	29230	5.154	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	5508	0.248	ng/ul	0.00
18) Fluoranthene-d10	19.262	212	12014	0.345	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.629	202	1876	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.658	252	3525	0.090	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021723\
Data File : BN024061.D
Acq On : 17 Feb 2023 11:33
Operator : CG/JU
Sample : PB150879BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK879

Quant Time: Feb 17 21:35:27 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 14:45:13 2023
Response via : Initial Calibration

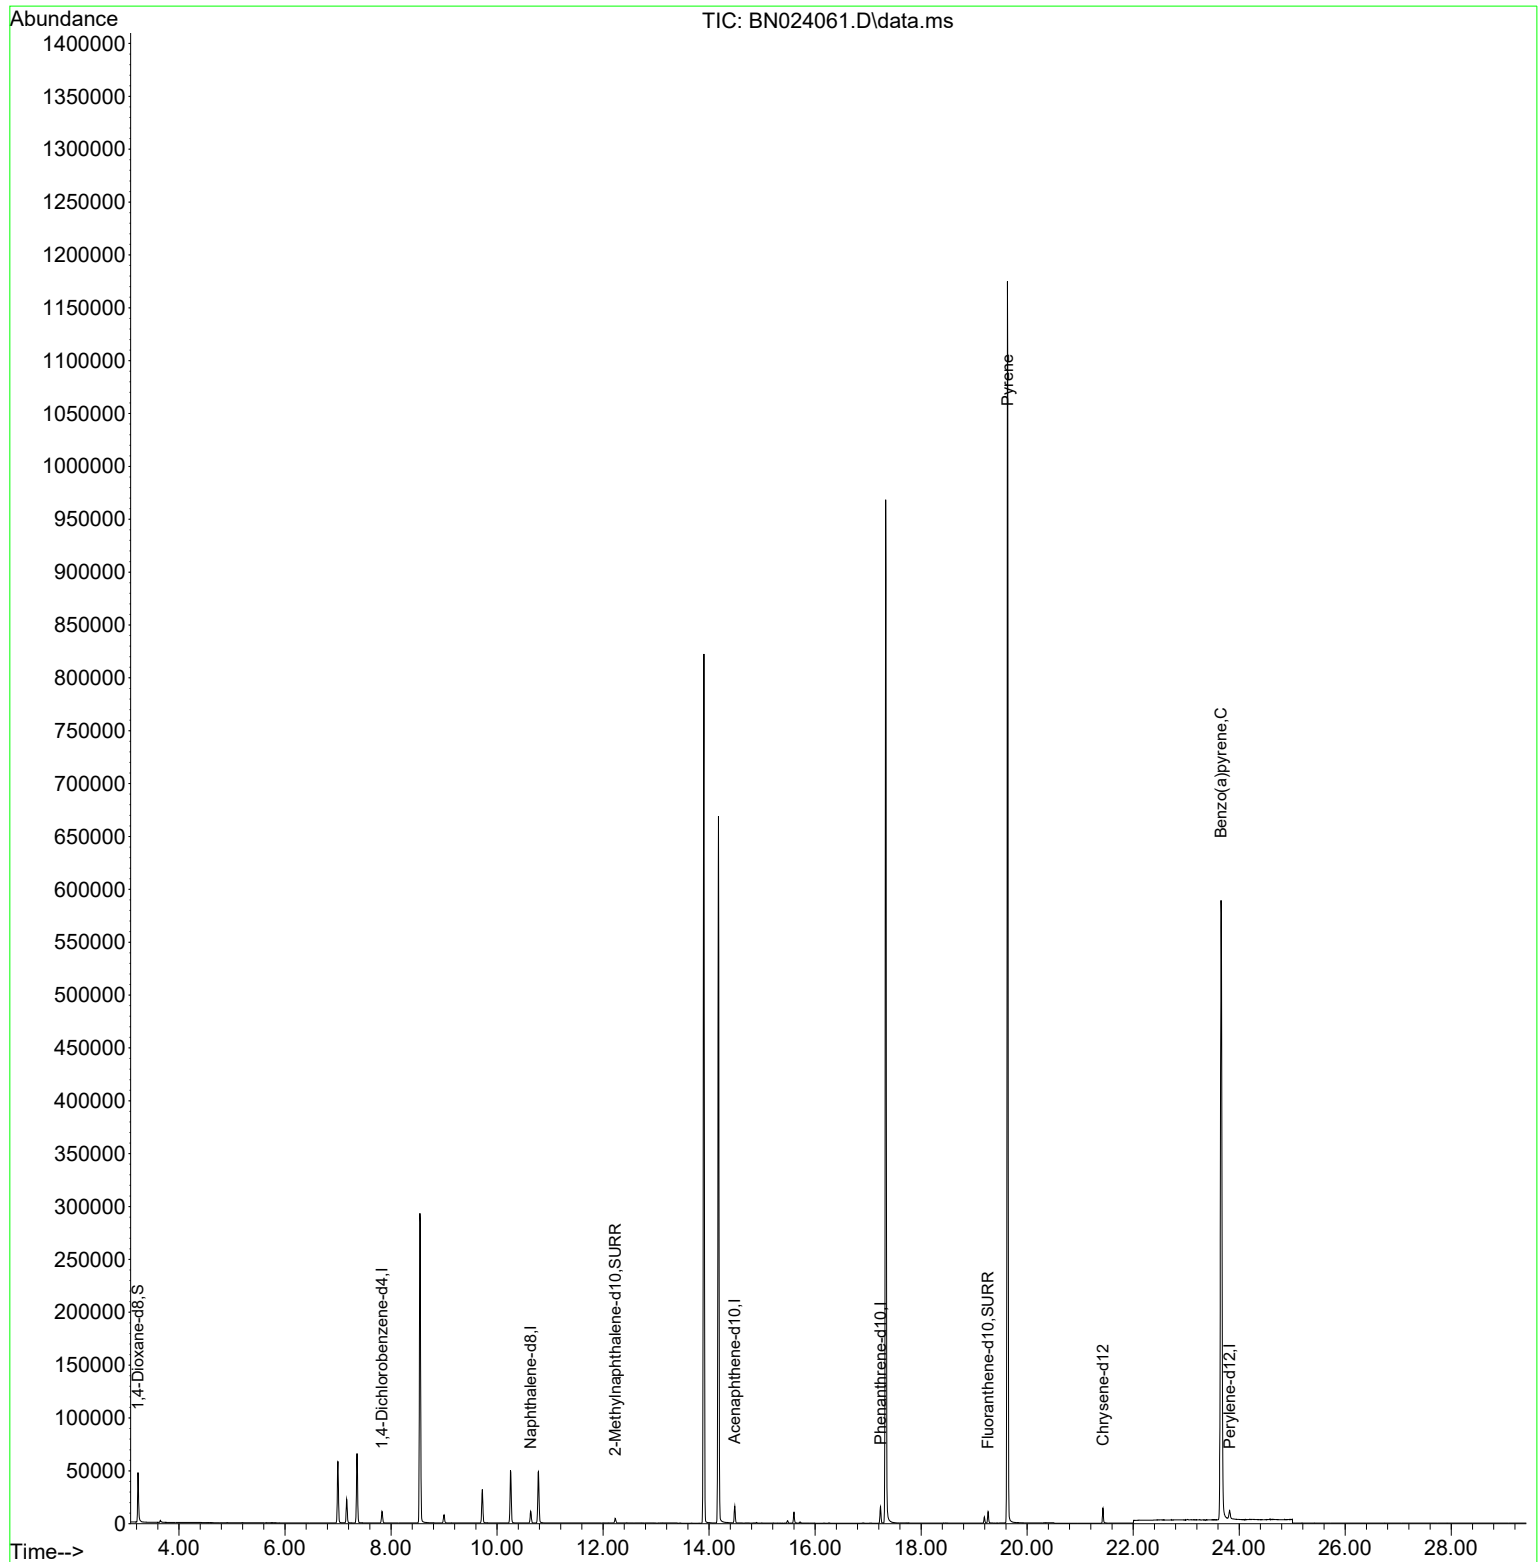

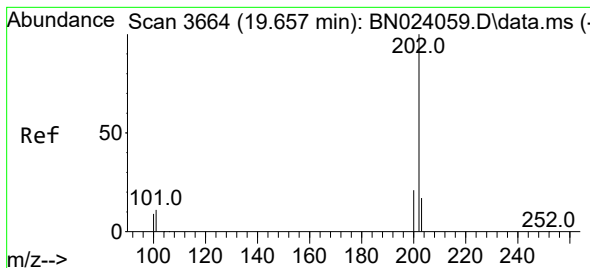

#20

Pyrene

Concen: 0.042 ng/ul

RT: 19.629 min Scan# 3

Delta R.T. -0.033 min

Lab File: BN024061.D

Acq: 17 Feb 2023 11:33

Instrument :

BNA_N

ClientSampleId :

SBLK879





Tgt Ion:202 Resp: 1876

Ion Ratio Lower Upper

202 100

101 165.9 8.1 12.1#

100 1288.6 6.2 9.4#

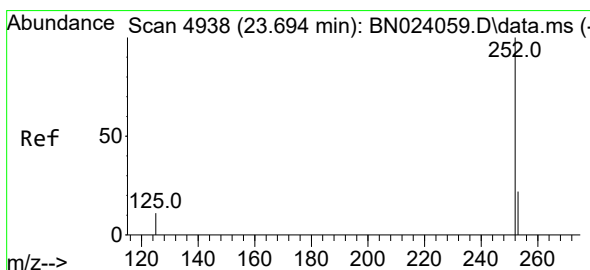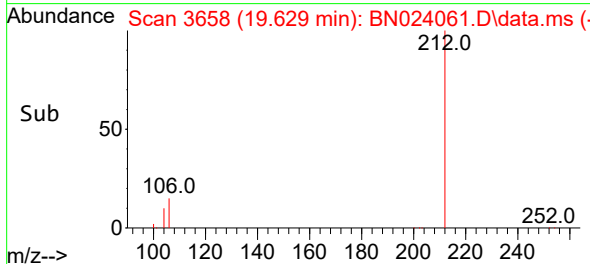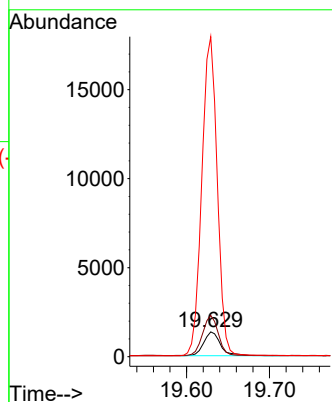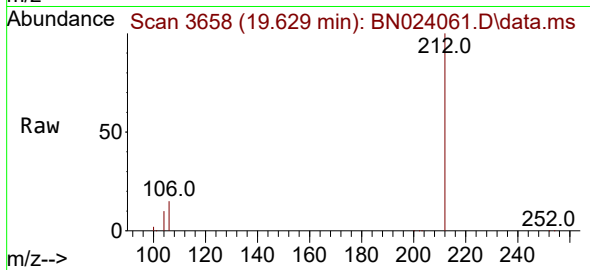

#26

Benzo(a)pyrene

Concen: 0.090 ng/ul

RT: 23.658 min Scan# 4925

Delta R.T. -0.048 min

Lab File: BN024061.D

Acq: 17 Feb 2023 11:33

Tgt Ion:252 Resp: 3525

Ion Ratio Lower Upper

252 100

253 49.8 21.5 32.3#

125 38.8 11.2 16.8#

