

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021723\
 Data File : BN024062.D
 Acq On : 17 Feb 2023 12:10
 Operator : CG/JU
 Sample : 01534-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B39

Quant Time: Feb 17 21:35:33 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 14:45:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.830	152	4914	0.400	ng/ul	0.00
4) Naphthalene-d8	10.634	136	13302	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.484	164	7671	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.235	188	17017	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.424	240	13412	0.400	ng/ul	# 0.00
23) Perylene-d12	23.794	264	10671	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.227	96	23274	4.418	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	4921	0.236	ng/ul	0.00
18) Fluoranthene-d10	19.263	212	11504	0.319	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.630	202	1833	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.645	252	3094	0.079	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021723\
Data File : BN024062.D
Acq On : 17 Feb 2023 12:10
Operator : CG/JU
Sample : 01534-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B39

Quant Time: Feb 17 21:35:33 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 14:45:13 2023
Response via : Initial Calibration

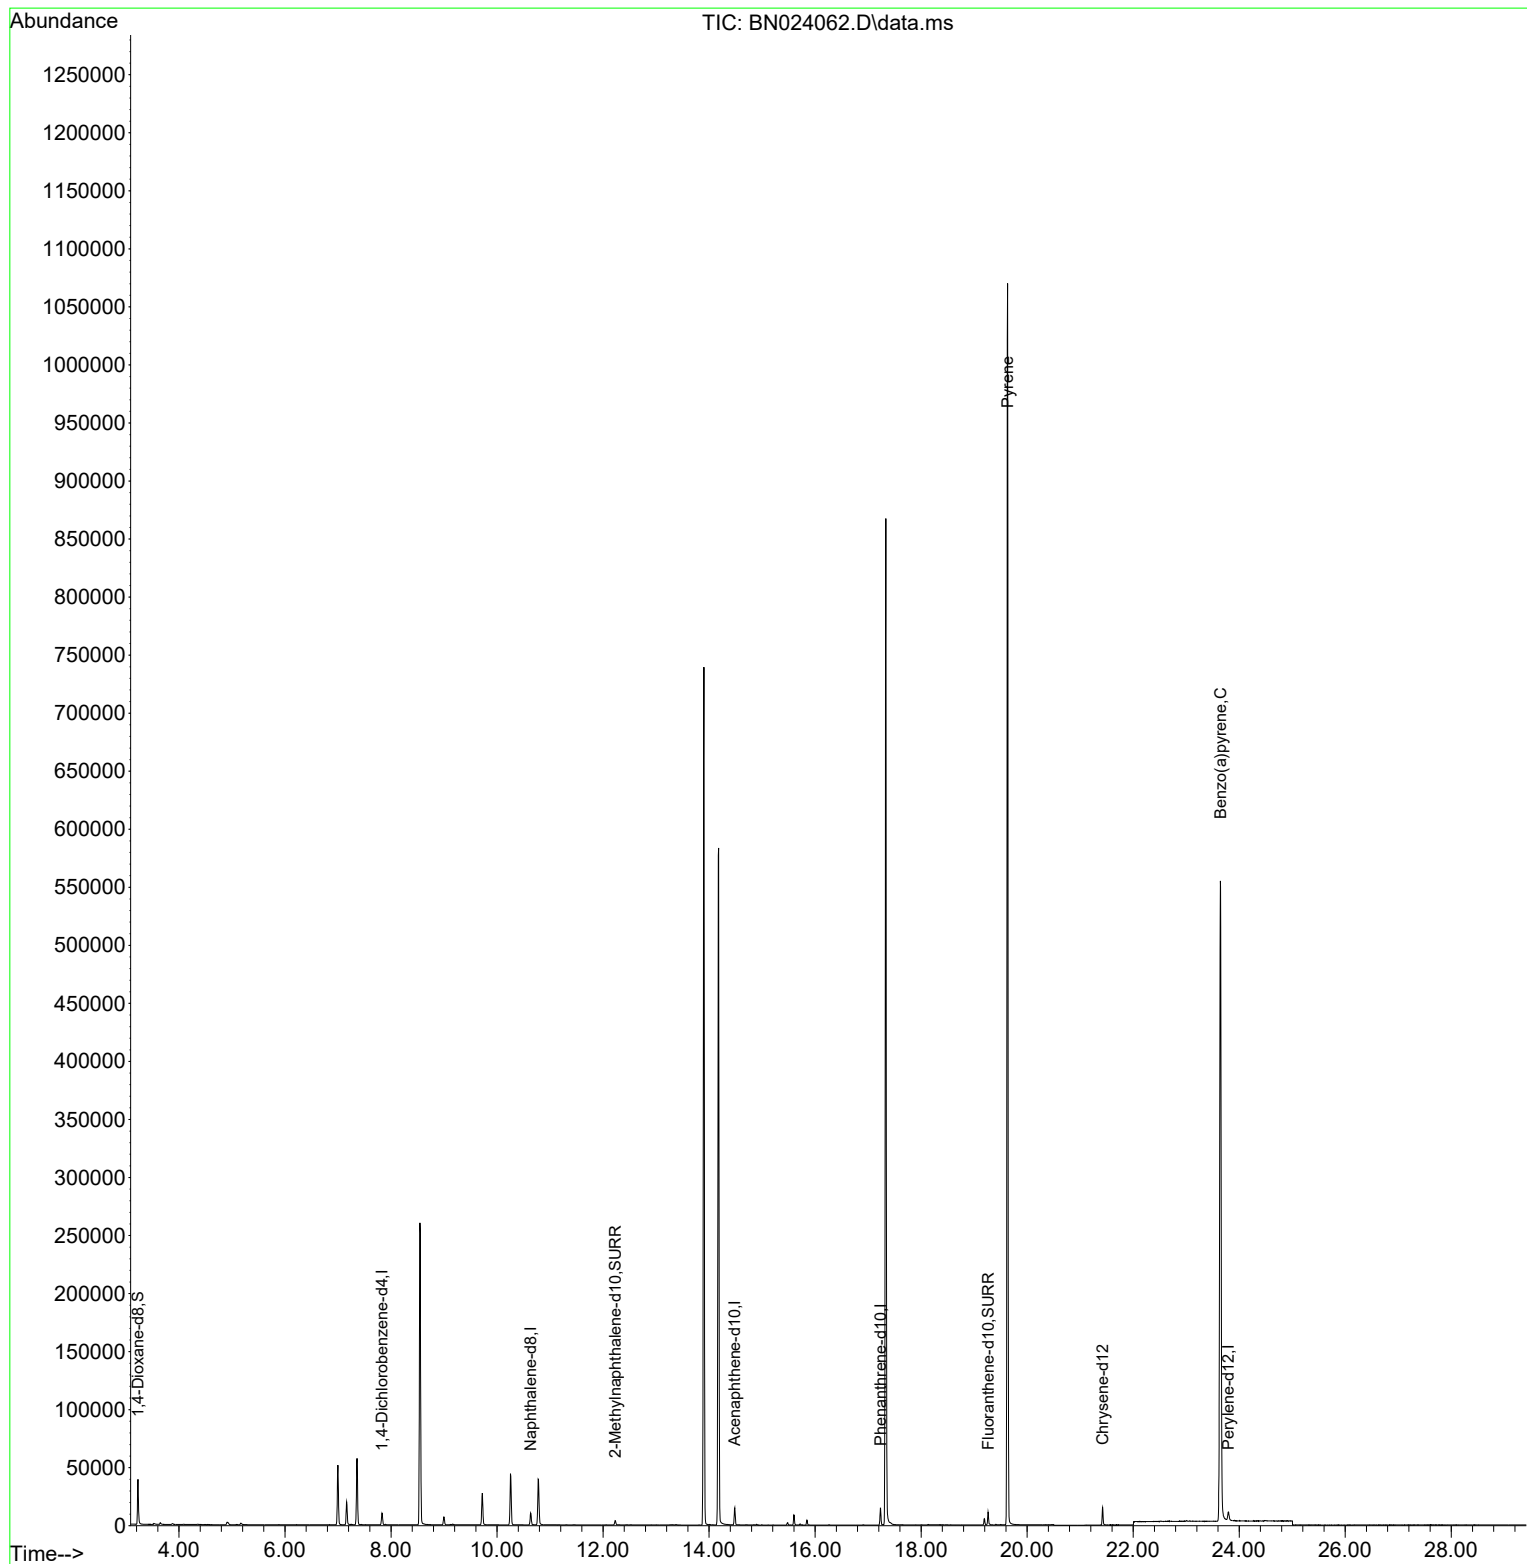

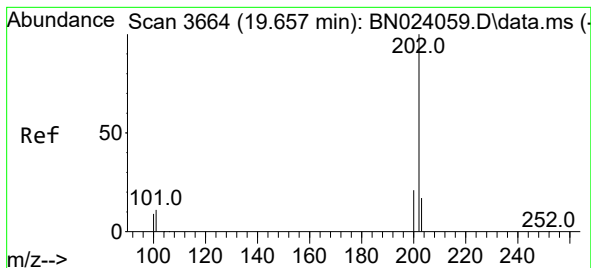

#20

Pyrene

Concen: 0.040 ng/ul

RT: 19.630 min Scan# 3

Delta R.T. -0.032 min

Lab File: BN024062.D

Acq: 17 Feb 2023 12:10

Instrument :

BNA_N

ClientSampleId :

C0B39





Tgt Ion:202 Resp: 1833

Ion Ratio Lower Upper

202 100

101 156.1 8.1 12.1#

100 1164.6 6.2 9.4#

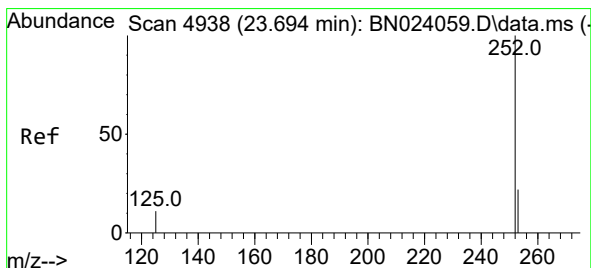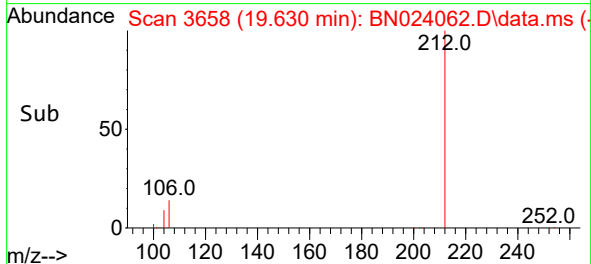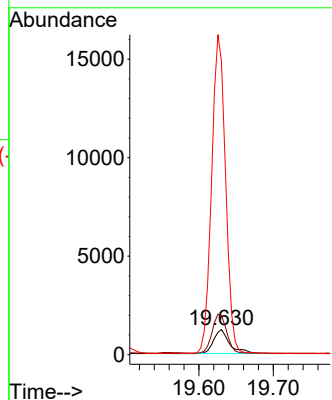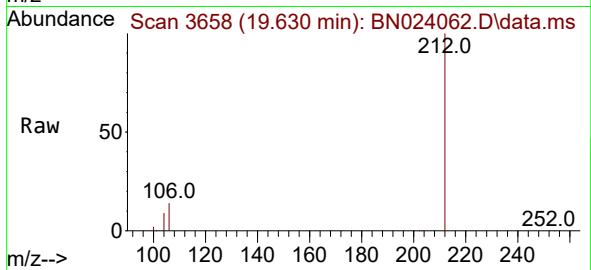

#26

Benzo(a)pyrene

Concen: 0.079 ng/ul

RT: 23.645 min Scan# 4921

Delta R.T. -0.061 min

Lab File: BN024062.D

Acq: 17 Feb 2023 12:10

Tgt Ion:252 Resp: 3094

Ion Ratio Lower Upper

252 100

253 53.6 21.5 32.3#

125 41.2 11.2 16.8#

