

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021723\
 Data File : BN024063.D
 Acq On : 17 Feb 2023 12:47
 Operator : CG/JU
 Sample : 01534-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B47

Quant Time: Feb 17 21:35:39 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 14:45:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.830	152	4324	0.400	ng/ul	0.00
4) Naphthalene-d8	10.634	136	11657	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.483	164	6961	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.234	188	16513	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.432	240	15276	0.400	ng/ul	# 0.00
23) Perylene-d12	23.820	264	12029	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.222	96	23658	5.104	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	5695	0.312	ng/ul	0.00
18) Fluoranthene-d10	19.262	212	17911	0.436	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.683	128	681	0.021	ng/ul#	73
15) Phenanthrene	17.272	178	1178	0.024	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021723\
Data File : BN024063.D
Acq On : 17 Feb 2023 12:47
Operator : CG/JU
Sample : 01534-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B47

Quant Time: Feb 17 21:35:39 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 14:45:13 2023
Response via : Initial Calibration




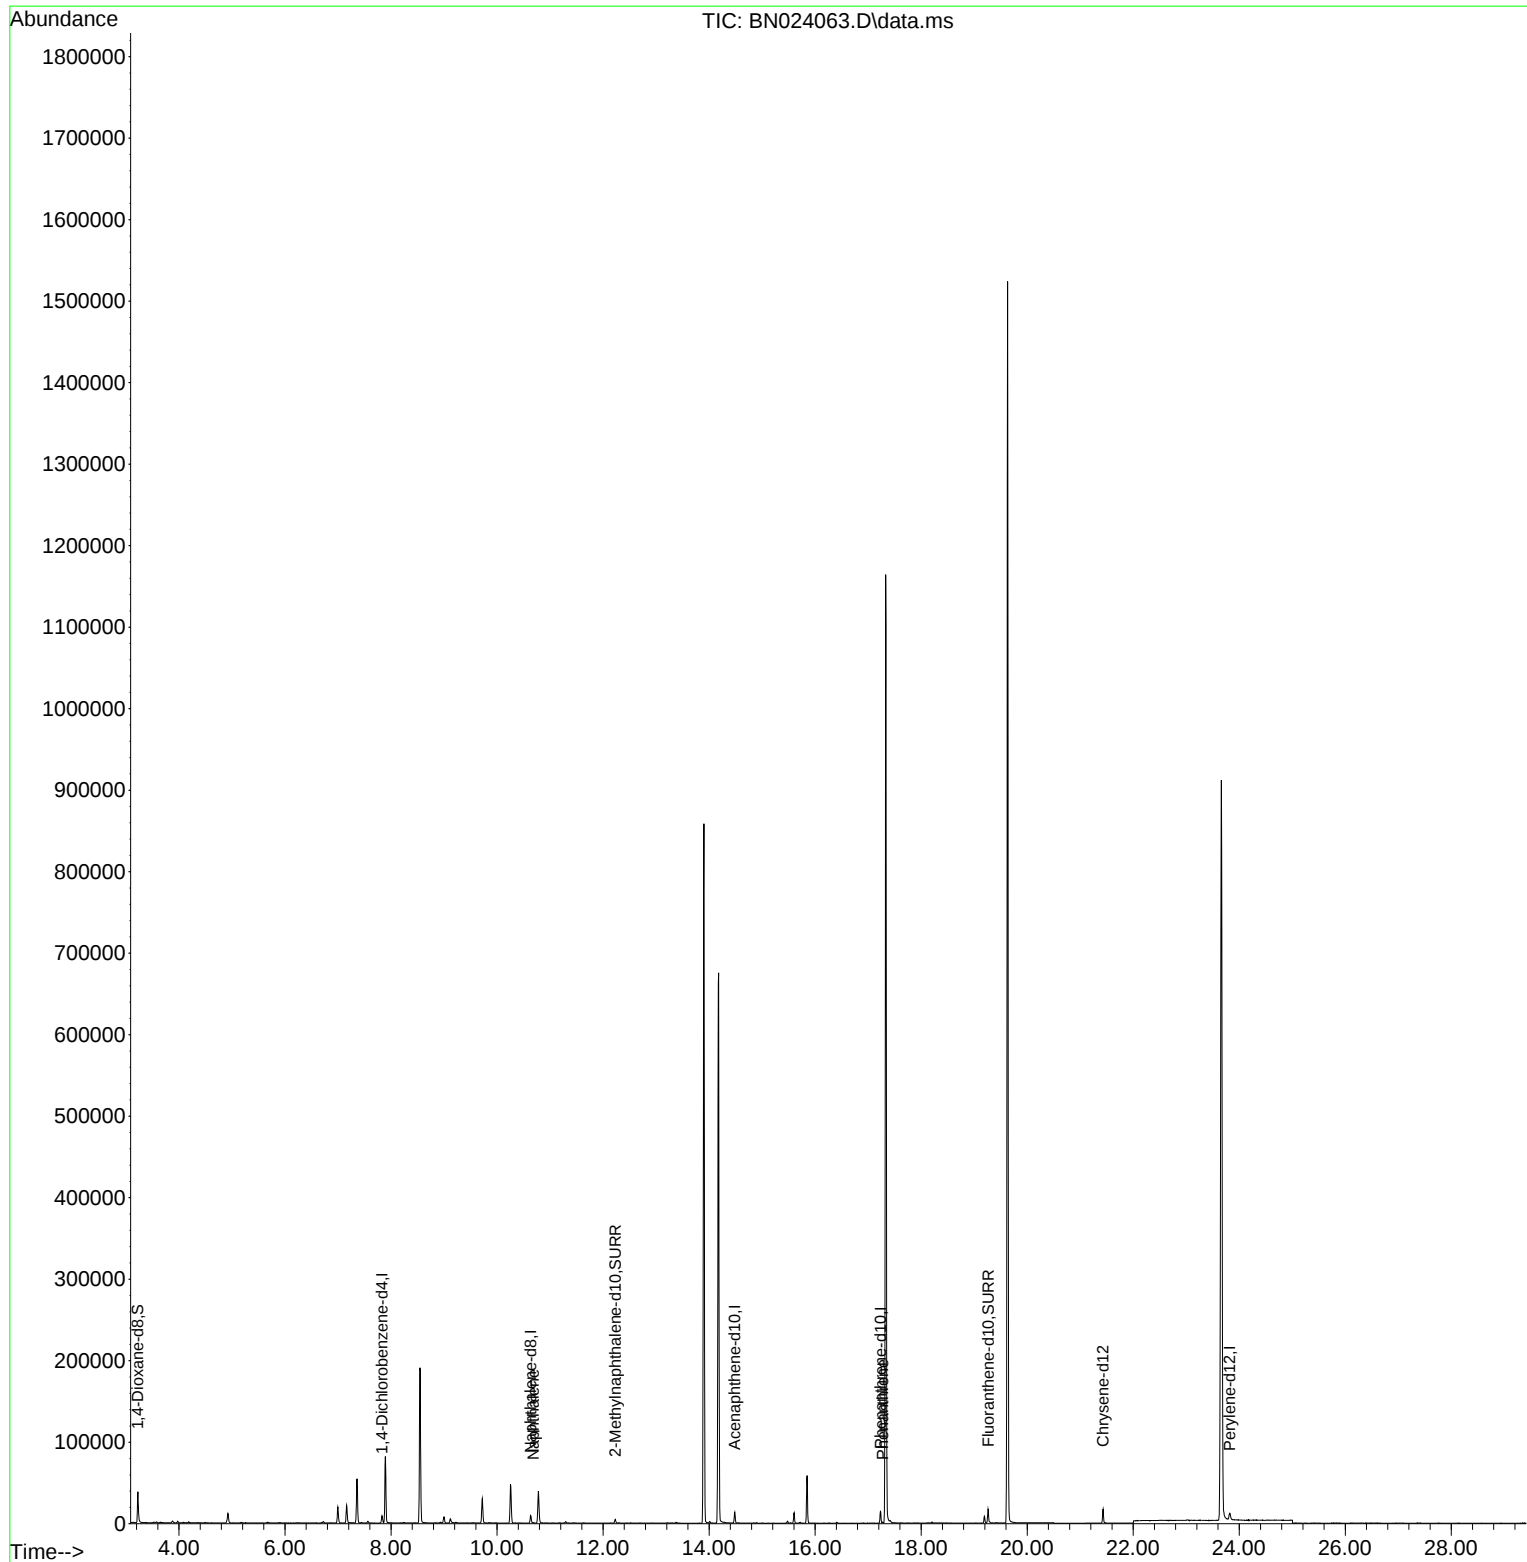


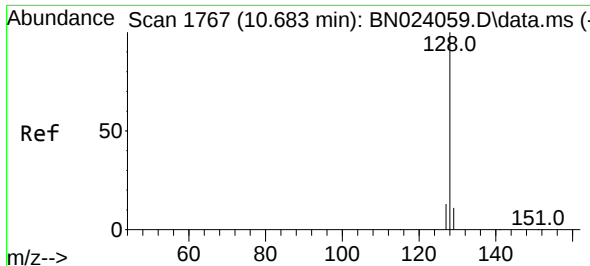

#5
Naphthalene
Concen: 0.021 ng/ul
RT: 10.683 min Scan# 1767
Delta R.T. -0.006 min
Lab File: BN024063.D
Acq: 17 Feb 2023 12:47

Instrument :
BNA_N
ClientSampleId :
C0B47

Tgt Ion:128 Resp: 681
Ion Ratio Lower Upper
128 100
129 24.3 9.7 14.5#
127 23.7 11.1 16.7#

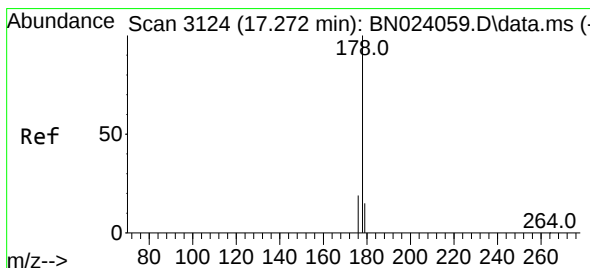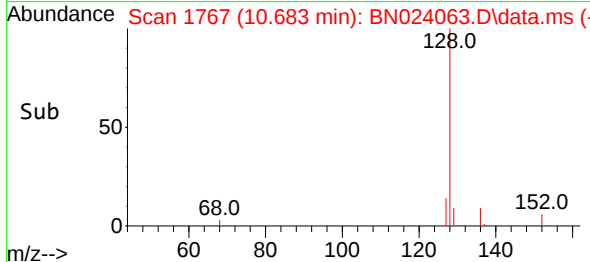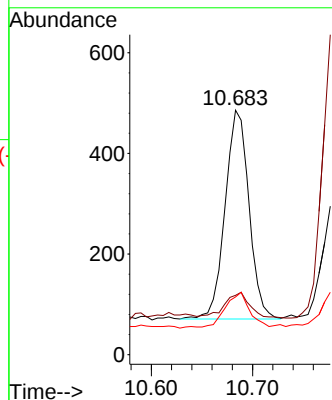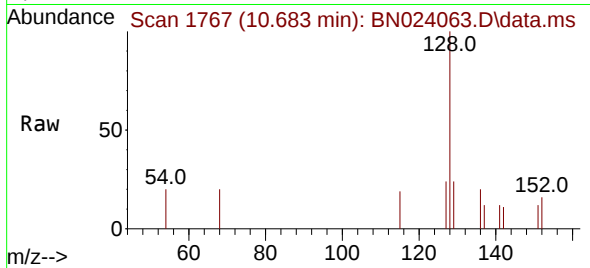

#15
Phenanthrene
Concen: 0.024 ng/ul
RT: 17.272 min Scan# 3124
Delta R.T. -0.009 min
Lab File: BN024063.D
Acq: 17 Feb 2023 12:47

Tgt Ion:178 Resp: 1178
Ion Ratio Lower Upper
178 100
179 24.1 12.6 19.0#
176 26.3 15.7 23.5#

