
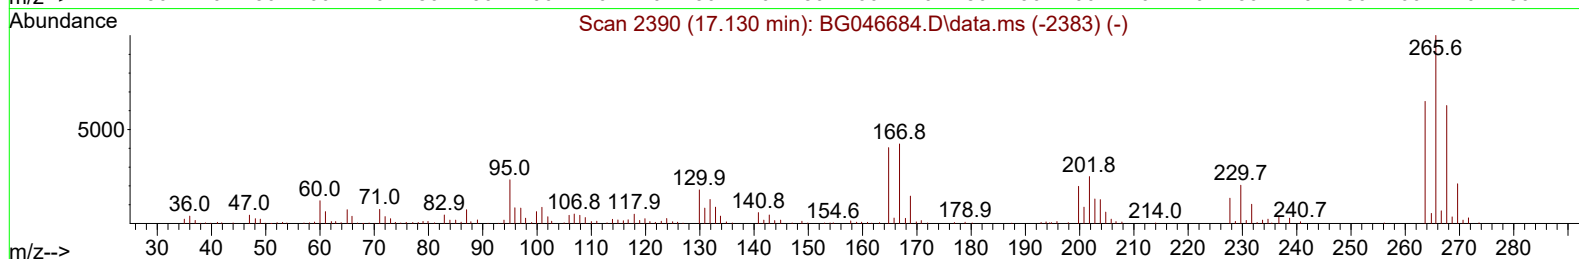
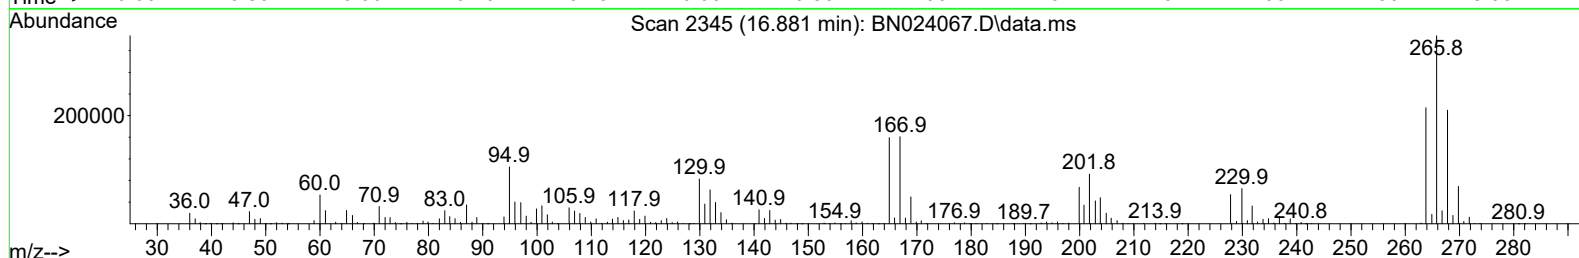


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021823\
Data File : BN024067.D
Acq On : 17 Feb 2023 15:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 03:57:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 18 03:57:25 2023
Response via : Initial Calibration

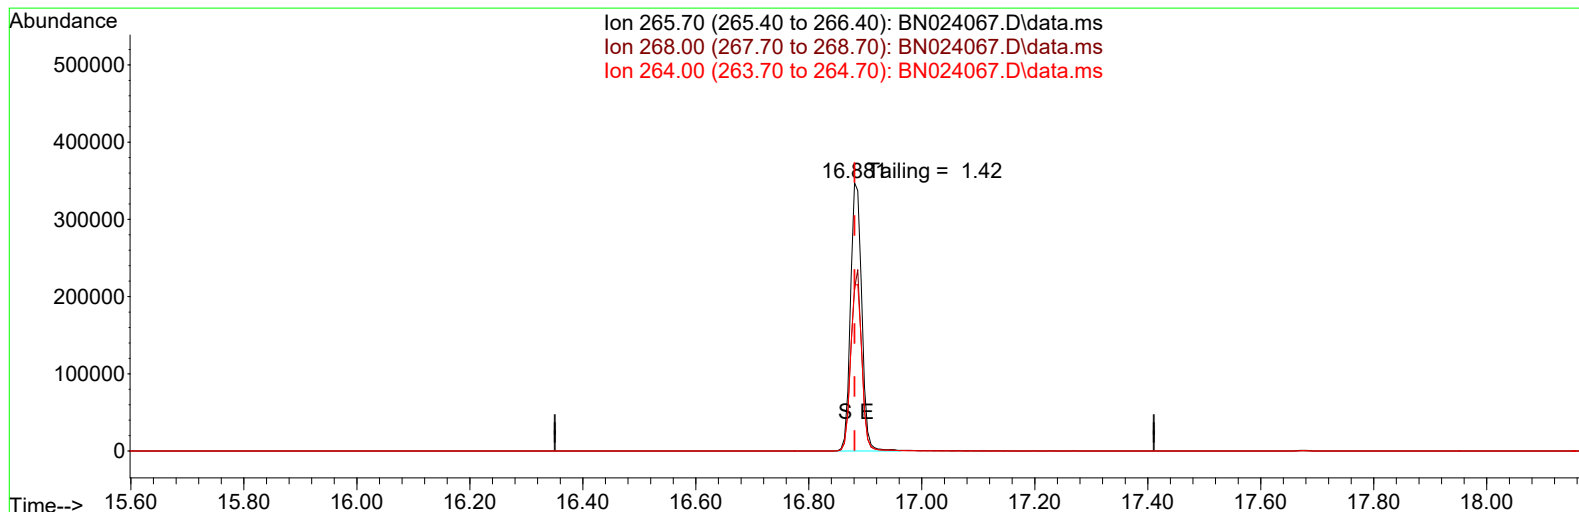

TIC: BN024067.D\data.ms

(70) Pentachlorophenol (C)




16.881min (0.000) 20666.14 ng

response 482169

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.49
264.00	61.60	61.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021823\
 Data File : BN024067.D
 Acq On : 17 Feb 2023 15:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 03:57:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 18 03:57:25 2023
 Response via : Initial Calibration

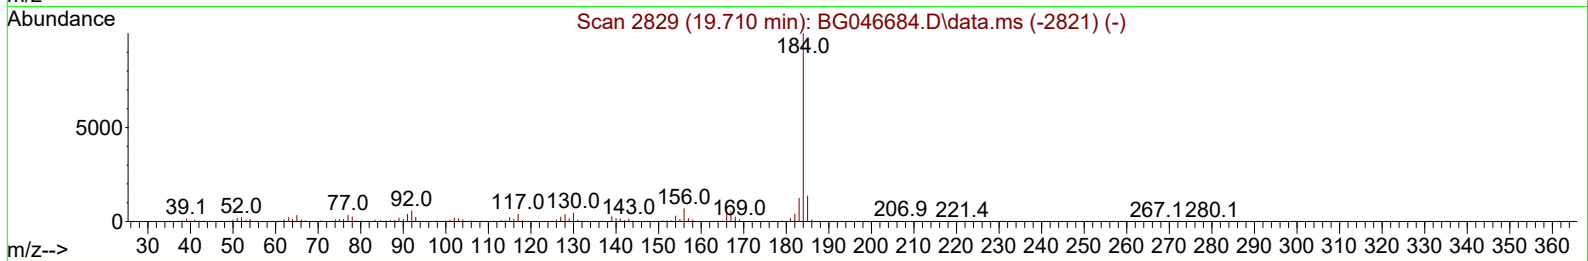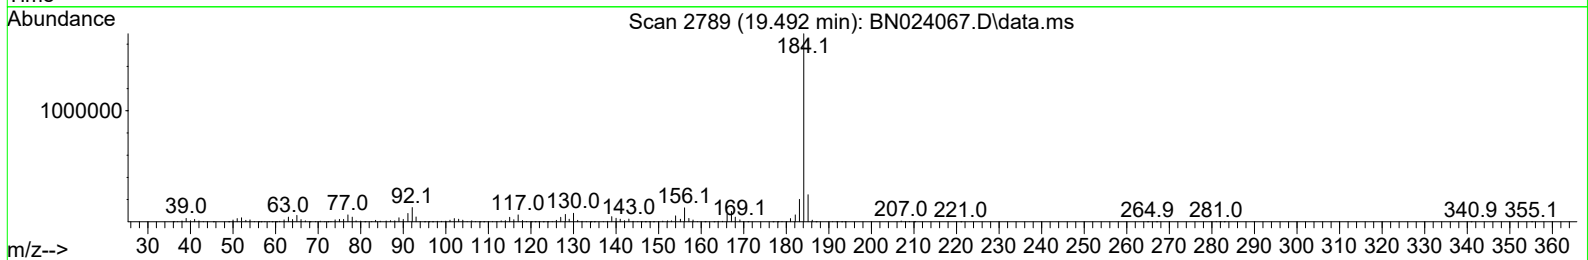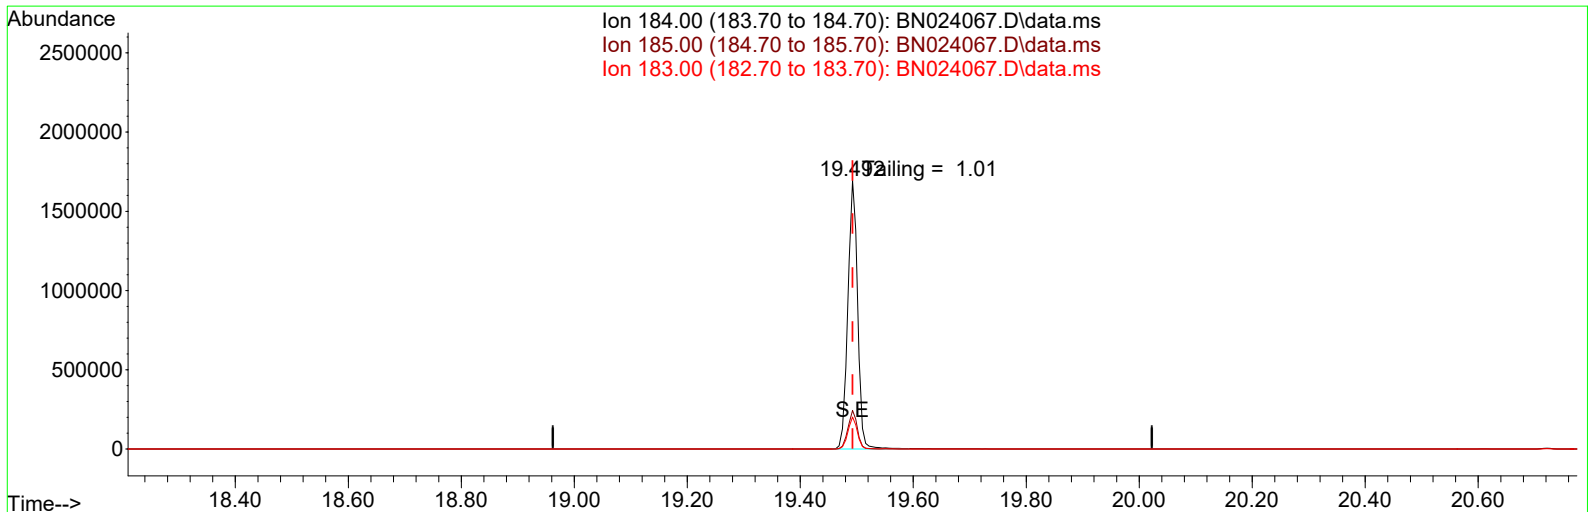

TIC: BN024067.D\data.ms

(77) Benzidine

19.492min (0.000) 0.00 ng

response 2043004

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.36
183.00	13.20	11.94
0.00	0.00	0.00