


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021823\
 Data File : BN024067.D
 Acq On : 17 Feb 2023 15:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN020723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 15 02:55:51 2023

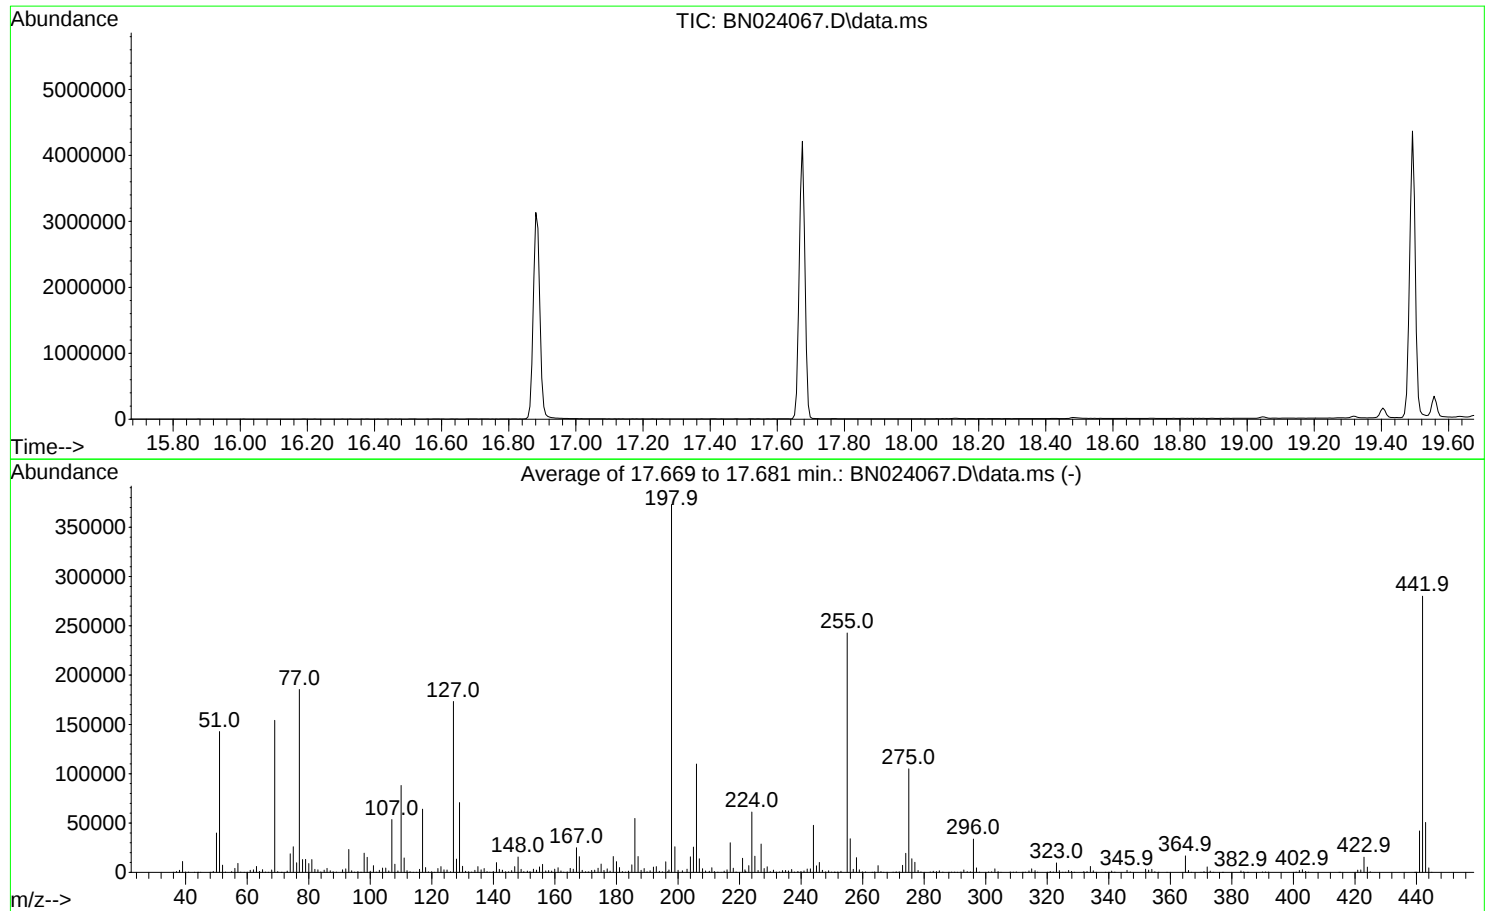




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	142800	PASS
68	69	0.00	2	1.6	2525	PASS
69	198	0.00	100	41.3	154117	PASS
70	69	0.00	2	0.6	849	PASS
127	198	10	80	46.5	173312	PASS
197	198	0.00	2	0.6	2418	PASS
198	198	100	100	100.0	373056	PASS
199	198	5	9	7.0	26037	PASS
275	198	10	60	28.1	105013	PASS
365	198	1	100	4.5	16734	PASS
441	198	0.01	100	11.3	42096	PASS
442	442	50	100	100.0	280149	PASS
443	442	15	24	18.1	50672	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021823\
Data File : BN024067.D
Acq On : 17 Feb 2023 15:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 18 03:57:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 18 03:57:25 2023
Response via : Initial Calibration

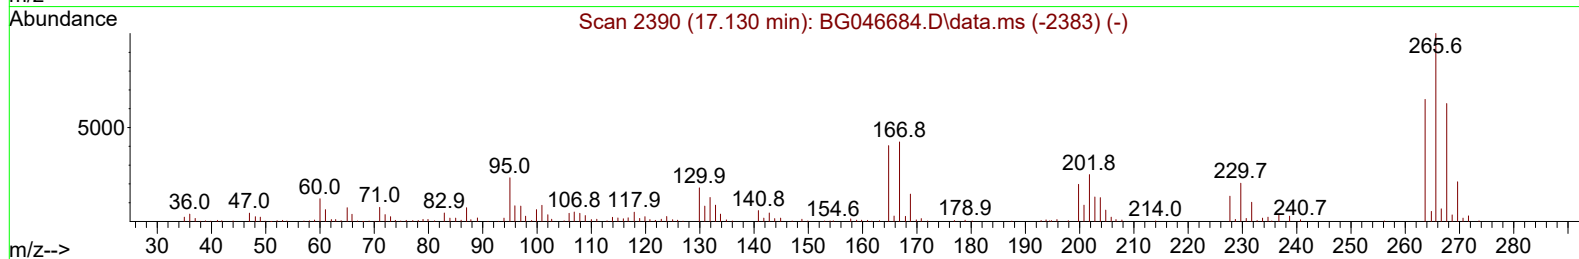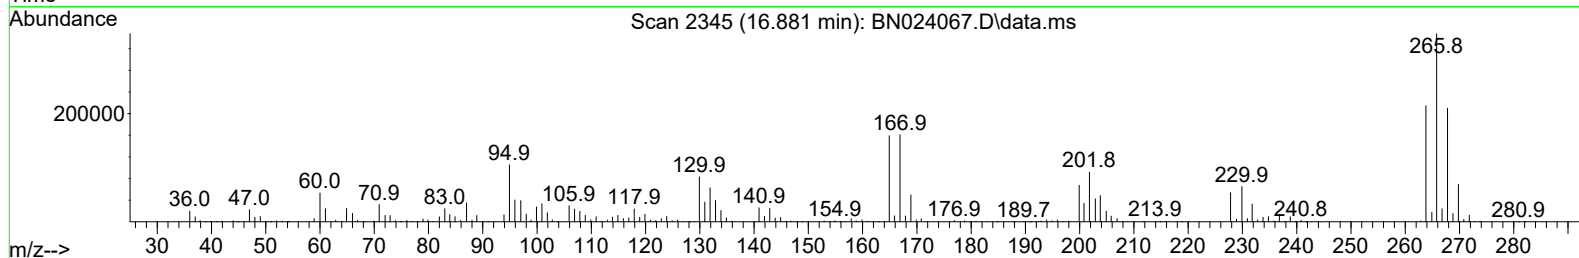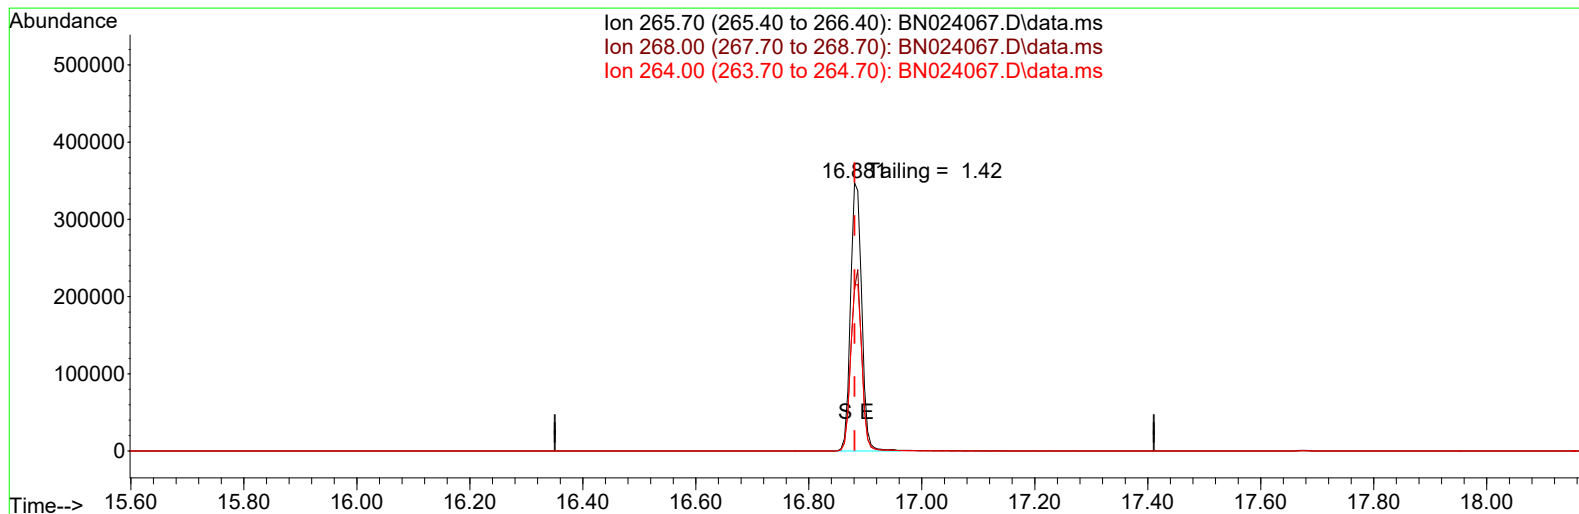

TIC: BN024067.D\data.ms

(70) Pentachlorophenol (C)

16.881min (0.000) 20666.14 ng




response 482169

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.49
264.00	61.60	61.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN021823\
Data File : BN024067.D
Acq On : 17 Feb 2023 15:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 18 03:57:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 18 03:57:25 2023
Response via : Initial Calibration

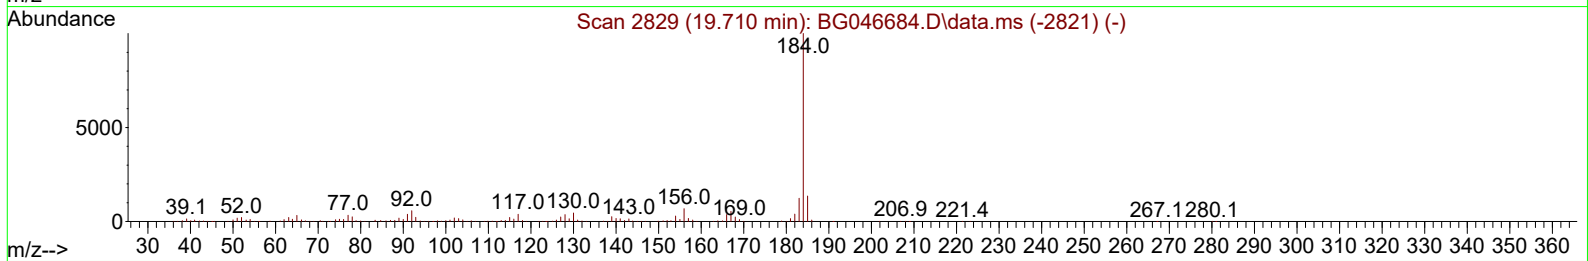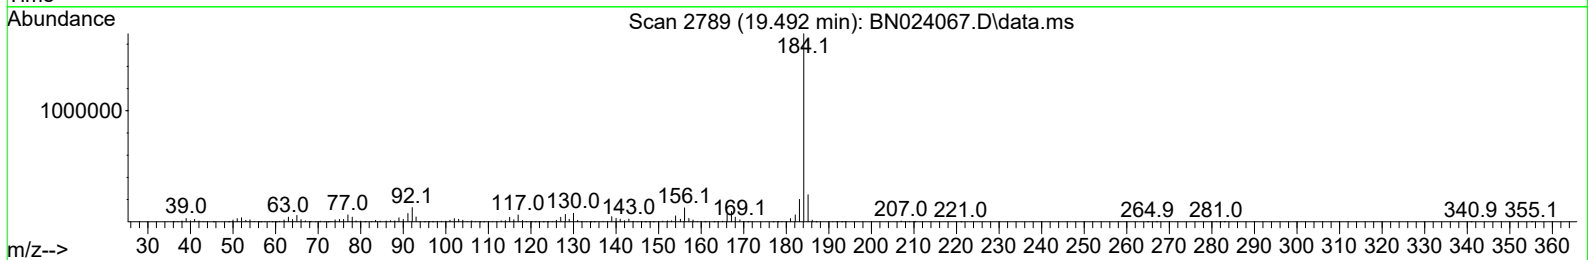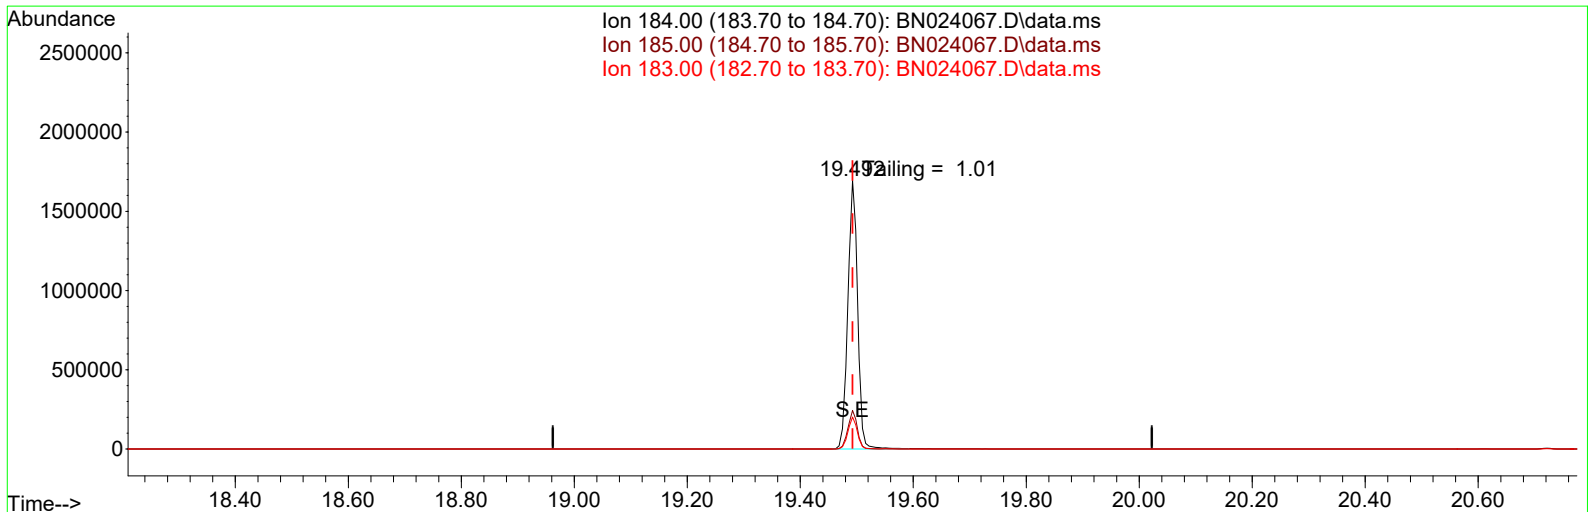

TIC: BN024067.D\data.ms

(77) Benzidine

19.492min (0.000) 0.00 ng

response 2043004

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.36
183.00	13.20	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/18/2023	BNA_N	<u>BN024067.D</u>
Compound Name	Response	Retention Time
DDT	1156990	20.722
DDD	18440	20.281
DDE	843	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19283	1176273	1.64

Instrument :
BNA_N
ClientSampleId :
DFTPP