

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022222\
 Data File : BN018678.D
 Acq On : 22 Feb 2022 15:37
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Feb 22 16:11:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 22 13:54:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	6859	0.400	ng	0.00
7) Naphthalene-d8	10.722	136	14186	0.400	ng	# 0.00
13) Acenaphthene-d10	14.549	164	6772	0.400	ng	0.00
19) Phenanthrene-d10	17.287	188	12165	0.400	ng	0.00
29) Chrysene-d12	21.458	240	10547	0.400	ng	# 0.00
35) Perylene-d12	23.858	264	8400	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.471	112	76894	4.413	ng	0.00
5) Phenol-d6	7.067	99	92292	4.832	ng	0.00
8) Nitrobenzene-d5	9.068	82	62304	6.354	ng	0.00
11) 2-Methylnaphthalene-d10	12.310	152	108834	4.754	ng	0.00
14) 2,4,6-Tribromophenol	0.000	330	0d	0.000	ng	
15) 2-Fluorobiphenyl	13.180	172	159789	5.950	ng	0.00
27) Fluoranthene-d10	19.312	212	181104	5.058	ng	0.00
31) Terphenyl-d14	19.906	244	111420	4.157	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.326	88	37161	7.612	ng	# 57
3) n-Nitrosodimethylamine	3.637	42	40786	5.743	ng	88
6) bis(2-Chloroethyl)ether	7.327	93	87404	4.319	ng	99
9) Naphthalene	10.776	128	205070	5.521	ng	100
10) Hexachlorobutadiene	11.075	225	48661	6.417	ng	# 100
12) 2-Methylnaphthalene	12.382	142	134256	5.378	ng	98
16) Acenaphthylene	14.260	152	182499	6.403	ng	100
17) Acenaphthene	14.613	154	116653	6.123	ng	96
18) Fluorene	15.586	166	140456	6.010	ng	99
21) 4-Bromophenyl-phenylether	16.477	248	46142	6.254	ng	96
22) Hexachlorobenzene	16.600	284	53906	6.533	ng	# 88
23) Atrazine	16.733	200	29234	6.524	ng	91
25) Phenanthrene	17.328	178	212016	5.958	ng	99
26) Anthracene	17.420	178	193079	6.391	ng	100
28) Fluoranthene	19.341	202	231851	5.913	ng	# 97
30) Pyrene	19.704	202	231935	6.420	ng	100
32) Benzo(a)anthracene	21.449	228	212732	6.069	ng	100
33) Chrysene	21.494	228	220896	6.218	ng	99
34) Bis(2-ethylhexyl)phtha...	21.378	149	92968	6.549	ng	# 96
36) Indeno(1,2,3-cd)pyrene	26.343	276	234140	7.751	ng	# 90
37) Benzo(b)fluoranthene	23.127	252	196761	6.804	ng	# 97
38) Benzo(k)fluoranthene	23.177	252	203086	7.027	ng	# 97
39) Benzo(a)pyrene	23.750	252	163297	7.057	ng	# 97
40) Dibenzo(a,h)anthracene	26.363	278	184170	7.820	ng	# 95
41) Benzo(g,h,i)perylene	27.109	276	196328	7.469	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022222\
Data File : BN018678.D
Acq On : 22 Feb 2022 15:37
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Quant Time: Feb 22 16:11:10 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 22 13:54:19 2022
Response via : Initial Calibration




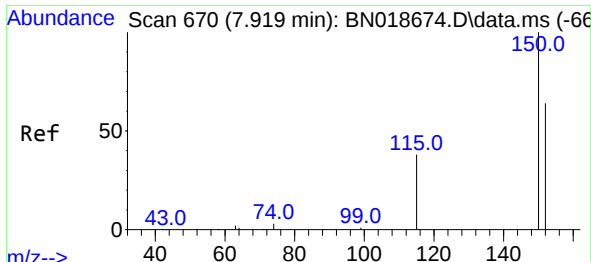


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.919 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0







Tgt Ion:152 Resp: 6859
Ion Ratio Lower Upper
152 100
150 153.4 121.7 182.5
115 58.3 43.8 65.8



#2
1,4-Dioxane
Concen: 7.612 ng
RT: 3.326 min Scan# 34
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion: 88 Resp: 37161
Ion Ratio Lower Upper
88 100
43 30.3 69.7 104.5#
58 76.9 83.8 125.8#









#3
n-Nitrosodimethylamine
Concen: 5.743 ng
RT: 3.637 min Scan# 71
Delta R.T. -0.007 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion: 42 Resp: 40786




Ion	Ratio	Lower	Upper
42	100		
74	120.6	108.6	163.0
44	6.6	5.8	8.8




#4
2-Fluorophenol
Concen: 4.413 ng
RT: 5.471 min Scan# 331
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion: 112 Resp: 76894

Ion	Ratio	Lower	Upper
112	100		
64	59.4	48.0	72.0
63	31.4	25.3	37.9









#5
Phenol-d6
Concen: 4.832 ng
RT: 7.067 min Scan# 51
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 92292
Ion Ratio Lower Upper
99 100
42 20.2 16.3 24.5
71 34.6 26.8 40.2



#6
bis(2-Chloroethyl)ether
Concen: 4.319 ng
RT: 7.327 min Scan# 588
Delta R.T. -0.007 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion: 93 Resp: 87404
Ion Ratio Lower Upper
93 100
63 77.8 61.7 92.5
95 32.7 26.2 39.4









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.722 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	14186
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.8	13.2
54	9.0	5.0	7.6#
68	6.9	4.4	6.6#



#8
Nitrobenzene-d5
Concen: 6.354 ng
RT: 9.068 min Scan# 795
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion:	82	Resp:	62304
Ion	Ratio	Lower	Upper
82	100		
128	38.0	33.7	50.5
54	52.2	36.6	55.0









#9
Naphthalene
Concen: 5.521 ng
RT: 10.776 min Scan# 955
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 205070
Ion Ratio Lower Upper
128 100
129 10.8 8.7 13.1
127 12.8 10.4 15.6



#10
Hexachlorobutadiene
Concen: 6.417 ng
RT: 11.075 min Scan# 983
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion:225 Resp: 48661
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.7 51.0 76.6









#11
2-Methylnaphthalene-d10
Concen: 4.754 ng
RT: 12.310 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 108834
Ion Ratio Lower Upper
152 100
151 20.8 16.2 24.2



#12
2-Methylnaphthalene
Concen: 5.378 ng
RT: 12.382 min Scan# 1254
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion:142 Resp: 134256
Ion Ratio Lower Upper
142 100
141 88.1 70.0 105.0
115 37.6 27.8 41.8









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.549 min Scan# 14
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 6772
Ion Ratio Lower Upper
164 100
162 105.2 80.2 120.2
160 48.7 36.9 55.3




#14
2,4,6-Tribromophenol
Concen: 0.000 ng
Expected RT: 16.03 min

Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion: 330
Sig Exp Ratio
330 100
332 0.0
141 26.6









#15
2-Fluorobiphenyl
Concen: 5.950 ng
RT: 13.180 min Scan# 1350
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:172 Resp: 159789
Ion Ratio Lower Upper
172 100
171 34.1 27.4 41.0
170 22.1 18.4 27.6



#16
Acenaphthylene
Concen: 6.403 ng
RT: 14.260 min Scan# 1451
Delta R.T. -0.011 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion:152 Resp: 182499
Ion Ratio Lower Upper
152 100
151 19.9 15.8 23.6
153 13.1 10.5 15.7









#17
Acenaphthene
Concen: 6.123 ng
RT: 14.613 min Scan# 1484
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 116653
Ion Ratio Lower Upper
154 100
153 109.0 90.9 136.3
152 53.4 45.0 67.4



#18
Fluorene
Concen: 6.010 ng
RT: 15.586 min Scan# 1575
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion:166 Resp: 140456
Ion Ratio Lower Upper
166 100
165 98.1 77.8 116.6
167 13.4 10.9 16.3









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.287 min Scan# 1740
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 12165
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.2 7.0 10.4



#21
4-Bromophenyl-phenylether
Concen: 6.254 ng
RT: 16.477 min Scan# 1661
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion:248 Resp: 46142
Ion Ratio Lower Upper
248 100
250 97.1 74.4 111.6
141 57.7 43.7 65.5









#22
Hexachlorobenzene
Concen: 6.533 ng
RT: 16.600 min Scan# 1673
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:284 Resp: 53906
Ion Ratio Lower Upper
284 100
142 36.9 21.6 32.4#
249 32.6 23.5 35.3



#23
Atrazine
Concen: 6.524 ng
RT: 16.733 min Scan# 1686
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion:200 Resp: 29234
Ion Ratio Lower Upper
200 100
173 29.9 20.3 30.5
215 44.7 40.4 60.6









#25
Phenanthrene
Concen: 5.958 ng
RT: 17.328 min Scan# 1744
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 212016
Ion Ratio Lower Upper
178 100
176 19.3 15.3 22.9
179 15.1 12.3 18.5



#26
Anthracene
Concen: 6.391 ng
RT: 17.420 min Scan# 1753
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion:178 Resp: 193079
Ion Ratio Lower Upper
178 100
176 18.6 14.8 22.2
179 15.2 12.2 18.4









#27
Fluoranthene-d10
Concen: 5.058 ng
RT: 19.312 min Scan# 2120
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 181104
Ion Ratio Lower Upper
212 100
106 15.2 8.4 12.6#
104 8.5 4.5 6.7#



#28
Fluoranthene
Concen: 5.913 ng
RT: 19.341 min Scan# 2127
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion:202 Resp: 231851
Ion Ratio Lower Upper
202 100
101 11.8 7.2 10.8#
203 17.3 13.7 20.5









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.458 min Scan# 2448
Delta R.T. -0.009 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 10547
Ion Ratio Lower Upper
240 100
120 16.6 6.0 9.0#
236 29.2 21.4 32.2



#30
Pyrene
Concen: 6.420 ng
RT: 19.704 min Scan# 2213
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion:202 Resp: 231935
Ion Ratio Lower Upper
202 100
200 21.1 16.6 25.0
203 17.7 14.1 21.1









#31
 Terphenyl-d14
 Concen: 4.157 ng
 RT: 19.906 min Scan# 2114
 Delta R.T. 0.000 min
 Lab File: BN018678.D
 Acq: 22 Feb 2022 15:37




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:244 Resp: 111420
 Ion Ratio Lower Upper
 244 100
 212 10.0 6.2 9.2#
 122 0.0 7.9 11.9#



#32
 Benzo(a)anthracene
 Concen: 6.069 ng
 RT: 21.449 min Scan# 2446
 Delta R.T. 0.000 min
 Lab File: BN018678.D
 Acq: 22 Feb 2022 15:37

Tgt Ion:228 Resp: 212732
 Ion Ratio Lower Upper
 228 100
 226 26.7 21.3 31.9
 229 19.8 15.9 23.9









#33
Chrysene
Concen: 6.218 ng
RT: 21.494 min Scan# 2451
Delta R.T. -0.009 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:228 Resp: 220896
Ion Ratio Lower Upper
228 100
226 31.1 24.2 36.4
229 19.3 15.5 23.3



#34
Bis(2-ethylhexyl)phthalate
Concen: 6.549 ng
RT: 21.378 min Scan# 2438
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion:149 Resp: 92968
Ion Ratio Lower Upper
149 100
167 27.3 23.7 35.5
279 2.7 3.6 5.4









#35
Perylene-d12
Concen: 0.400 ng
RT: 23.858 min Scan# 30
Delta R.T. -0.003 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:264 Resp: 8400
Ion Ratio Lower Upper
264 100
260 27.6 20.2 30.4
265 35.2 18.2 27.2#



#36
Indeno(1,2,3-cd)pyrene
Concen: 7.751 ng
RT: 26.343 min Scan# 3899
Delta R.T. -0.009 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Tgt Ion:276 Resp: 234140
Ion Ratio Lower Upper
276 100
138 28.6 14.9 22.3#
277 24.8 19.9 29.9





#37

Benzo(b)fluoranthene

Concen: 6.804 ng

RT: 23.127 min Scan# 21

Delta R.T. -0.003 min

Lab File: BN018678.D

Acq: 22 Feb 2022 15:37

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:252 Resp: 196761

Ion Ratio Lower Upper

252 100

253 22.0 17.8 26.6

125 11.1 6.0 9.0#



#38

Benzo(k)fluoranthene

Concen: 7.027 ng

RT: 23.177 min Scan# 2816

Delta R.T. 0.000 min

Lab File: BN018678.D

Acq: 22 Feb 2022 15:37




Tgt Ion:252 Resp: 203086


Ion Ratio Lower Upper

252 100

253 22.0 17.7 26.5

125 10.9 6.2 9.2#









#39
Benzo(a)pyrene
Concen: 7.057 ng
RT: 23.750 min Scan# 3013
Delta R.T. -0.003 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 163297
Ion Ratio Lower Upper
252 100
253 21.8 17.8 26.6
125 12.2 7.0 10.4#



#40
Dibenzo(a,h)anthracene
Concen: 7.820 ng
RT: 26.363 min Scan# 3906
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37


Tgt Ion:278 Resp: 184170
Ion Ratio Lower Upper
278 100
139 19.4 10.8 16.2#
279 23.6 19.0 28.4





#41
Benzo(g,h,i)perylene
Concen: 7.469 ng
RT: 27.109 min Scan# 41
Delta R.T. 0.000 min
Lab File: BN018678.D
Acq: 22 Feb 2022 15:37

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Tgt Ion:276 Resp: 196328
Ion Ratio Lower Upper
276 100
277 23.6 19.0 28.6
138 24.7 12.6 19.0#

