
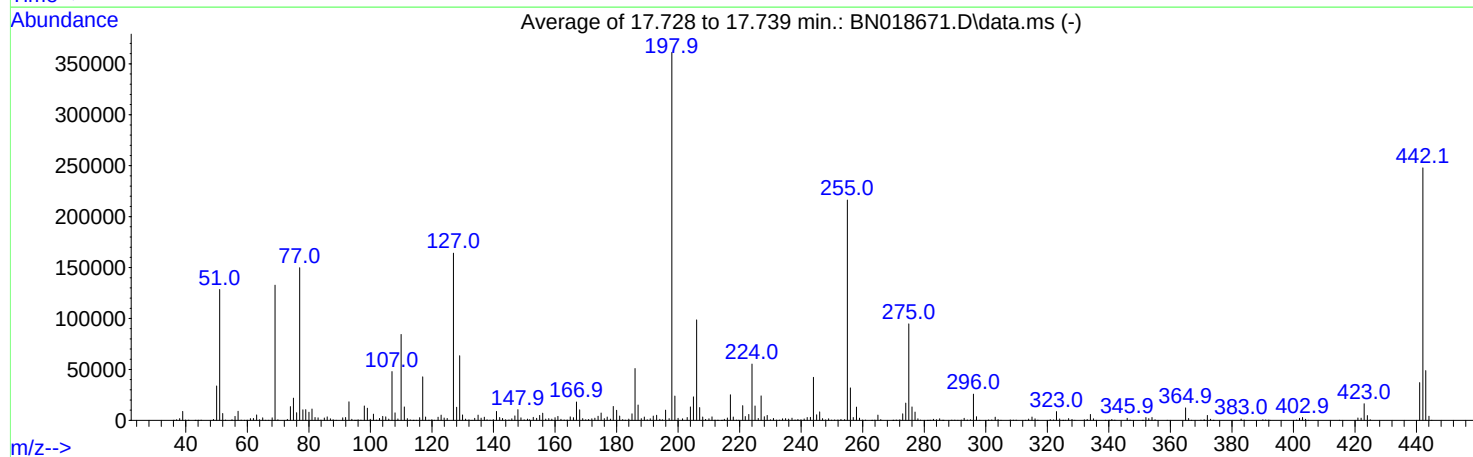


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022222\
 Data File : BN018671.D
 Acq On : 22 Feb 2022 10:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 22 16:23:51 2022

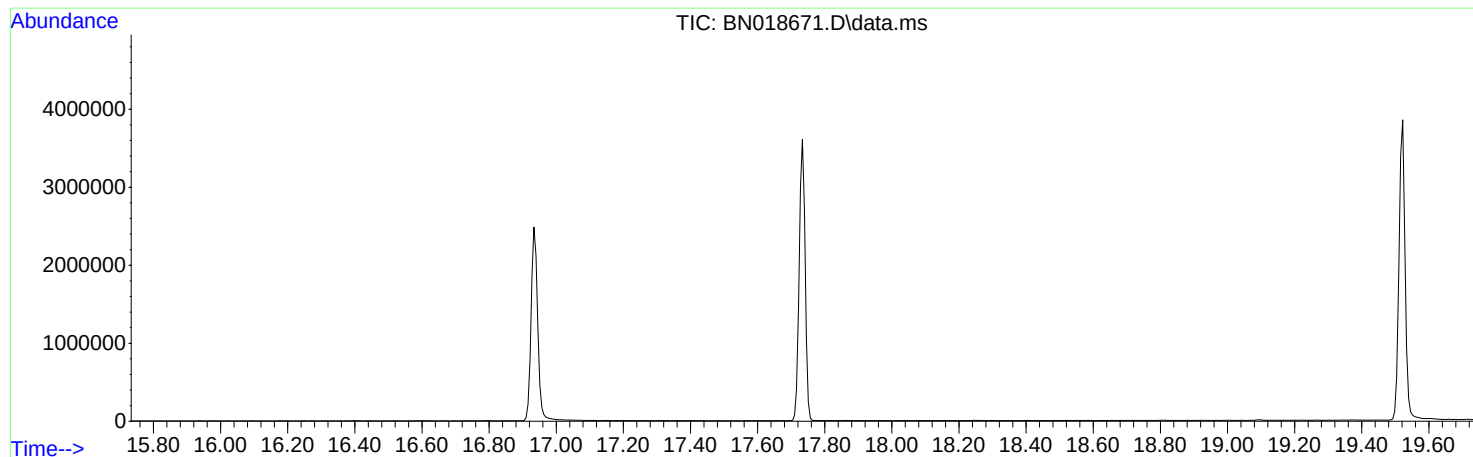




AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	128405	PASS
68	69	0.00	2	2.0	2602	PASS
69	198	0.00	100	36.8	132779	PASS
70	69	0.00	2	0.5	692	PASS
127	198	10	80	45.5	164160	PASS
197	198	0.00	2	0.5	1746	PASS
198	198	100	100	100.0	361088	PASS
199	198	5	9	6.6	23920	PASS
275	198	10	60	26.2	94688	PASS
365	198	1	100	3.4	12301	PASS
441	198	0.01	100	10.2	37008	PASS
442	442	50	100	100.0	247851	PASS
443	442	15	24	19.7	48928	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022222\
Data File : BN018671.D
Acq On : 22 Feb 2022 10:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 22 12:59:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 22 12:59:22 2022
Response via : Initial Calibration

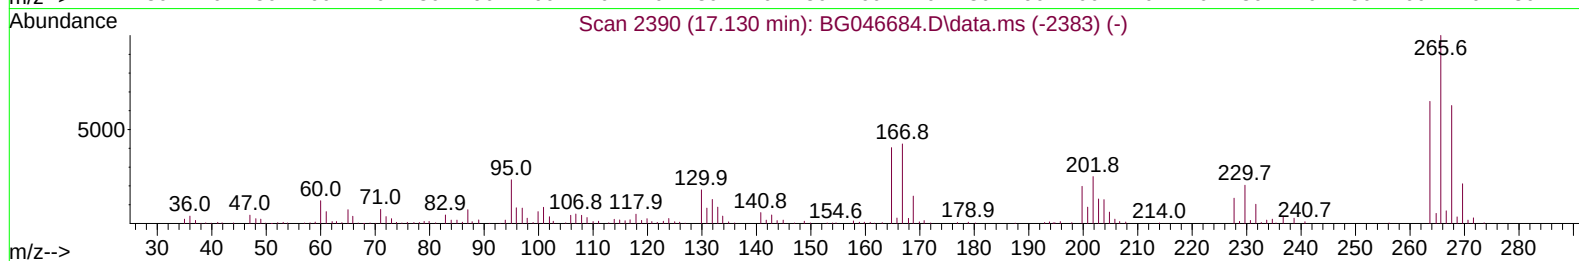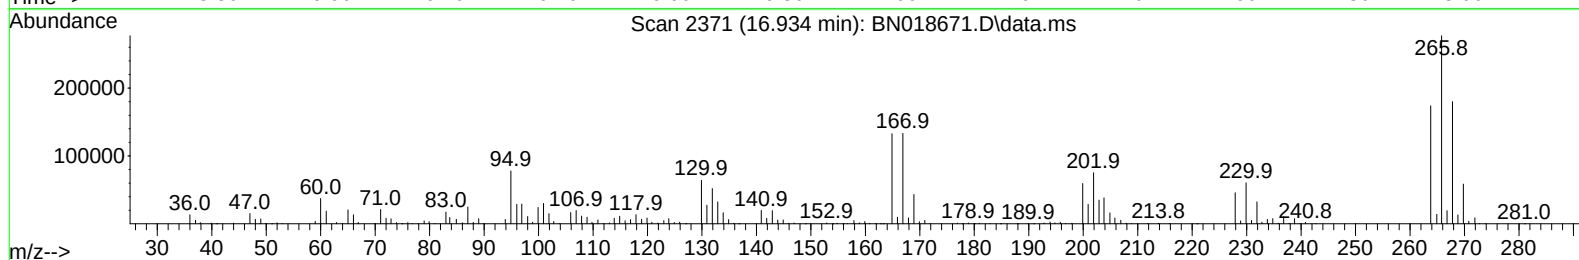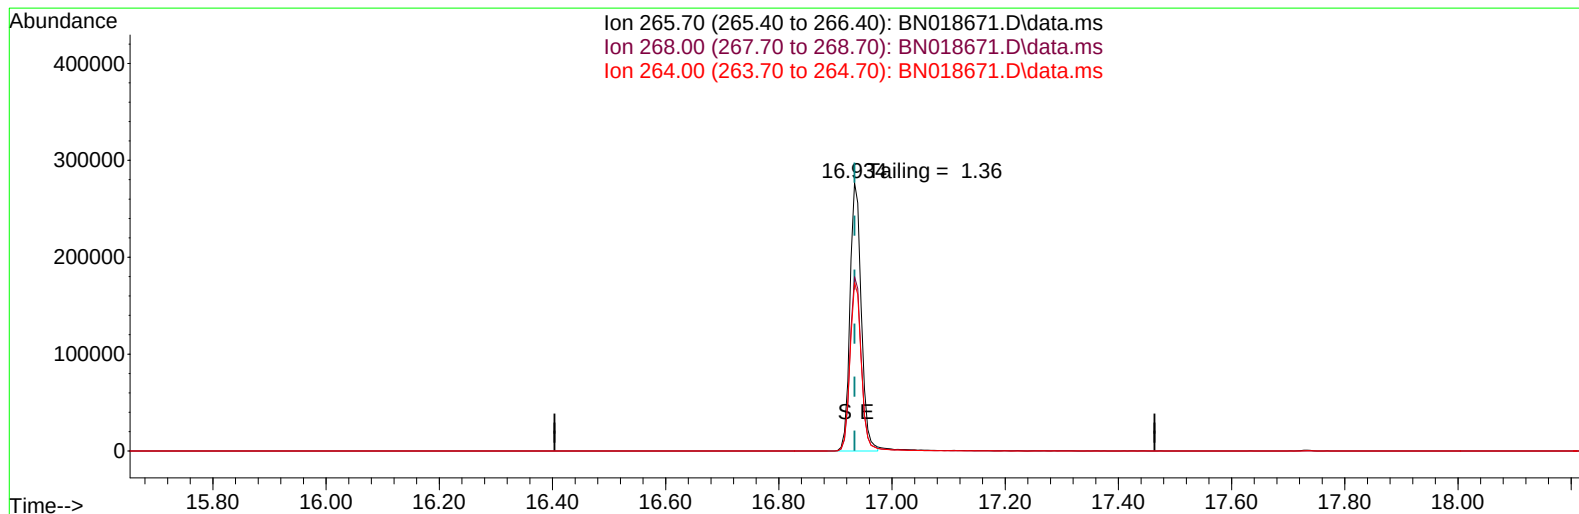

TIC: BN018671.D\data.ms

(70) Pentachlorophenol (C)

16.934min (0.000) 18971.00 ng




response 392149

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.95
264.00	61.60	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022222\
 Data File : BN018671.D
 Acq On : 22 Feb 2022 10:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Feb 22 12:59:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 22 12:59:22 2022
 Response via : Initial Calibration

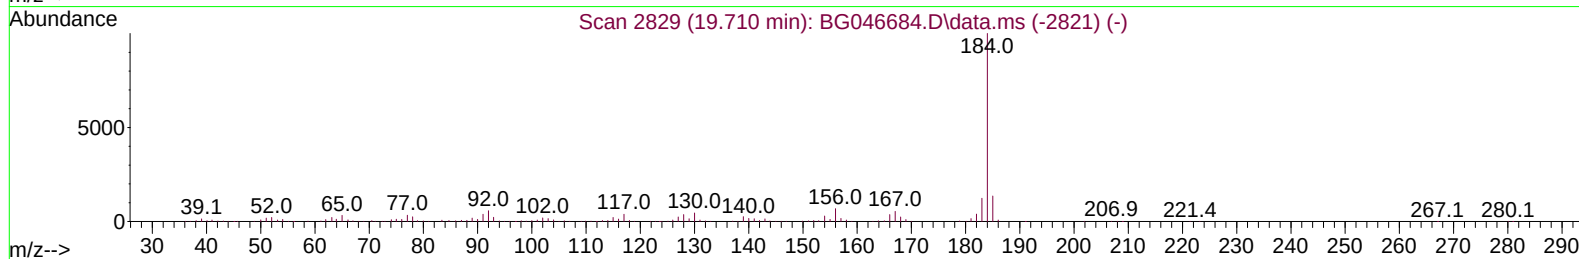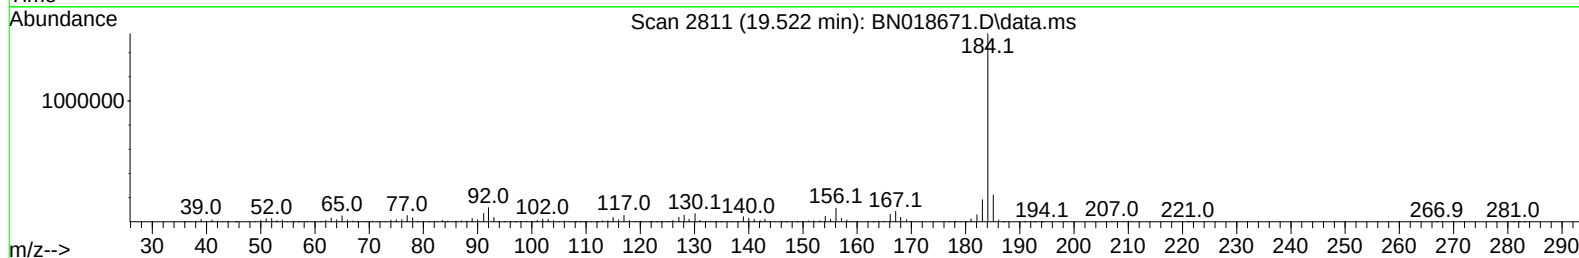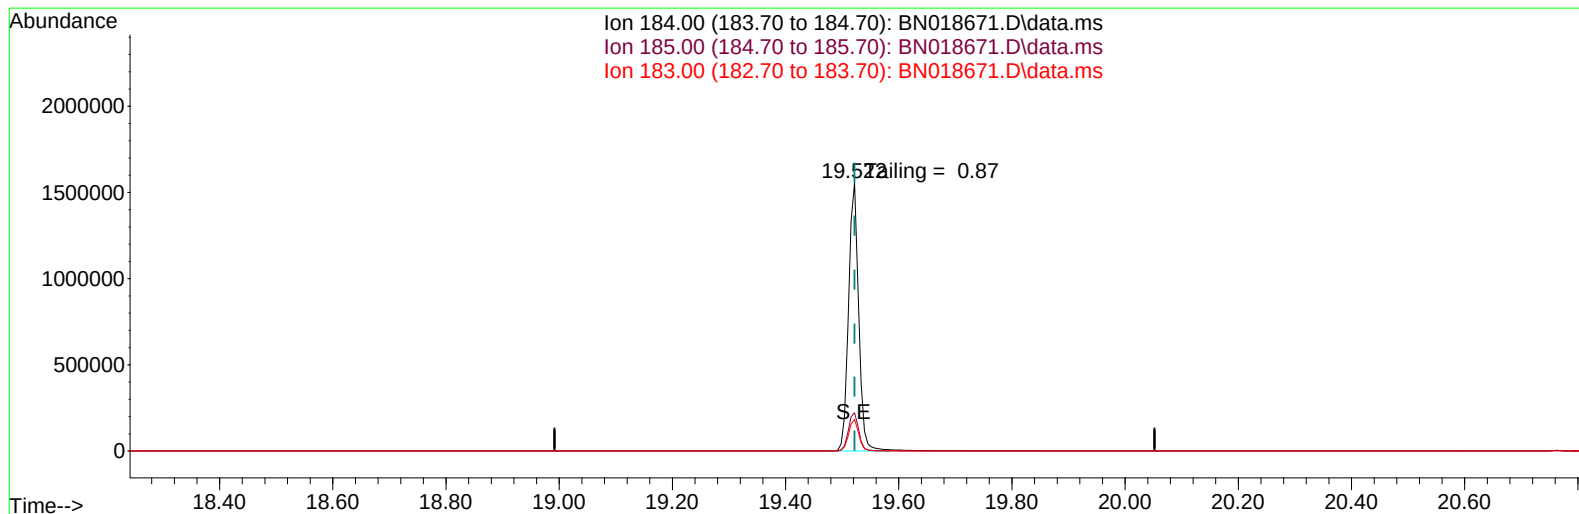

TIC: BN018671.D\data.ms

(77) Benzidine

19.522min (0.000) 0.00 ng

response 1951769

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/22/2022	BNA_N	<u>BN018671.D</u>
Compound Name	Response	Retention Time
DDT	1041667	20.76
DDD	11231	20.32
DDE	606	19.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11837	1053504	1.12

Instrument :
BNA_N
ClientSampleId :
DFTPP