

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022422\
 Data File : BN018720.D
 Acq On : 24 Feb 2022 22:31
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Feb 25 00:49:37 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 22 16:23:51 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.912	152	6509	0.400	ng	0.00
7) Naphthalene-d8	10.722	136	15425	0.400	ng	# 0.00
13) Acenaphthene-d10	14.538	164	7523	0.400	ng	-0.01
19) Phenanthrene-d10	17.287	188	14026	0.400	ng	0.00
29) Chrysene-d12	21.467	240	10895	0.400	ng	# 0.00
35) Perylene-d12	23.861	264	10237	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.464	112	5839	0.392	ng	0.00
5) Phenol-d6	7.067	99	6571	0.383	ng	0.00
8) Nitrobenzene-d5	9.067	82	4166	0.349	ng	0.00
11) 2-Methylnaphthalene-d10	12.306	152	8766	0.377	ng	0.00
14) 2,4,6-Tribromophenol	16.026	330	1038	0.353	ng	0.00
15) 2-Fluorobiphenyl	13.170	172	13449	0.377	ng	-0.01
27) Fluoranthene-d10	19.312	212	14388	0.378	ng	0.00
31) Terphenyl-d14	19.906	244	8467	0.358	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.319	88	3042	0.402	ng	# 60
3) n-Nitrosodimethylamine	3.644	42	3087	0.412	ng	# 87
6) bis(2-Chloroethyl)ether	7.327	93	6906	0.392	ng	98
9) Naphthalene	10.765	128	17158	0.385	ng	98
10) Hexachlorobutadiene	11.064	225	3997	0.373	ng	# 100
12) 2-Methylnaphthalene	12.378	142	11524	0.387	ng	97
16) Acenaphthylene	14.260	152	12378	0.347	ng	99
17) Acenaphthene	14.602	154	9076	0.368	ng	99
18) Fluorene	15.586	166	11023	0.372	ng	99
20) 4,6-Dinitro-2-methylph...	15.660	198	634	0.355	ng	100
21) 4-Bromophenyl-phenylether	16.477	248	3569	0.358	ng	95
22) Hexachlorobenzene	16.600	284	4531	0.363	ng	# 86
23) Atrazine	16.733	200	1772	0.322	ng	# 93
24) Pentachlorophenol	16.938	266	943	0.393	ng	97
25) Phenanthrene	17.328	178	17800	0.379	ng	100
26) Anthracene	17.410	178	14040	0.353	ng	100
28) Fluoranthene	19.341	202	18474	0.377	ng	# 97
30) Pyrene	19.704	202	18683	0.384	ng	100
32) Benzo(a)anthracene	21.449	228	14814	0.359	ng	99
33) Chrysene	21.503	228	17826	0.387	ng	99
34) Bis(2-ethylhexyl)phtha...	21.378	149	5648	0.336	ng	# 94
36) Indeno(1,2,3-cd)pyrene	26.346	276	20906	0.387	ng	# 88
37) Benzo(b)fluoranthene	23.130	252	17048	0.367	ng	# 91
38) Benzo(k)fluoranthene	23.176	252	17131	0.372	ng	# 93
39) Benzo(a)pyrene	23.755	252	13741	0.371	ng	# 84
40) Dibenzo(a,h)anthracene	26.360	278	16034	0.380	ng	# 91
41) Benzo(g,h,i)perylene	27.109	276	17151	0.371	ng	# 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022422\
Data File : BN018720.D
Acq On : 24 Feb 2022 22:31
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Quant Time: Feb 25 00:49:37 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 22 16:23:51 2022
Response via : Initial Calibration



Abundance Scan 670 (7.919 min): BN018674.D\data.ms (-66)





#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.912 min Scan# 6
Delta R.T. -0.007 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:152 Resp: 6509
Ion Ratio Lower Upper
152 100
150 159.3 121.7 182.5
115 61.0 43.8 65.8


Abundance Scan 669 (7.912 min): BN018720.D\data.ms



Abundance Scan 669 (7.912 min): BN018720.D\data.ms (-65)





Abundance Scan 34 (3.326 min): BN018674.D\data.ms (-28)




#2
1,4-Dioxane
Concen: 0.402 ng
RT: 3.319 min Scan# 33
Delta R.T. -0.007 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31


Tgt Ion: 88 Resp: 3042
Ion Ratio Lower Upper
88 100
43 31.6 69.7 104.5#
58 80.7 83.8 125.8#

Abundance Scan 33 (3.319 min): BN018720.D\data.ms



Abundance Scan 33 (3.319 min): BN018720.D\data.ms (-20)









#3
n-Nitrosodimethylamine
Concen: 0.412 ng
RT: 3.644 min Scan# 71
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 3087
Ion Ratio Lower Upper
42 100
74 119.6 108.6 163.0
44 9.1 5.8 8.8#



#4
2-Fluorophenol
Concen: 0.392 ng
RT: 5.464 min Scan# 330
Delta R.T. -0.007 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion: 112 Resp: 5839
Ion Ratio Lower Upper
112 100
64 59.5 48.0 72.0
63 31.5 25.3 37.9









#5
Phenol-d6
Concen: 0.383 ng
RT: 7.067 min Scan# 51
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion: 99 Resp: 6571




Ion	Ratio	Lower	Upper
99	100		
42	20.0	16.3	24.5
71	34.4	26.8	40.2




#6
bis(2-Chloroethyl)ether
Concen: 0.392 ng
RT: 7.327 min Scan# 588
Delta R.T. -0.007 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion: 93 Resp: 6906

Ion	Ratio	Lower	Upper
93	100		
63	79.0	61.7	92.5
95	32.9	26.2	39.4







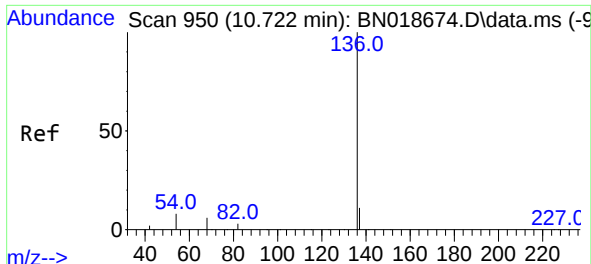

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.722 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	136	Resp:	15425
Ion	Ratio	Lower	Upper
136	100		
137	11.4	8.8	13.2
54	7.7	5.0	7.6#
68	6.0	4.4	6.6



#8
Nitrobenzene-d5
Concen: 0.349 ng
RT: 9.067 min Scan# 795
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion:	82	Resp:	4166
Ion	Ratio	Lower	Upper
82	100		
128	39.6	33.7	50.5
54	52.0	36.6	55.0









#9
Naphthalene
Concen: 0.385 ng
RT: 10.765 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	128	Resp:	17158
Ion	Ratio	Lower	Upper
128	100		
129	11.6	8.7	13.1
127	13.6	10.4	15.6

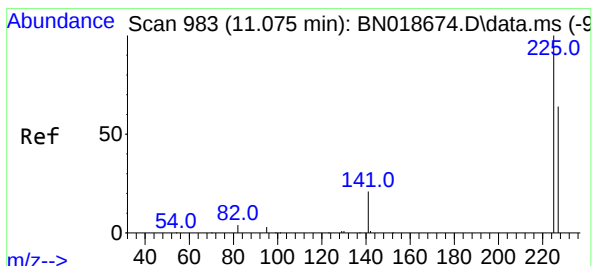

#10
Hexachlorobutadiene
Concen: 0.373 ng
RT: 11.064 min Scan# 982
Delta R.T. -0.011 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion:	225	Resp:	3997
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.9	51.0	76.6





#11

2-Methylnaphthalene-d10

Concen: 0.377 ng

RT: 12.306 min Scan# 11

Delta R.T. -0.004 min

Lab File: BN018720.D

Acq: 24 Feb 2022 22:31

Instrument :

BNA_N

ClientSampleId :





SSTDCCC0.4EC

Tgt Ion:152 Resp: 8766

Ion Ratio Lower Upper

152 100

151 21.0 16.2 24.2



#12

2-Methylnaphthalene

Concen: 0.387 ng

RT: 12.378 min Scan# 1253

Delta R.T. -0.004 min

Lab File: BN018720.D

Acq: 24 Feb 2022 22:31




Tgt Ion:142 Resp: 11524


Ion Ratio Lower Upper

142 100

141 88.9 70.0 105.0

115 37.8 27.8 41.8









#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.538 min Scan# 1478
 Delta R.T. -0.011 min
 Lab File: BN018720.D
 Acq: 24 Feb 2022 22:31




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:164 Resp: 7523
 Ion Ratio Lower Upper
 164 100
 162 106.6 80.2 120.2
 160 51.1 36.9 55.3



#14
 2,4,6-Tribromophenol
 Concen: 0.353 ng
 RT: 16.026 min Scan# 1617
 Delta R.T. 0.001 min
 Lab File: BN018720.D
 Acq: 24 Feb 2022 22:31

Tgt Ion:330 Resp: 1038
 Ion Ratio Lower Upper
 330 100
 332 95.7 0.0 0.0#
 141 37.6 21.3 31.9#









#15
2-Fluorobiphenyl
Concen: 0.377 ng
RT: 13.170 min Scan# 1349
Delta R.T. -0.011 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:172	Resp:	13449
Ion Ratio	Lower	Upper
172	100	
171	35.5	27.4 41.0
170	24.2	18.4 27.6



#16
Acenaphthylene
Concen: 0.347 ng
RT: 14.260 min Scan# 1451
Delta R.T. -0.011 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion:152	Resp:	12378
Ion Ratio	Lower	Upper
152	100	
151	19.7	15.8 23.6
153	12.5	10.5 15.7









#17
Acenaphthene
Concen: 0.368 ng
RT: 14.602 min Scan# 1483
Delta R.T. -0.011 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 9076
Ion Ratio Lower Upper
154 100
153 112.6 90.9 136.3
152 55.9 45.0 67.4



#18
Fluorene
Concen: 0.372 ng
RT: 15.586 min Scan# 1575
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion:166 Resp: 11023
Ion Ratio Lower Upper
166 100
165 98.7 77.8 116.6
167 13.8 10.9 16.3









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.287 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:188 Resp: 14026
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.7 7.0 10.4



#20
4,6-Dinitro-2-methylphenol
Concen: 0.355 ng
RT: 15.660 min Scan# 1582
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion:198 Resp: 634
Ion Ratio Lower Upper
198 100
182 19.4 15.5 23.3
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.358 ng
RT: 16.477 min Scan# 1661
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	248	Resp:	3569
Ion	Ratio	Lower	Upper
248	100		
250	100.1	74.4	111.6
141	54.2	43.7	65.5



#22
Hexachlorobenzene
Concen: 0.363 ng
RT: 16.600 min Scan# 1673
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion:	284	Resp:	4531
Ion	Ratio	Lower	Upper
284	100		
142	37.9	21.6	32.4
249	33.1	23.5	35.3









#23
 Atrazine
 Concen: 0.322 ng
 RT: 16.733 min Scan# 1686
 Delta R.T. 0.000 min
 Lab File: BN018720.D
 Acq: 24 Feb 2022 22:31




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:	200	Resp:	1772
Ion	Ratio	Lower	Upper
200	100		
173	30.5	20.3	30.5#
215	46.9	40.4	60.6



#24
 Pentachlorophenol
 Concen: 0.393 ng
 RT: 16.938 min Scan# 1706
 Delta R.T. 0.000 min
 Lab File: BN018720.D
 Acq: 24 Feb 2022 22:31

Tgt Ion:	266	Resp:	943
Ion	Ratio	Lower	Upper
266	100		
264	63.7	49.5	74.3
268	66.3	50.6	76.0









#25
Phenanthrene
Concen: 0.379 ng
RT: 17.328 min Scan# 1744
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:178 Resp: 17800
Ion Ratio Lower Upper
178 100
176 19.3 15.3 22.9
179 15.2 12.3 18.5



#26
Anthracene
Concen: 0.353 ng
RT: 17.410 min Scan# 1752
Delta R.T. -0.010 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion:178 Resp: 14040
Ion Ratio Lower Upper
178 100
176 18.6 14.8 22.2
179 15.5 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.378 ng
RT: 19.312 min Scan# 2120
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 14388
Ion Ratio Lower Upper
212 100
106 16.2 8.4 12.6#
104 9.1 4.5 6.7#



#28
Fluoranthene
Concen: 0.377 ng
RT: 19.341 min Scan# 2127
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion:202 Resp: 18474
Ion Ratio Lower Upper
202 100
101 12.0 7.2 10.8#
203 16.8 13.7 20.5









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.467 min Scan# 2448
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:240 Resp: 10895
Ion Ratio Lower Upper
240 100
120 10.8 6.0 9.0#
236 28.5 21.4 32.2



#30
Pyrene
Concen: 0.384 ng
RT: 19.704 min Scan# 2213
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion:202 Resp: 18683
Ion Ratio Lower Upper
202 100
200 20.9 16.6 25.0
203 17.9 14.1 21.1









#31
 Terphenyl-d14
 Concen: 0.358 ng
 RT: 19.906 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN018720.D
 Acq: 24 Feb 2022 22:31




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:244 Resp: 8467
 Ion Ratio Lower Upper
 244 100
 212 10.8 6.2 9.2#
 122 0.0 7.9 11.9#



#32
 Benzo(a)anthracene
 Concen: 0.359 ng
 RT: 21.449 min Scan# 2446
 Delta R.T. 0.000 min
 Lab File: BN018720.D
 Acq: 24 Feb 2022 22:31

Tgt Ion:228 Resp: 14814
 Ion Ratio Lower Upper
 228 100
 226 27.4 21.3 31.9
 229 19.8 15.9 23.9







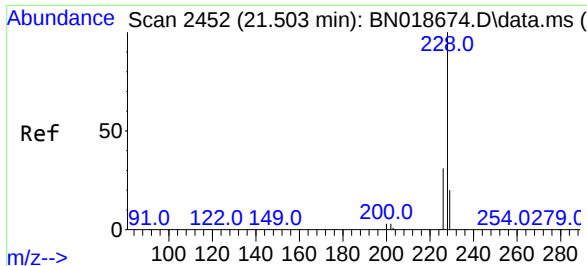

#33
Chrysene
Concen: 0.387 ng
RT: 21.503 min Scan# 2452
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:228	Resp:	17826
Ion Ratio	Lower	Upper
228	100	
226	29.8	24.2 36.4
229	20.1	15.5 23.3

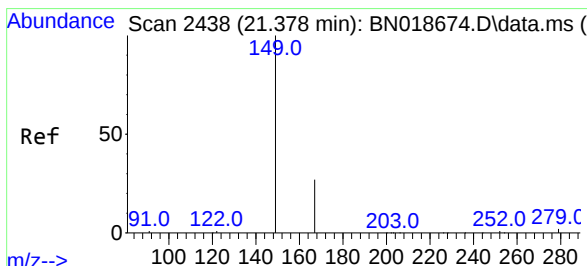

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.336 ng
RT: 21.378 min Scan# 2438
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31


Tgt Ion:149	Resp:	5648
Ion Ratio	Lower	Upper
149	100	
167	26.5	23.7 35.5
279	2.5	3.6 5.4








#35
Perylene-d12
Concen: 0.400 ng
RT: 23.861 min Scan# 3050
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:264 Resp: 10237
Ion Ratio Lower Upper
264 100
260 28.2 20.2 30.4
265 33.2 18.2 27.2#



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.387 ng
RT: 26.346 min Scan# 3900
Delta R.T. -0.006 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion:276 Resp: 20906
Ion Ratio Lower Upper
276 100
138 31.0 14.9 22.3#
277 24.7 19.9 29.9









#37
Benzo(b)fluoranthene
Concen: 0.367 ng
RT: 23.130 min Scan# 2800
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 17048
Ion Ratio Lower Upper
252 100
253 24.4 17.8 26.6
125 16.0 6.0 9.0#



#38
Benzo(k)fluoranthene
Concen: 0.372 ng
RT: 23.176 min Scan# 2816
Delta R.T. 0.000 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31


Tgt Ion:252 Resp: 17131
Ion Ratio Lower Upper
252 100
253 24.4 17.7 26.5
125 13.0 6.2 9.2#








#39
Benzo(a)pyrene
Concen: 0.371 ng
RT: 23.755 min Scan# 3013
Delta R.T. 0.003 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:252 Resp: 13741
Ion Ratio Lower Upper
252 100
253 25.8 17.8 26.6
125 22.5 7.0 10.4#



#40
Dibenzo(a,h)anthracene
Concen: 0.380 ng
RT: 26.360 min Scan# 3905
Delta R.T. -0.003 min
Lab File: BN018720.D
Acq: 24 Feb 2022 22:31

Tgt Ion:278 Resp: 16034
Ion Ratio Lower Upper
278 100
139 21.8 10.8 16.2#
279 25.2 19.0 28.4



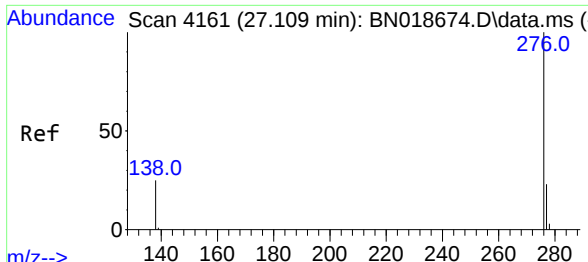

#41
 Benzo(g,h,i)perylene
 Concen: 0.371 ng
 RT: 27.109 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BN018720.D
 Acq: 24 Feb 2022 22:31

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:	276	Resp:	17151
Ion	Ratio	Lower	Upper
276	100		
277	24.4	19.0	28.6
138	27.4	12.6	19.0#

