
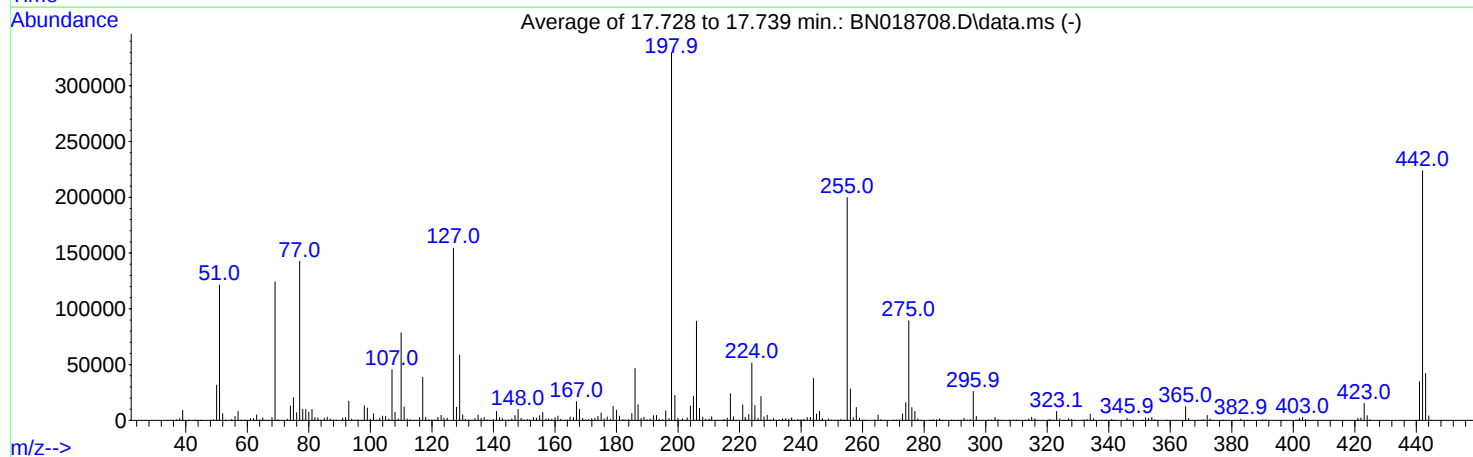


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022422\
 Data File : BN018708.D
 Acq On : 24 Feb 2022 14:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 22 16:23:51 2022

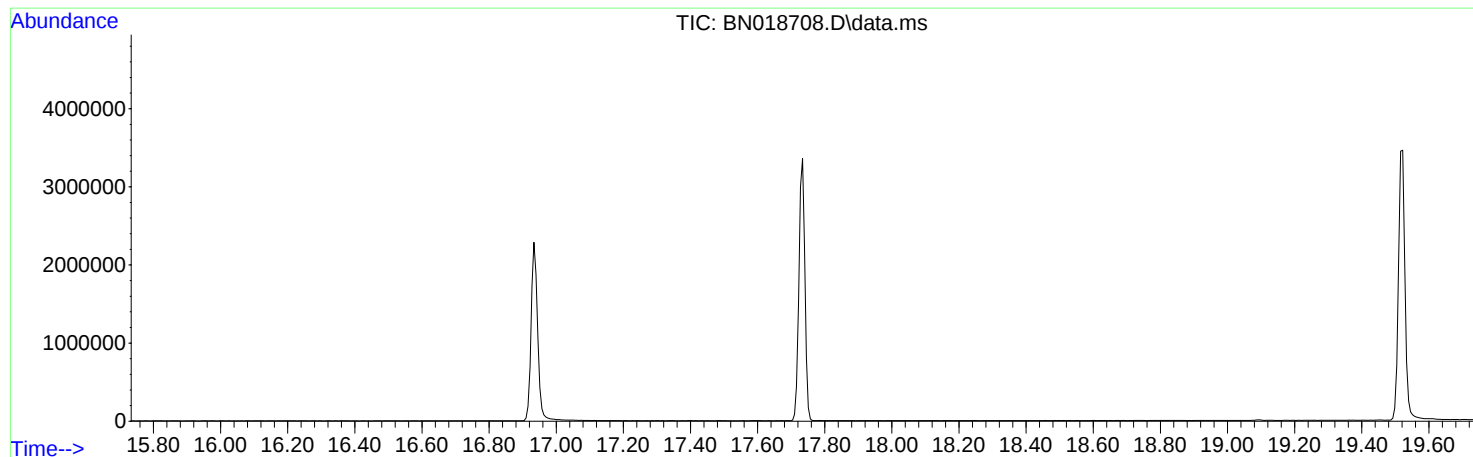




AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	121342	PASS
68	69	0.00	2	1.9	2397	PASS
69	198	0.00	100	37.7	124299	PASS
70	69	0.00	2	0.5	595	PASS
127	198	10	80	46.8	154424	PASS
197	198	0.00	2	0.5	1555	PASS
198	198	100	100	100.0	329835	PASS
199	198	5	9	6.8	22408	PASS
275	198	10	60	27.0	89187	PASS
365	198	1	100	3.7	12233	PASS
441	198	0.01	100	10.5	34760	PASS
442	442	50	100	100.0	223872	PASS
443	442	15	24	18.8	42072	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022422\
Data File : BN018708.D
Acq On : 24 Feb 2022 14:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 25 04:36:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 25 04:36:39 2022
Response via : Initial Calibration

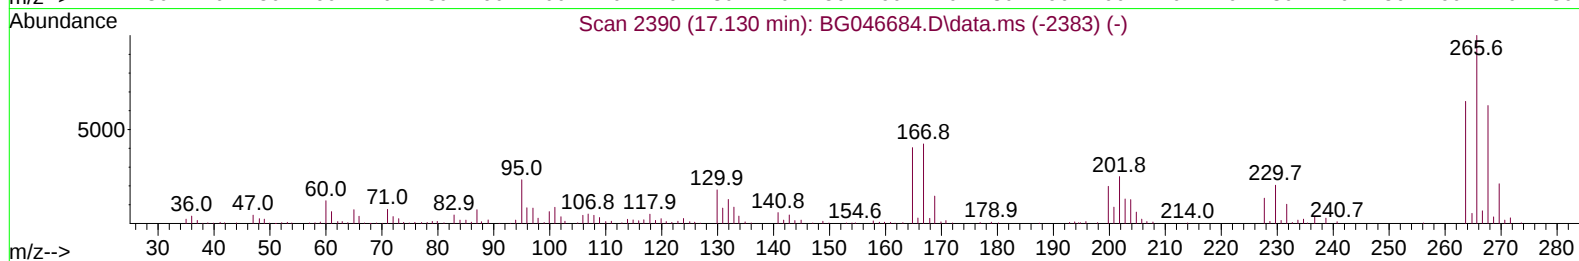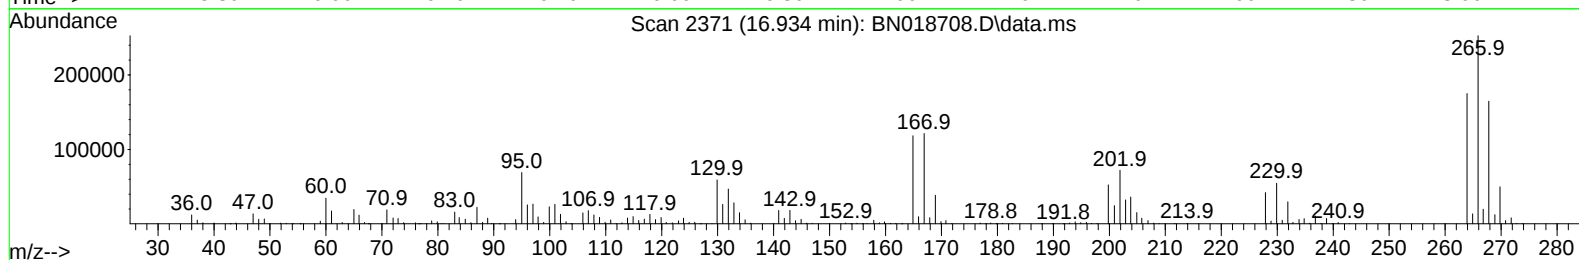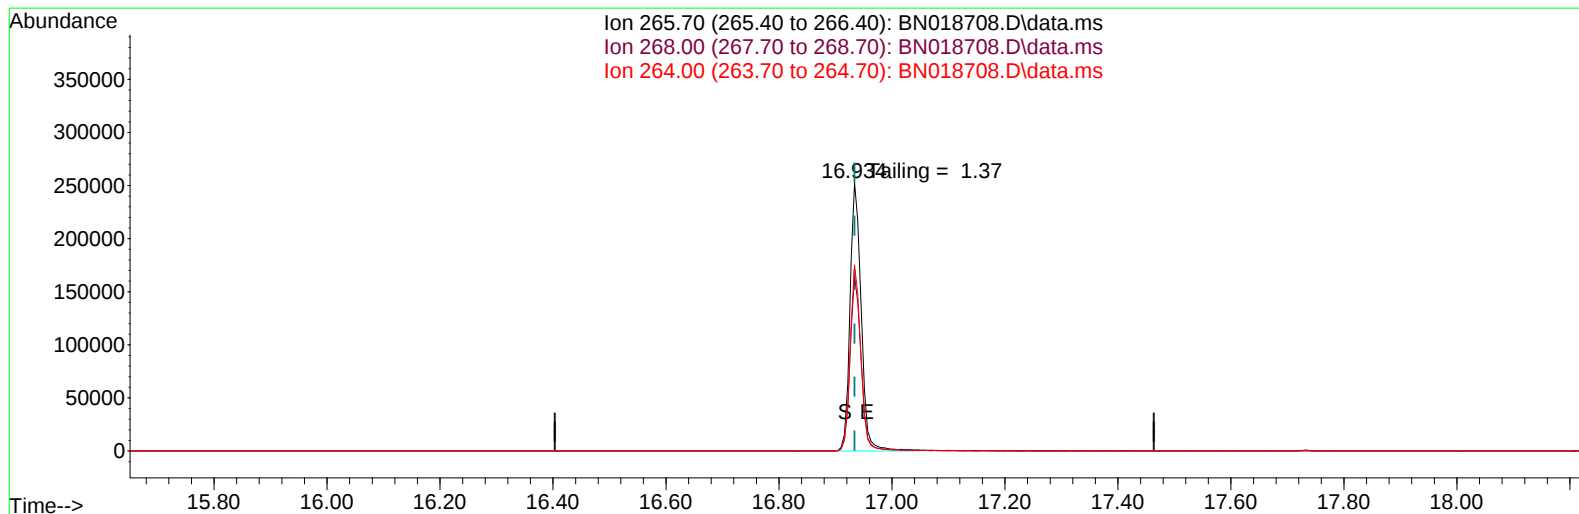

TIC: BN018708.D\data.ms

(70) Pentachlorophenol (C)

16.934min (0.000) 17848.82 ng




response 351023

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.26
264.00	61.60	69.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022422\
Data File : BN018708.D
Acq On : 24 Feb 2022 14:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 25 04:36:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 25 04:36:39 2022
Response via : Initial Calibration

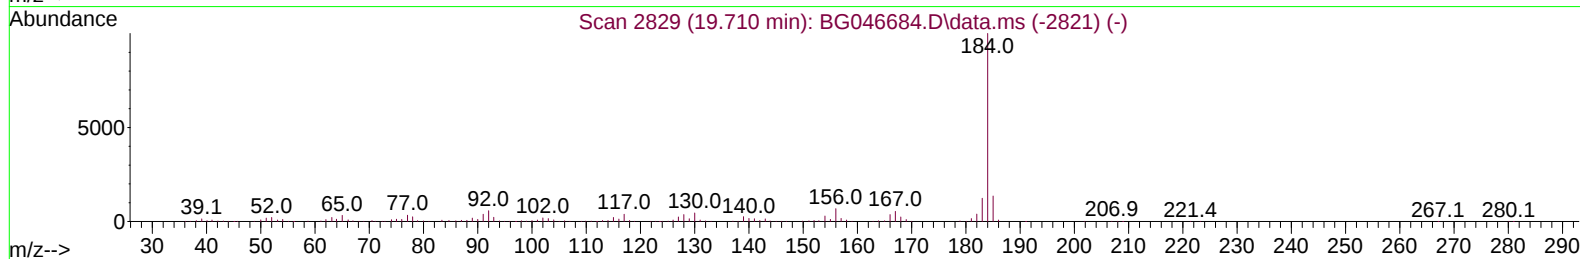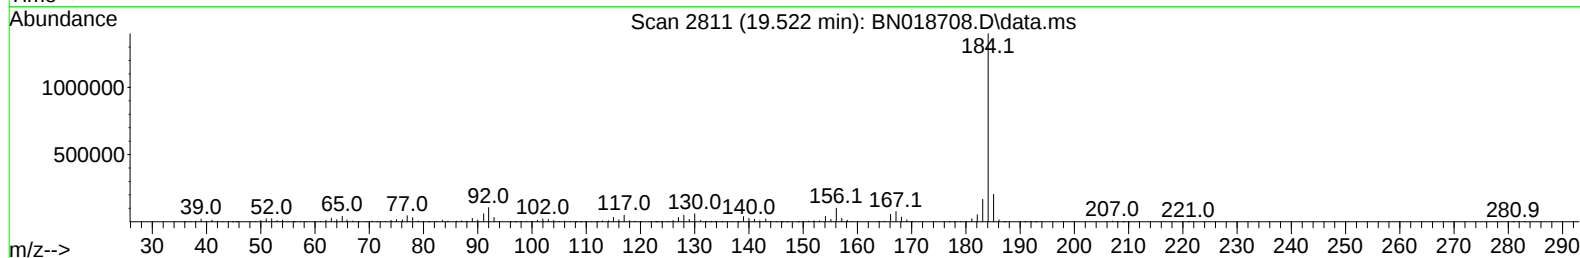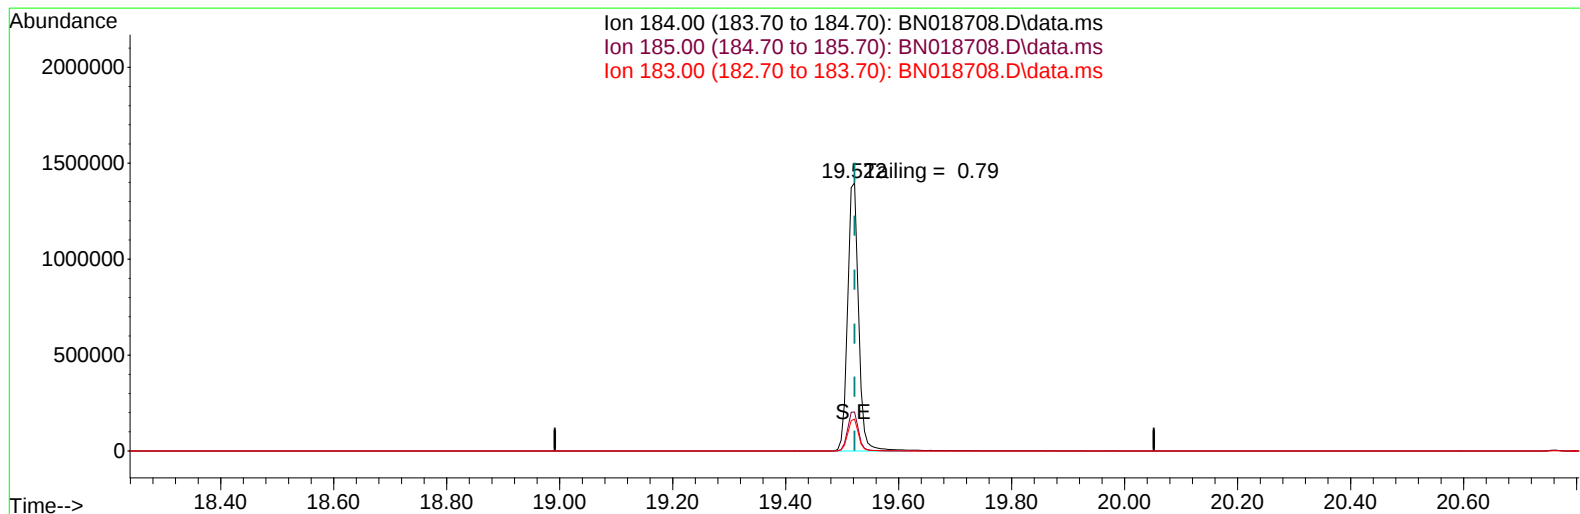

TIC: BN018708.D\data.ms

(77) Benzidine

19.522min (0.000) 0.00 ng

response 1903313

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.54
183.00	13.20	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/24/2022	BNA_N	<u>BN018708.D</u>
Compound Name	Response	Retention Time
DDT	1112160	20.763
DDD	30055	20.322
DDE	720	19.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30775	1142935	2.69

Instrument :
BNA_N
ClientSampleId :
DFTPP