

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024177.D
 Acq On : 08 Mar 2023 21:08
 Operator : CG/JU
 Sample : PB151198BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK198

Quant Time: Mar 09 03:51:49 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 03:48:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	9209	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	27687	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.694	164	15052	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.435	188	29305	0.400	ng/ul	0.00
17) Chrysene-d12	21.627	240	18488	0.400	ng/ul	0.00
23) Perylene-d12	24.147	264	16546	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	56666	5.591	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	10320	0.314	ng/ul	0.00
18) Fluoranthene-d10	19.460	212	19474	0.396	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.684	166	3492	0.065	ng/ul#	13
20) Pyrene	19.822	202	3119	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.980	252	5734	0.105	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024177.D
Acq On : 08 Mar 2023 21:08
Operator : CG/JU
Sample : PB151198BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK198

Quant Time: Mar 09 03:51:49 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 03:48:21 2023
Response via : Initial Calibration




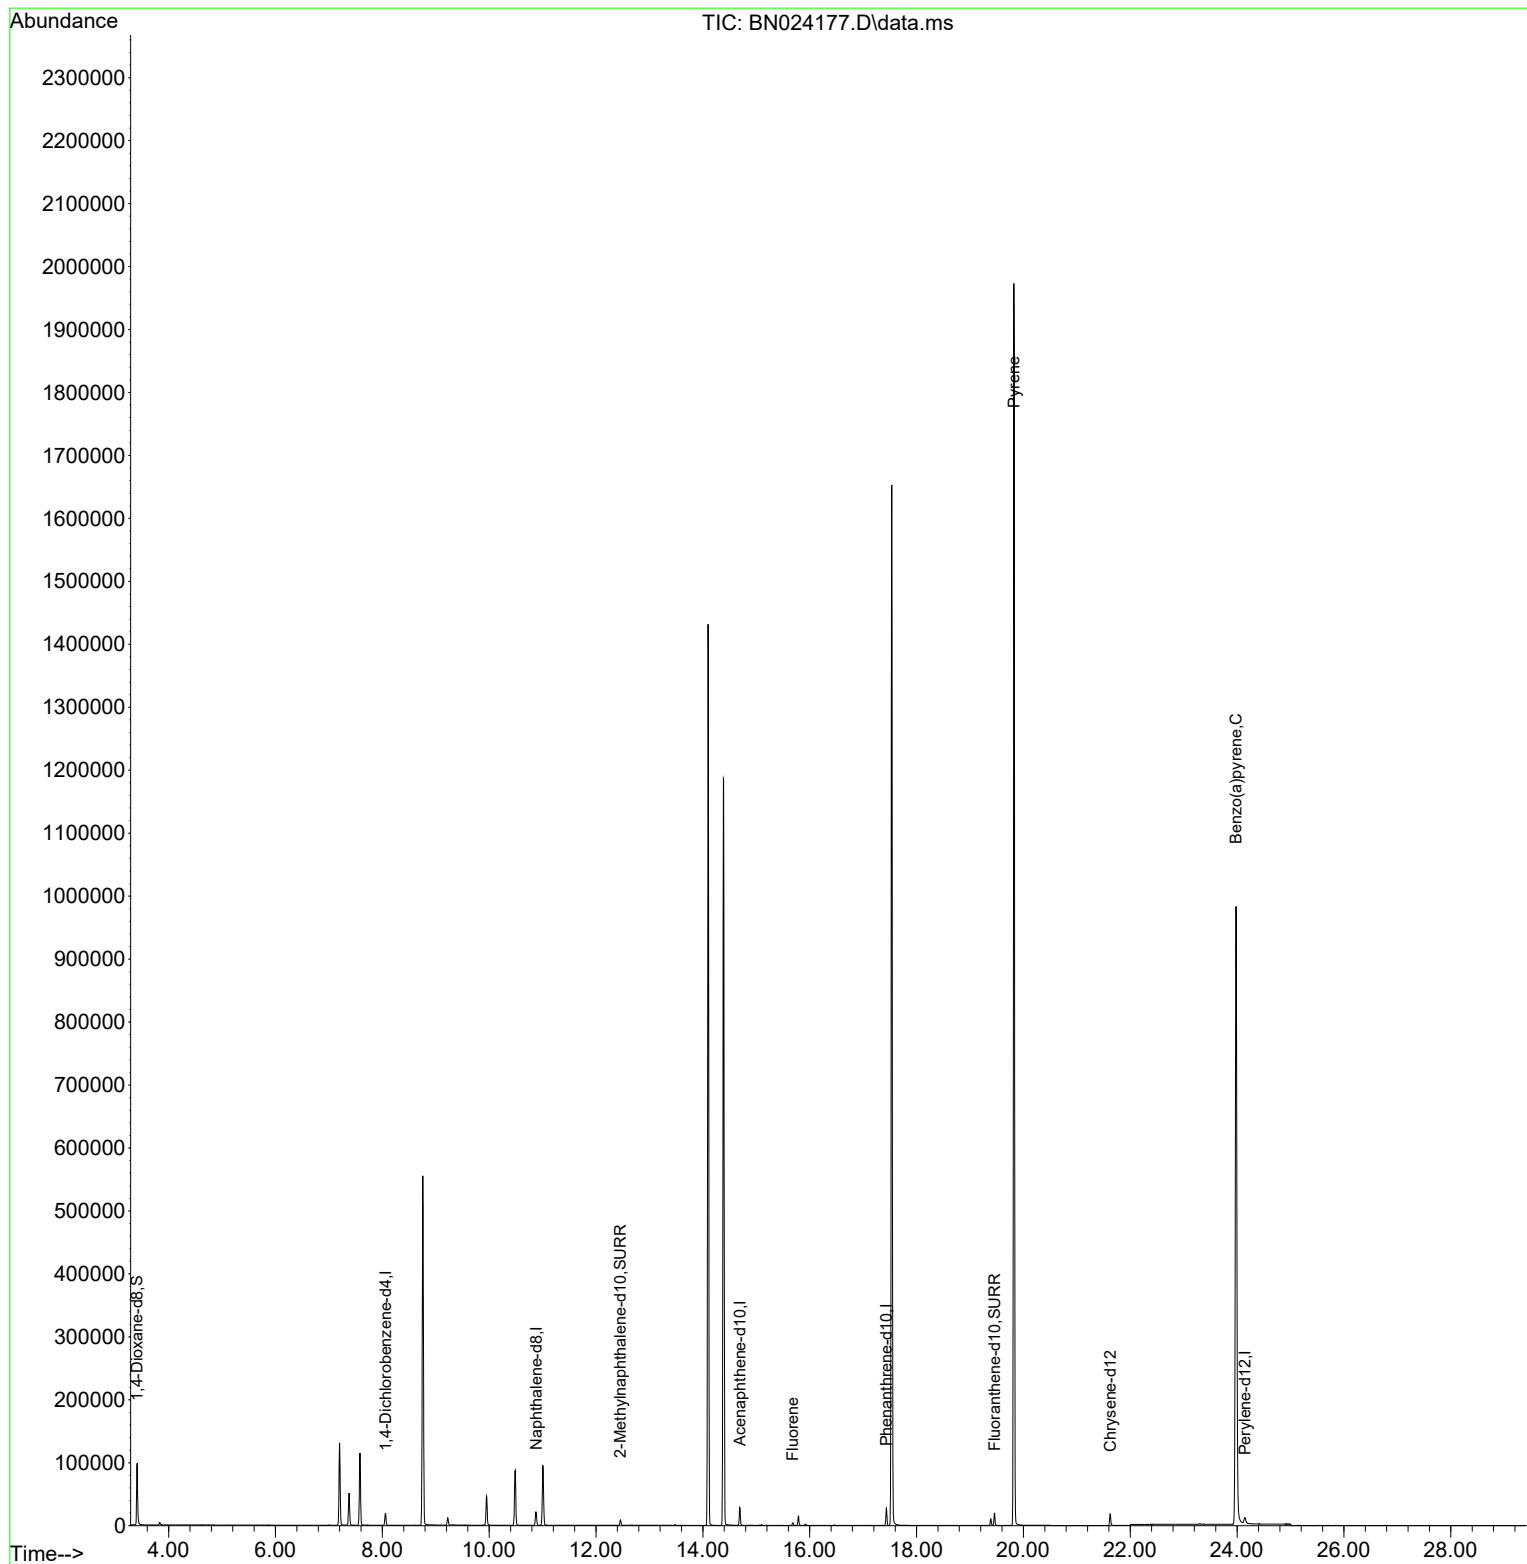


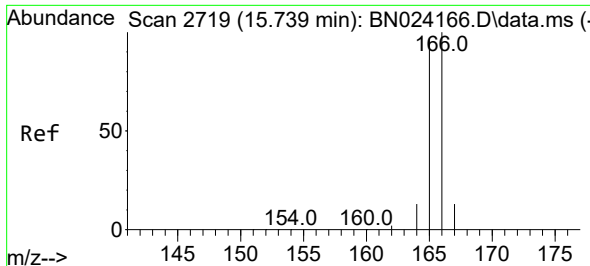

#12
Fluorene
Concen: 0.065 ng/ul
RT: 15.684 min Scan# 21
Delta R.T. -0.051 min
Lab File: BN024177.D
Acq: 08 Mar 2023 21:08




Instrument :
BNA_N
ClientSampleId :
SBLK198


Tgt Ion:166 Resp: 3492
Ion Ratio Lower Upper
166 100
165 6.4 77.4 116.0#
167 35.1 10.9 16.3#

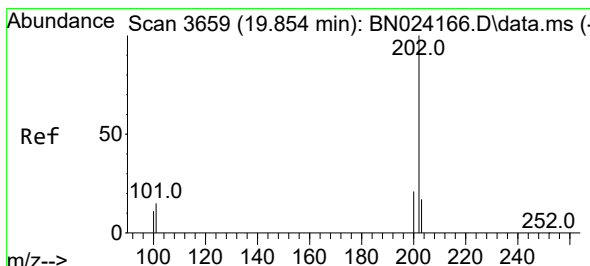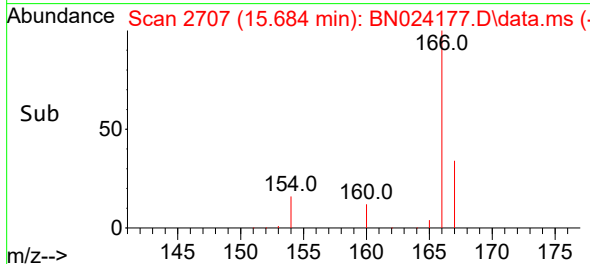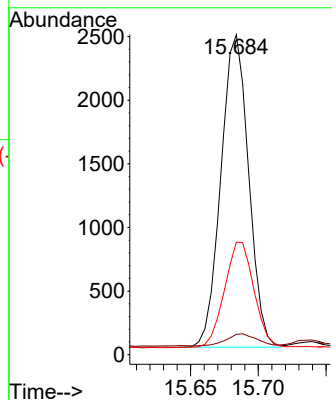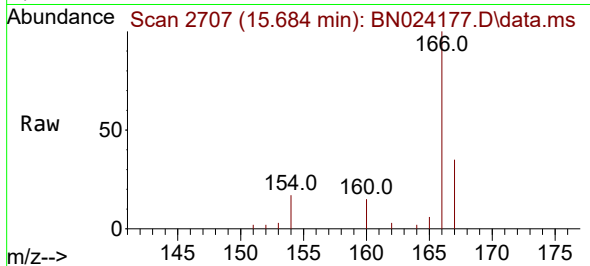

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.822 min Scan# 3652
Delta R.T. -0.028 min
Lab File: BN024177.D
Acq: 08 Mar 2023 21:08


Tgt Ion:202 Resp: 3119
Ion Ratio Lower Upper
202 100
101 173.9 12.1 18.1#
100 1323.3 9.4 14.0#

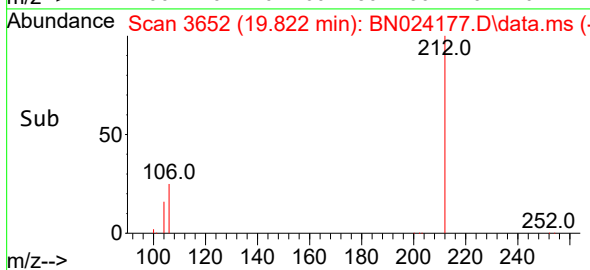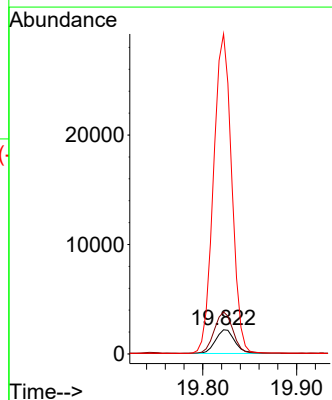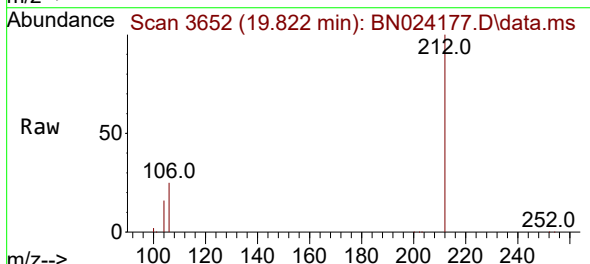

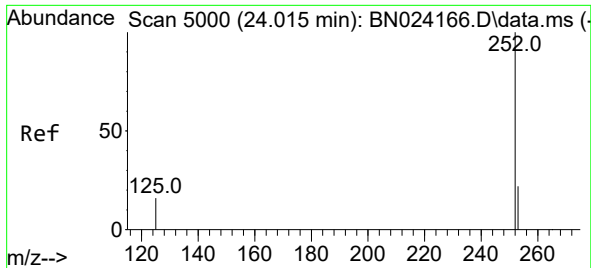

#26
Benzo(a)pyrene
Concen: 0.105 ng/ul
RT: 23.980 min Scan# 4988
Delta R.T. -0.047 min
Lab File: BN024177.D
Acq: 08 Mar 2023 21:08

Instrument :
BNA_N
ClientSampleId :
SBLK198

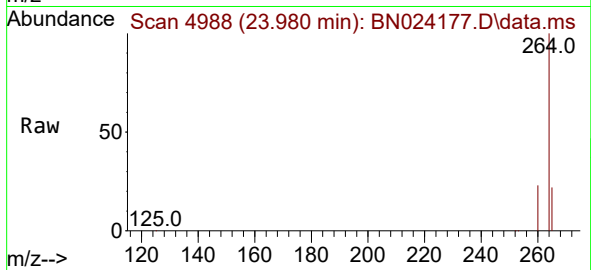

Tgt Ion:252 Resp: 5734
Ion Ratio Lower Upper
252 100
253 37.1 19.2 28.8#
125 36.6 15.8 23.6#

