

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024178.D
 Acq On : 08 Mar 2023 21:45
 Operator : CG/JU
 Sample : PB151200BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK200

Quant Time: Mar 09 03:51:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 03:48:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	12894	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	27929	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.694	164	11731	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	22512	0.400	ng/ul	0.00
17) Chrysene-d12	21.624	240	14576	0.400	ng/ul	0.00
23) Perylene-d12	24.144	264	14067	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	52439	3.696	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	9042	0.272	ng/ul	0.00
18) Fluoranthene-d10	19.459	212	16161	0.417	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.684	166	3164	0.075	ng/ul#	13
20) Pyrene	19.822	202	2762	0.047	ng/ul#	1
26) Benzo(a)pyrene	23.980	252	5672	0.123	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024178.D
Acq On : 08 Mar 2023 21:45
Operator : CG/JU
Sample : PB151200BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK200

Quant Time: Mar 09 03:51:55 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 03:48:21 2023
Response via : Initial Calibration




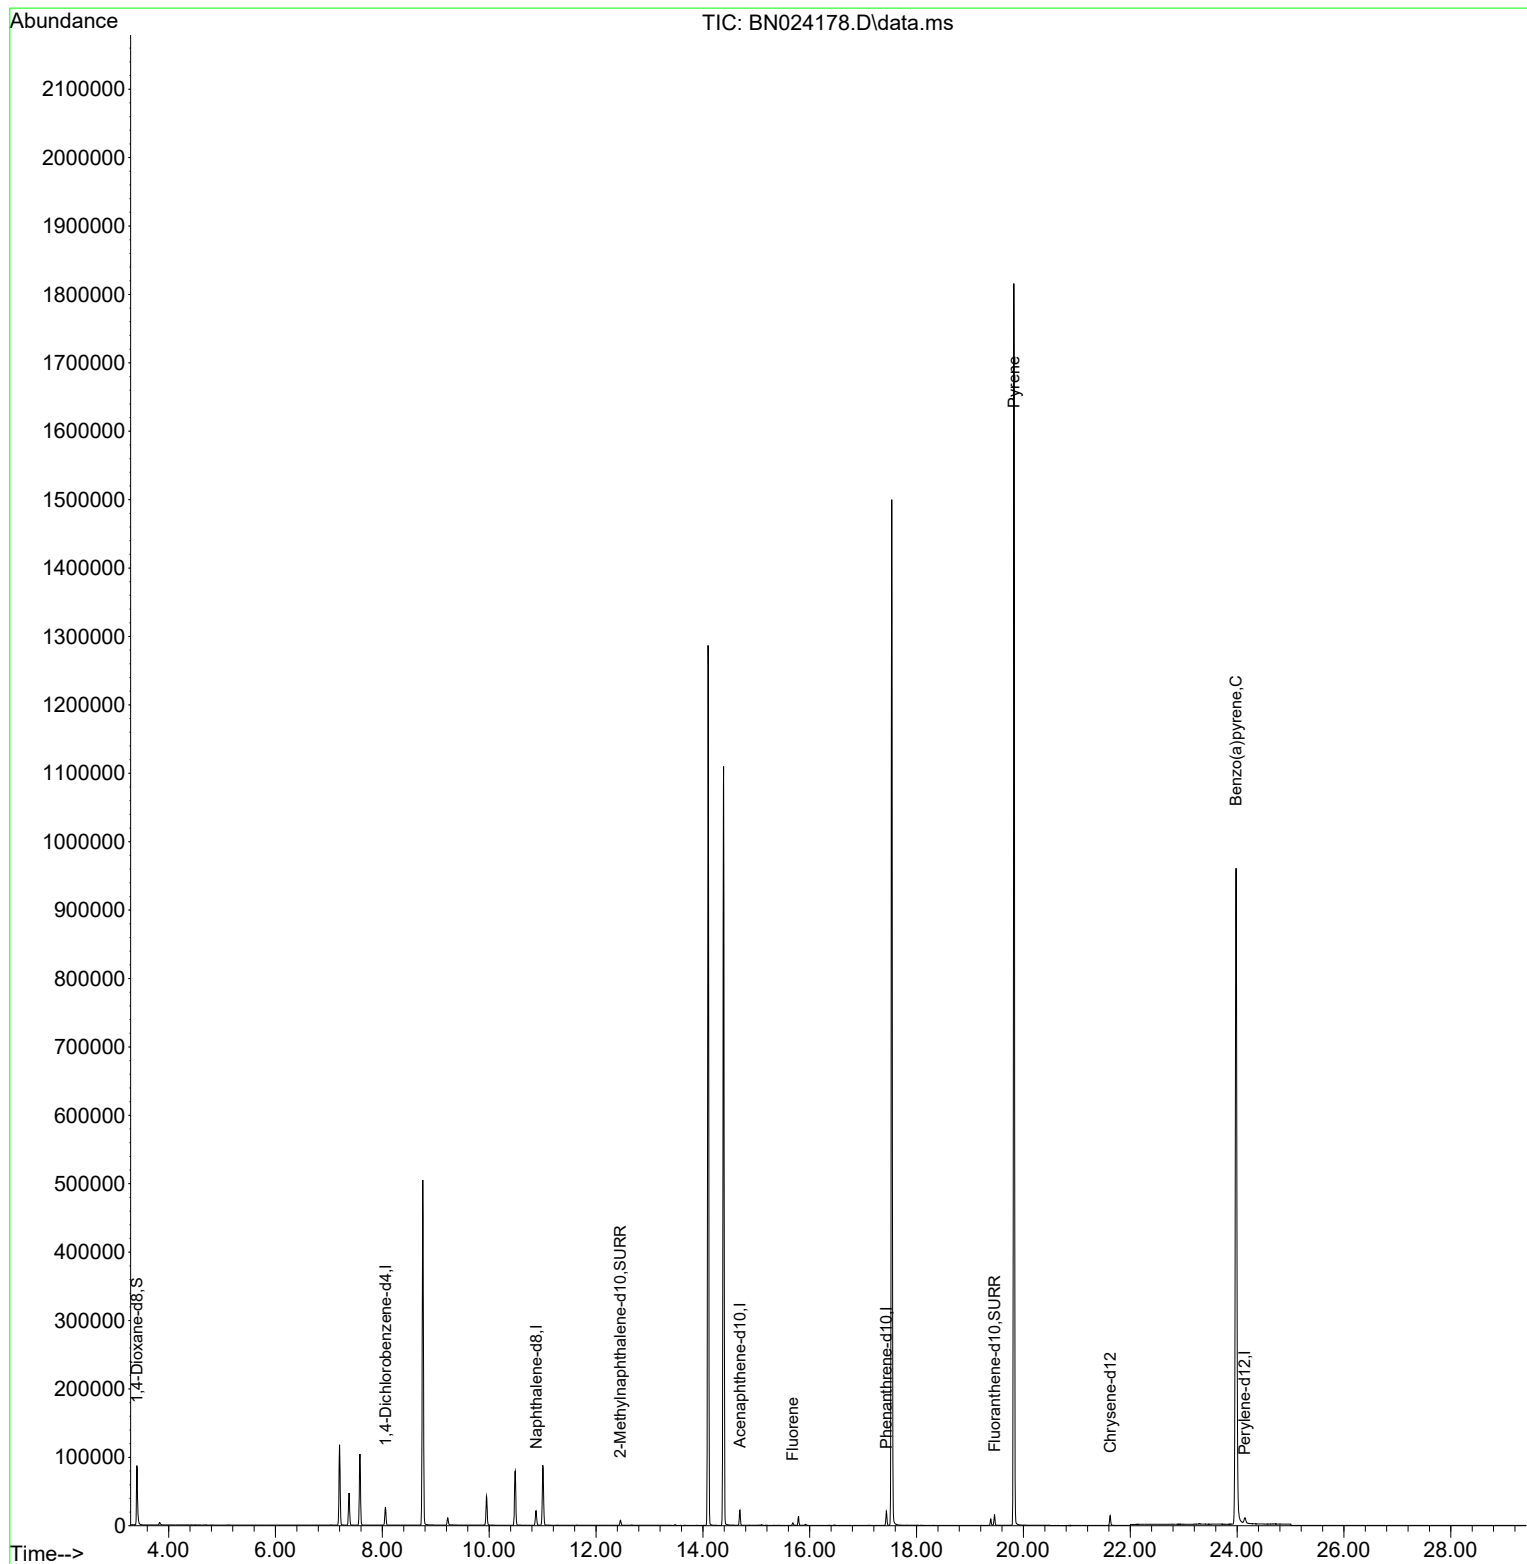


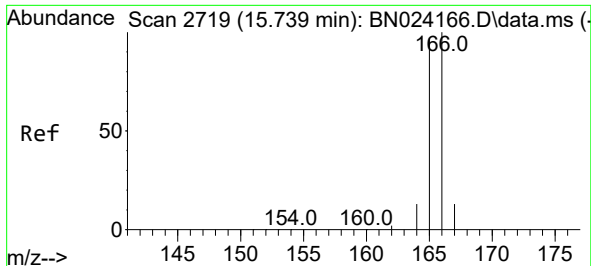

#12
Fluorene
Concen: 0.075 ng/ul
RT: 15.684 min Scan# 21
Delta R.T. -0.051 min
Lab File: BN024178.D
Acq: 08 Mar 2023 21:45




Instrument :
BNA_N
ClientSampleId :
SBLK200


Tgt Ion:166 Resp: 3164
Ion Ratio Lower Upper
166 100
165 6.2 77.4 116.0#
167 33.0 10.9 16.3#

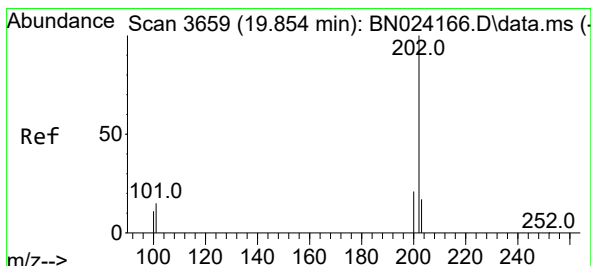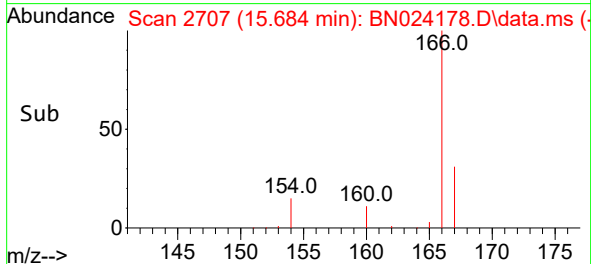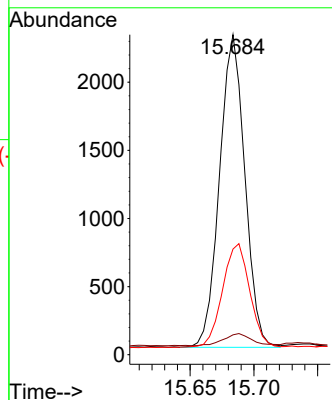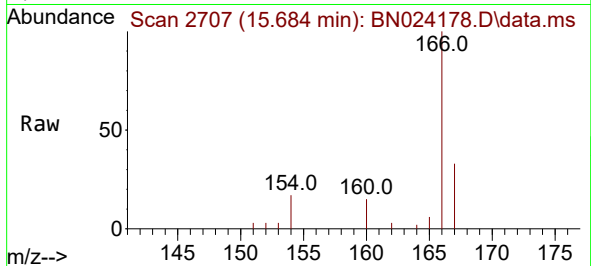

#20
Pyrene
Concen: 0.047 ng/ul
RT: 19.822 min Scan# 3652
Delta R.T. -0.028 min
Lab File: BN024178.D
Acq: 08 Mar 2023 21:45


Tgt Ion:202 Resp: 2762
Ion Ratio Lower Upper
202 100
101 173.8 12.1 18.1#
100 1295.8 9.4 14.0#

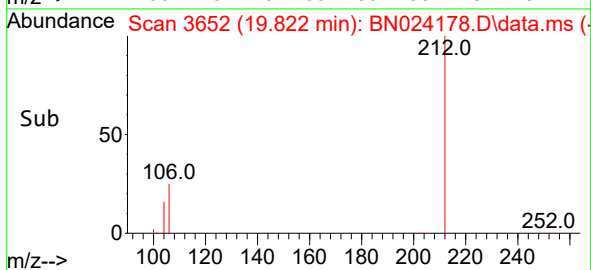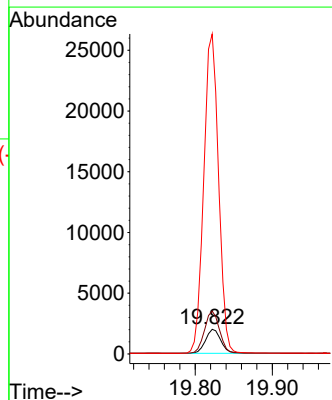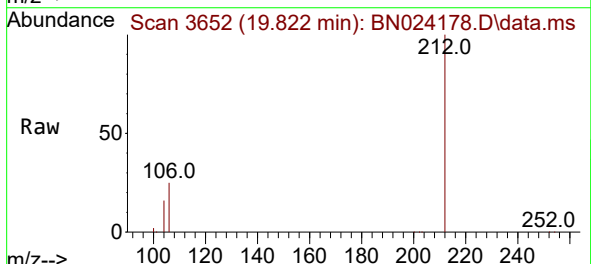

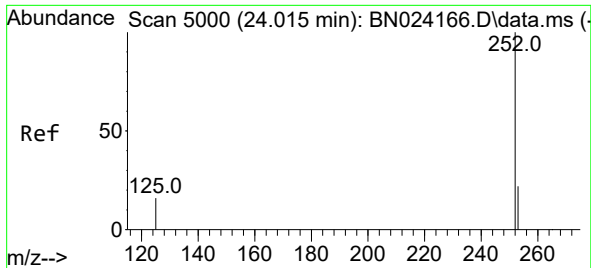

#26
Benzo(a)pyrene
Concen: 0.123 ng/ul
RT: 23.980 min Scan# 4988
Delta R.T. -0.047 min
Lab File: BN024178.D
Acq: 08 Mar 2023 21:45

Instrument :
BNA_N
ClientSampleId :
SBLK200

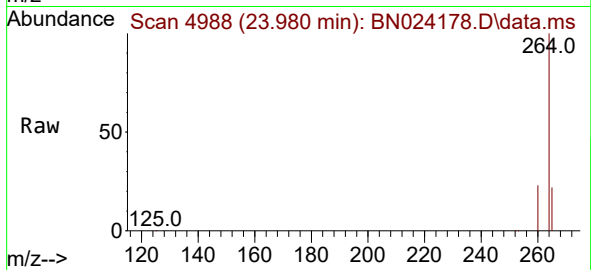

Tgt Ion:252 Resp: 5672
Ion Ratio Lower Upper
252 100
253 37.9 19.2 28.8#
125 38.4 15.8 23.6#

