

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024194.D
 Acq On : 09 Mar 2023 09:31
 Operator : CG/JU
 Sample : PB151238BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK238

Quant Time: Mar 10 02:23:37 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	9208	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	27578	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	14793	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	28902	0.400	ng/ul	0.00
17) Chrysene-d12	21.624	240	18119	0.400	ng/ul	0.00
23) Perylene-d12	24.126	264	17666	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.401	96	33845	3.340	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.450	152	5931	0.181	ng/ul	0.00
18) Fluoranthene-d10	19.459	212	10808	0.224	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.679	166	2107	0.040	ng/ul#	15
20) Pyrene	19.826	202	2037	0.028	ng/ul#	1
26) Benzo(a)pyrene	23.965	252	3830	0.066	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024194.D
Acq On : 09 Mar 2023 09:31
Operator : CG/JU
Sample : PB151238BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK238

Quant Time: Mar 10 02:23:37 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration




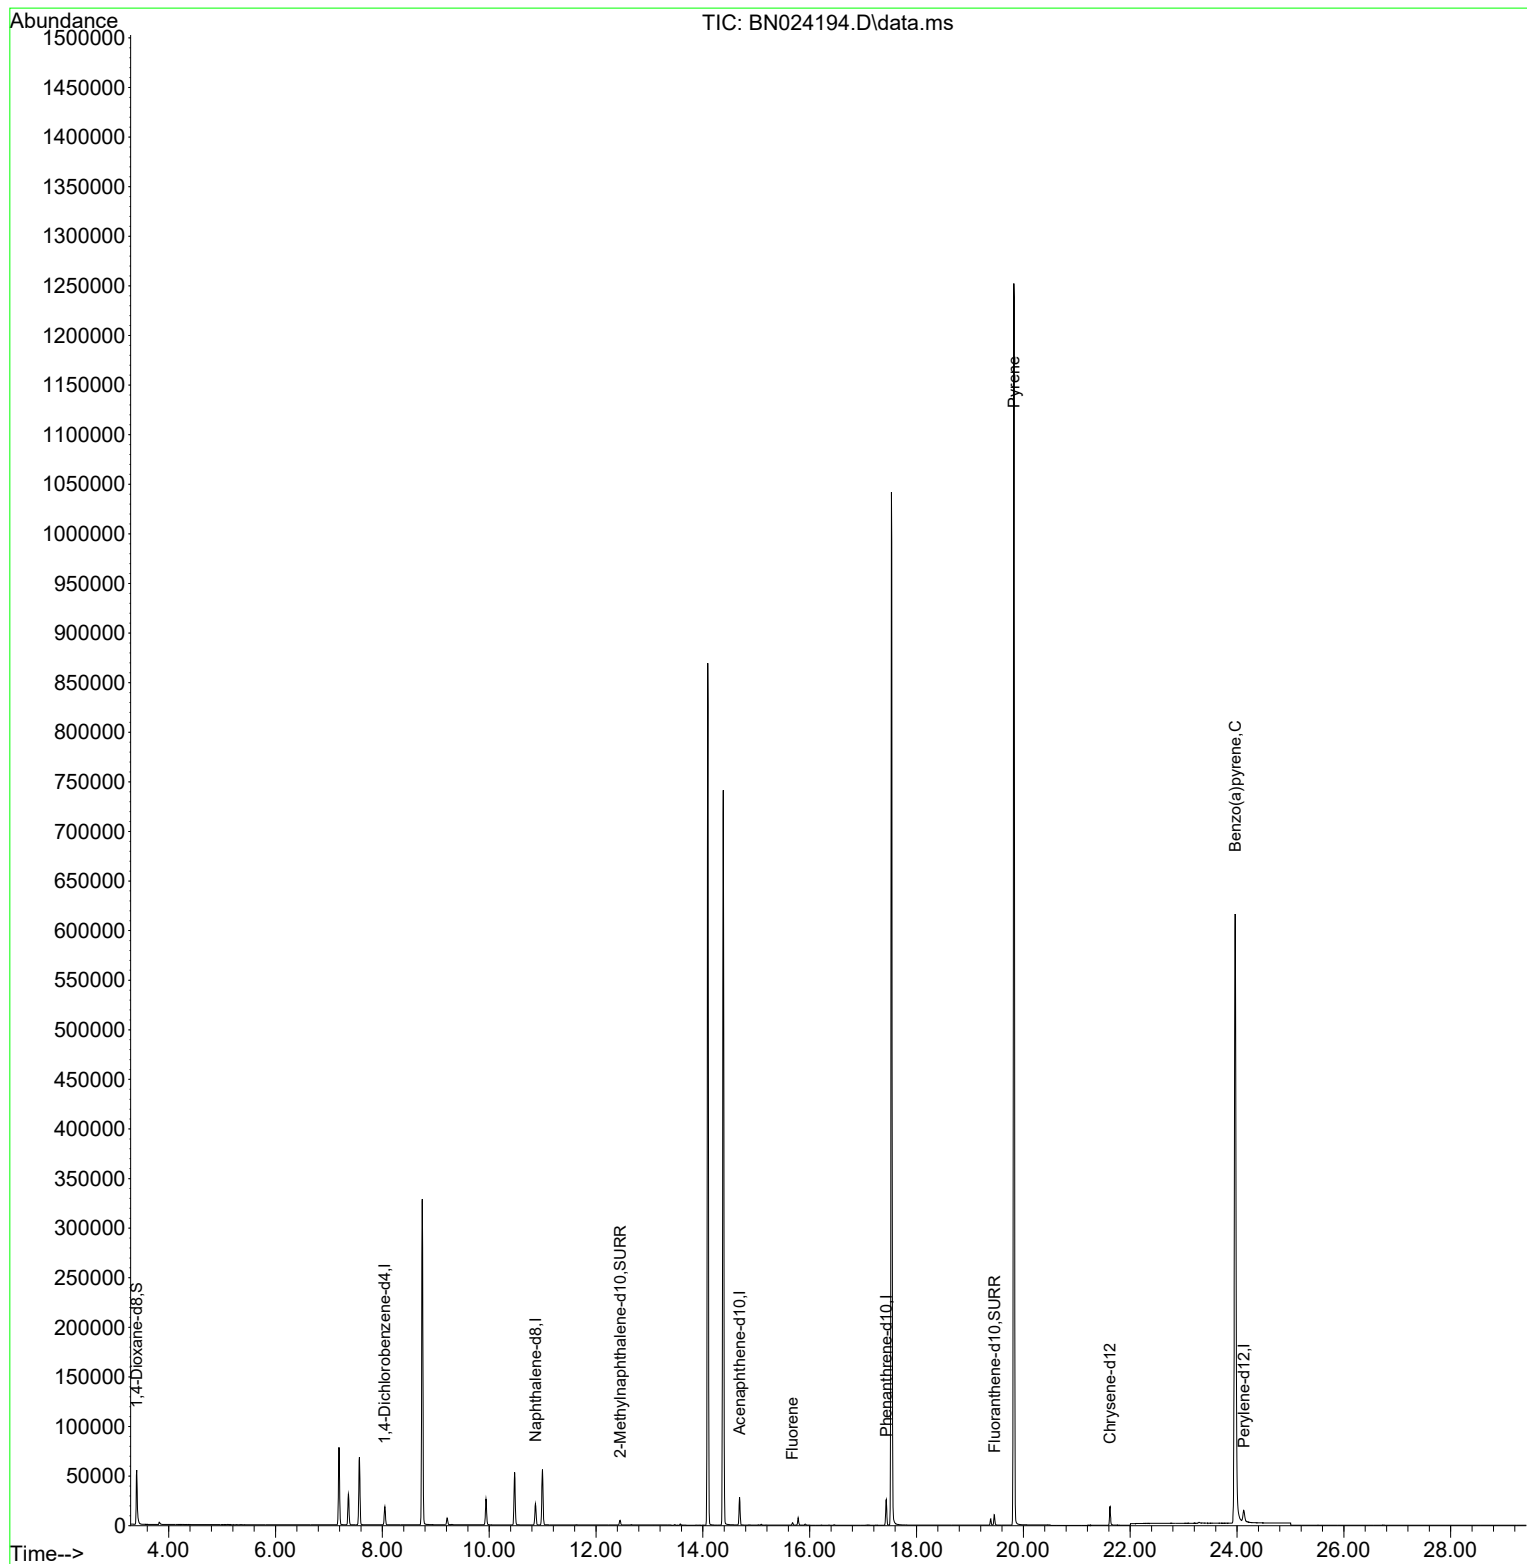


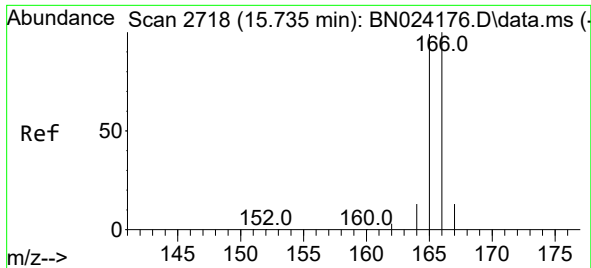

#12
Fluorene
Concen: 0.040 ng/ul
RT: 15.679 min Scan# 2107
Delta R.T. -0.056 min
Lab File: BN024194.D
Acq: 09 Mar 2023 09:31




Instrument :
BNA_N
ClientSampleId :
SBLK238


Tgt Ion:166 Resp: 2107
Ion Ratio Lower Upper
166 100
165 8.5 77.4 116.0#
167 34.1 10.9 16.3#

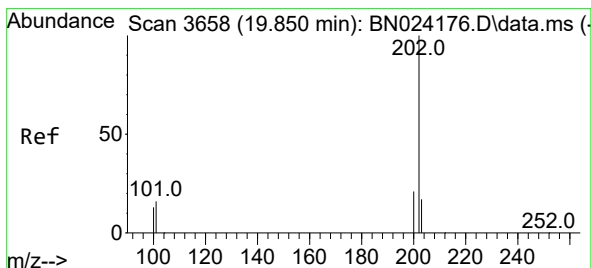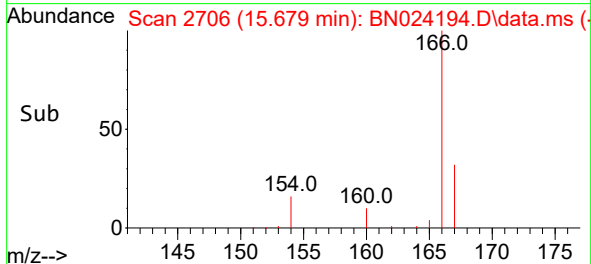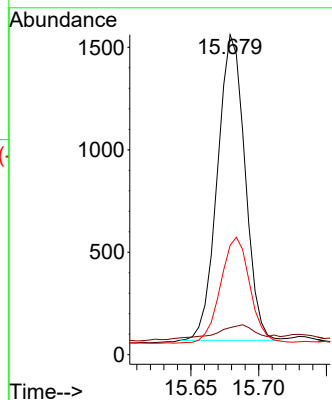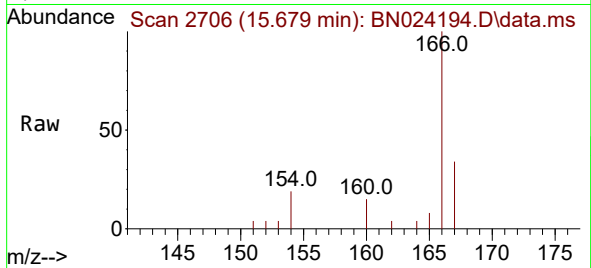

#20
Pyrene
Concen: 0.028 ng/ul
RT: 19.826 min Scan# 3653
Delta R.T. -0.019 min
Lab File: BN024194.D
Acq: 09 Mar 2023 09:31


Tgt Ion:202 Resp: 2037
Ion Ratio Lower Upper
202 100
101 163.4 12.1 18.1#
100 1144.0 9.4 14.0#

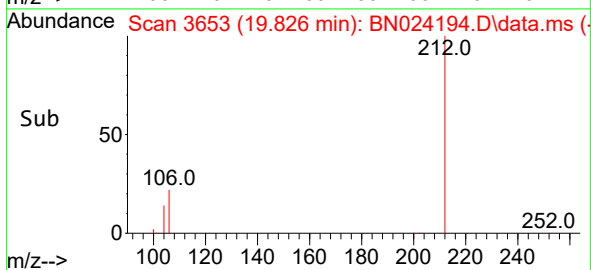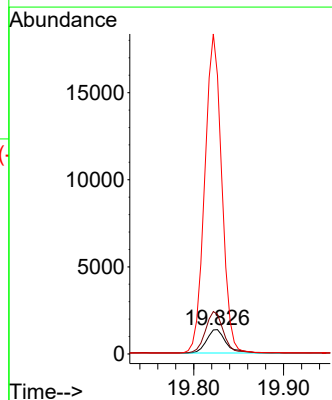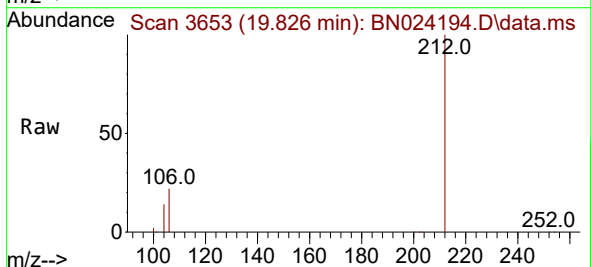

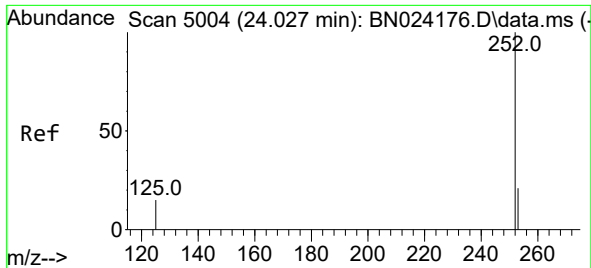

#26
Benzo(a)pyrene
Concen: 0.066 ng/ul
RT: 23.965 min Scan# 4983
Delta R.T. -0.038 min
Lab File: BN024194.D
Acq: 09 Mar 2023 09:31

Instrument :
BNA_N
ClientSampleId :
SBLK238

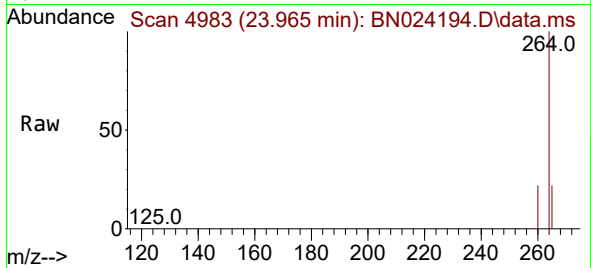

Tgt Ion:252 Resp: 3830
Ion Ratio Lower Upper
252 100
253 40.1 19.2 28.8#
125 43.4 15.8 23.6#

