

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024196.D
 Acq On : 09 Mar 2023 11:47
 Operator : CG/JU
 Sample : 01729-14
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BY9

Quant Time: Mar 10 02:23:44 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.050	152	9811	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	30191	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.684	164	16481	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188	33944	0.400	ng/ul	0.00
17) Chrysene-d12	21.621	240	23615	0.400	ng/ul	0.00
23) Perylene-d12	24.149	264	14887	0.400	ng/ul	0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	42824	3.966	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.450	152	9249	0.258	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	22520	0.358	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.443	88	250	0.021	ng/ul#	56
20) Pyrene	19.822	202	3812	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.980	252	6447	0.132	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024196.D
Acq On : 09 Mar 2023 11:47
Operator : CG/JU
Sample : 01729-14
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BY9

Quant Time: Mar 10 02:23:44 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration




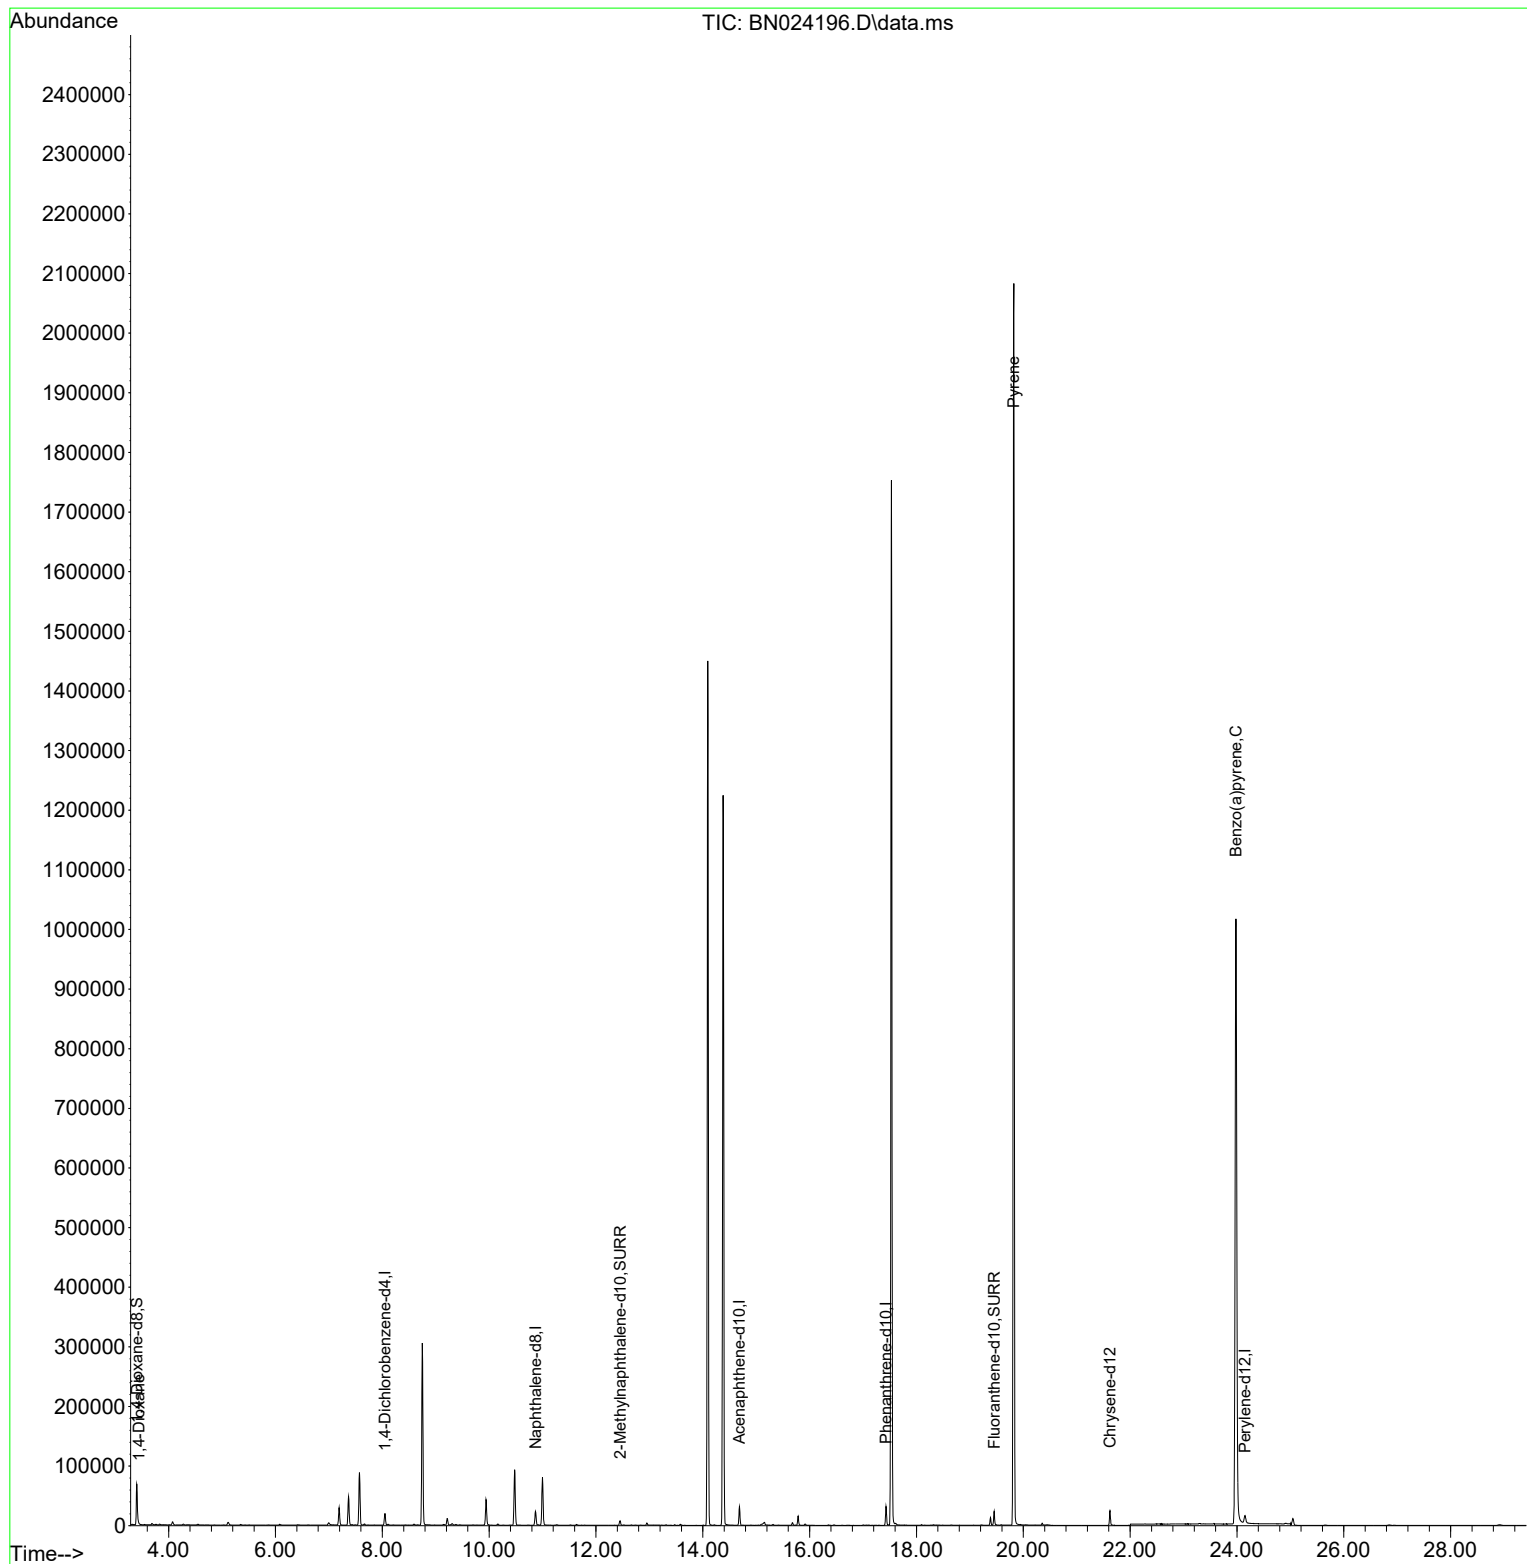


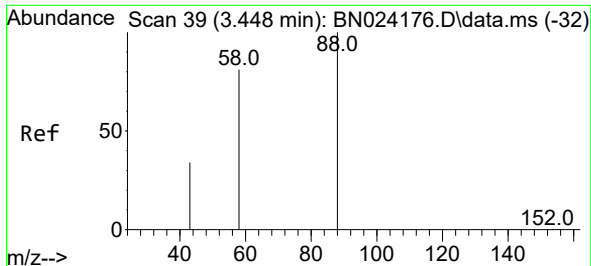

#2
1,4-Dioxane
Concen: 0.021 ng/ul
RT: 3.443 min Scan# 31
Delta R.T. -0.004 min
Lab File: BN024196.D
Acq: 09 Mar 2023 11:47




Instrument :
BNA_N
ClientSampleId :
C0BY9


Tgt Ion: 88 Resp: 250
Ion Ratio Lower Upper
88 100
43 80.4 32.1 48.1#
58 43.2 55.1 82.7#

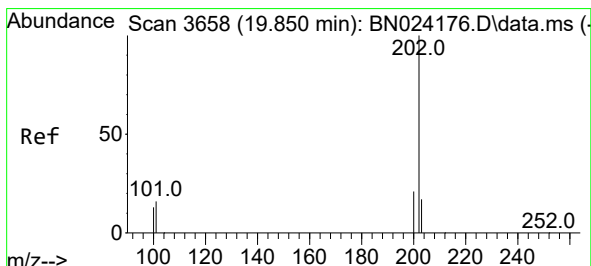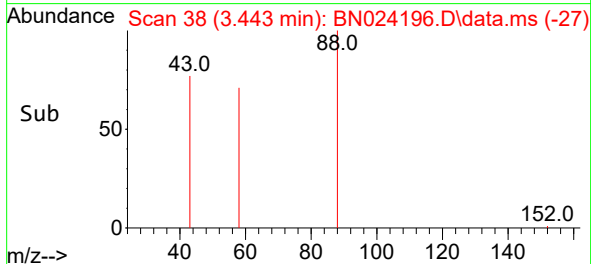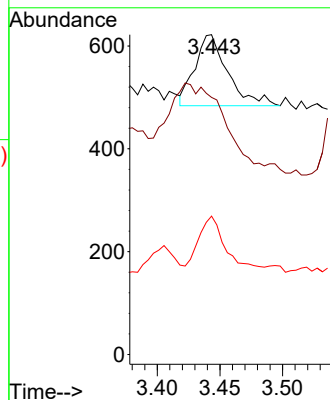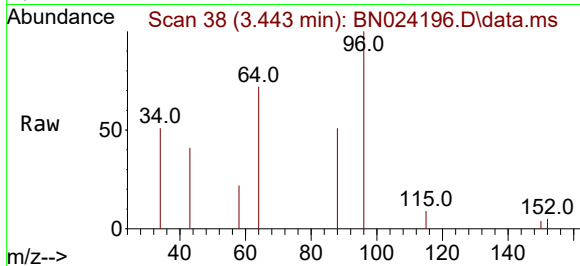

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.822 min Scan# 3652
Delta R.T. -0.023 min
Lab File: BN024196.D
Acq: 09 Mar 2023 11:47


Tgt Ion: 202 Resp: 3812
Ion Ratio Lower Upper
202 100
101 166.4 12.1 18.1#
100 1187.9 9.4 14.0#

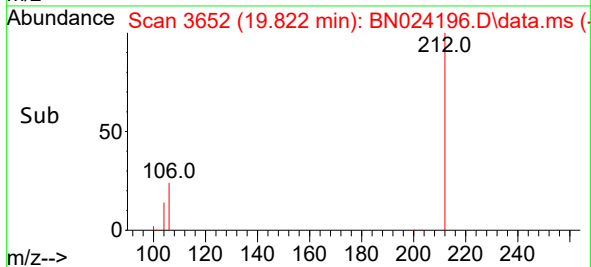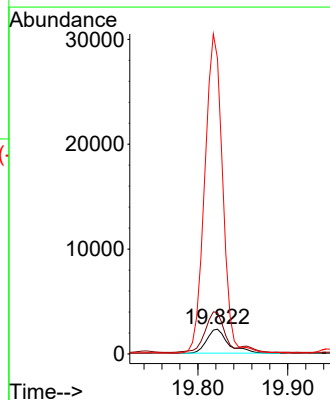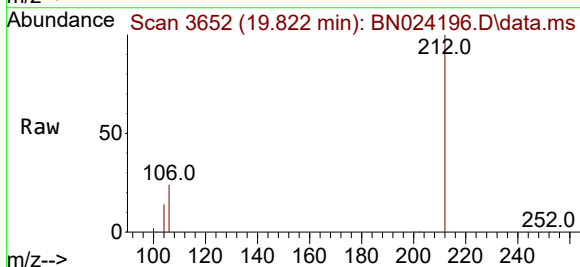

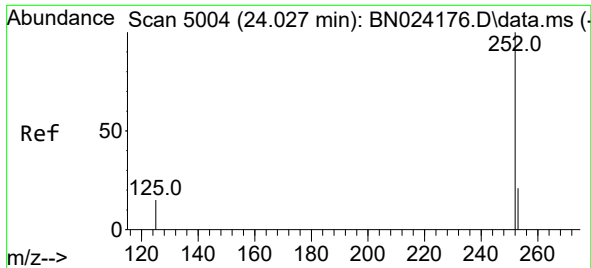

#26
Benzo(a)pyrene
Concen: 0.132 ng/ul
RT: 23.980 min Scan# 4988
Delta R.T. -0.023 min
Lab File: BN024196.D
Acq: 09 Mar 2023 11:47

Instrument :
BNA_N
ClientSampleId :
C0BY9

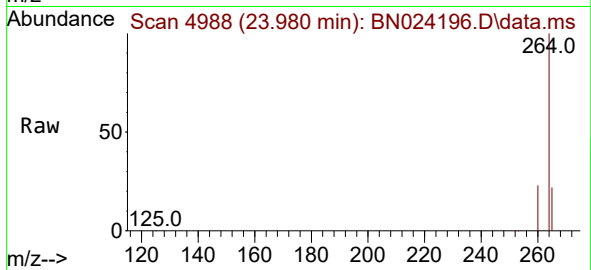

Tgt Ion:252 Resp: 6447
Ion Ratio Lower Upper
252 100
253 39.2 19.2 28.8#
125 43.2 15.8 23.6#

