

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024201.D
 Acq On : 09 Mar 2023 15:58
 Operator : CG/JU
 Sample : PB151255BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK255

Quant Time: Mar 10 02:24:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	8711	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	26420	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	14242	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188	27572	0.400	ng/ul	0.00
17) Chrysene-d12	21.621	240	17401	0.400	ng/ul	0.00
23) Perylene-d12	24.123	264	15950	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	33386	3.483	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	6035	0.192	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	10903	0.235	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.822	202	1935	0.028	ng/ul#	1
26) Benzo(a)pyrene	23.962	252	3412	0.065	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024201.D
Acq On : 09 Mar 2023 15:58
Operator : CG/JU
Sample : PB151255BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK255

Quant Time: Mar 10 02:24:25 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration




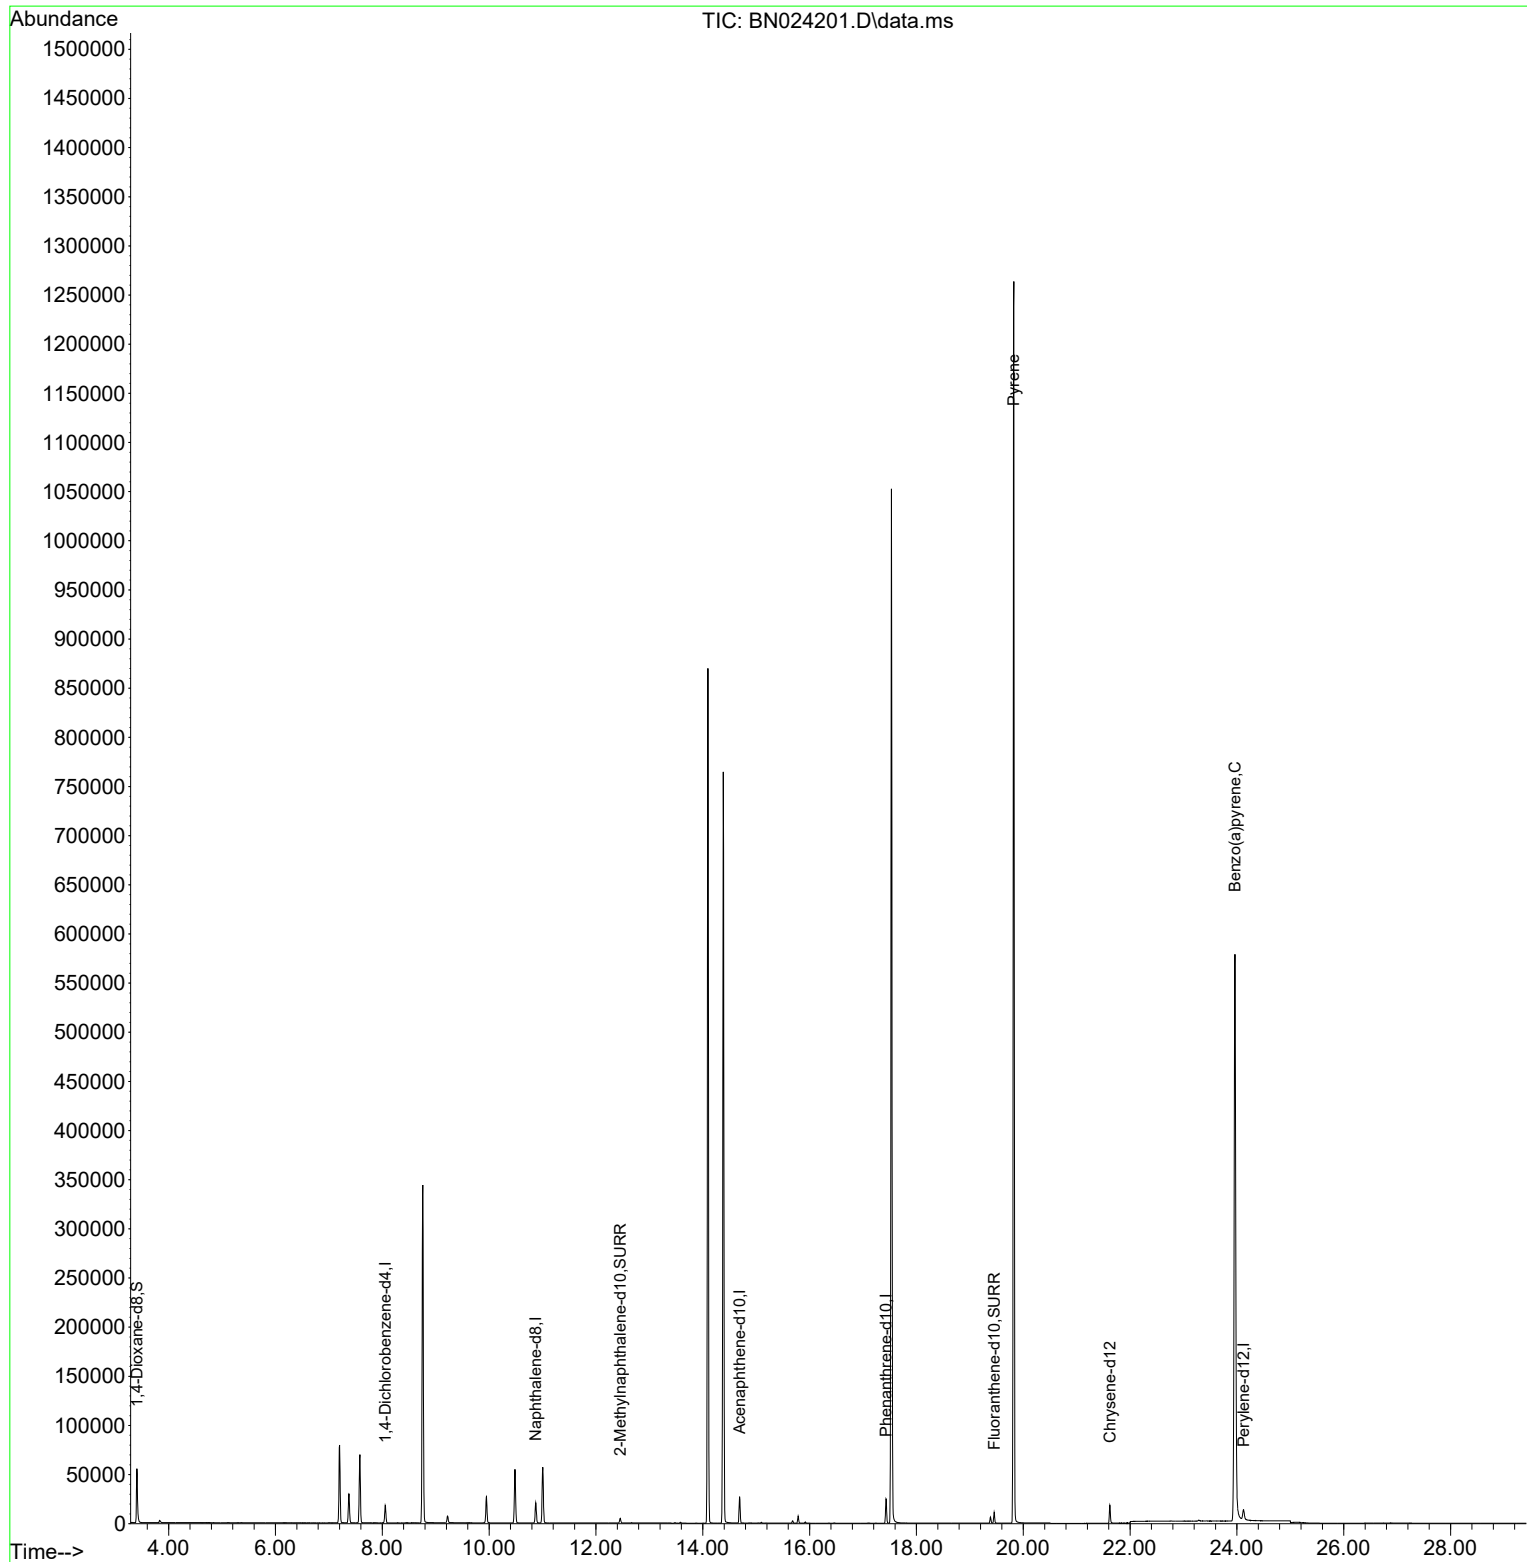


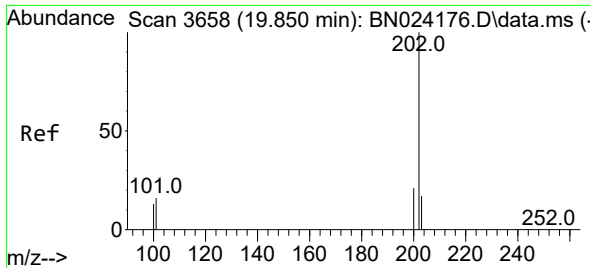

#20
Pyrene
Concen: 0.028 ng/ul
RT: 19.822 min Scan# 30
Delta R.T. -0.023 min
Lab File: BN024201.D
Acq: 09 Mar 2023 15:58

Instrument :
BNA_N
ClientSampleId :
SBLK255

Tgt Ion:202 Resp: 1935
Ion Ratio Lower Upper
202 100
101 158.2 12.1 18.1#
100 1103.3 9.4 14.0#

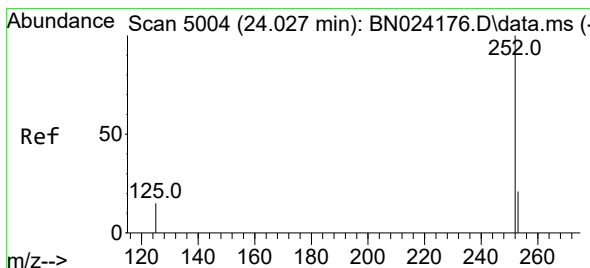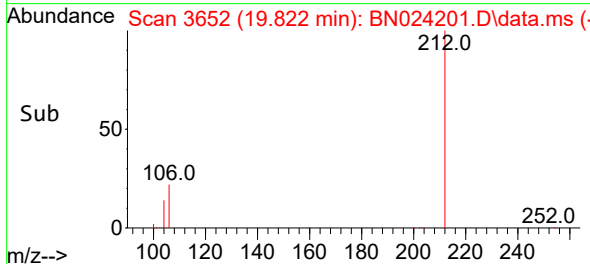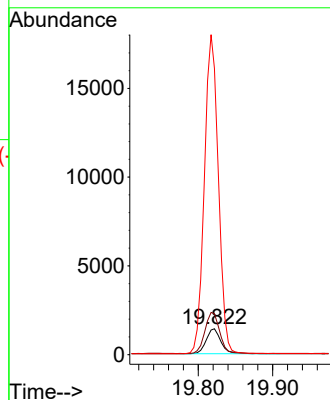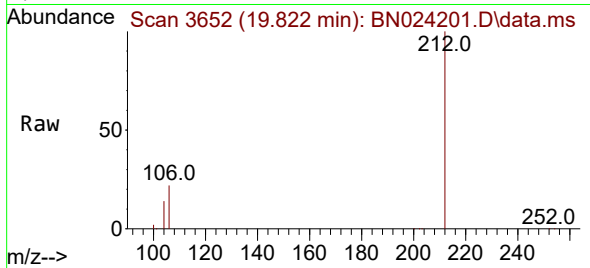

#26
Benzo(a)pyrene
Concen: 0.065 ng/ul
RT: 23.962 min Scan# 4982
Delta R.T. -0.041 min
Lab File: BN024201.D
Acq: 09 Mar 2023 15:58

Tgt Ion:252 Resp: 3412
Ion Ratio Lower Upper
252 100
253 42.6 19.2 28.8#
125 44.9 15.8 23.6#

