

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024230.D
 Acq On : 10 Mar 2023 10:56
 Operator : CG/JU
 Sample : PB151313BL
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK313

Quant Time: Mar 11 00:07:27 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 03:43:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	8427	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	25681	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.684	164	13710	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188	26424	0.400	ng/ul	0.00
17) Chrysene-d12	21.618	240	17691	0.400	ng/ul	0.00
23) Perylene-d12	24.132	264	18625	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	56439	6.086	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	9929	0.325	ng/ul	0.00
18) Fluoranthene-d10	19.450	212	18251	0.388	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.679	166	3409	0.069	ng/ul#	13
20) Pyrene	19.817	202	3049	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.974	252	6428	0.105	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024230.D
Acq On : 10 Mar 2023 10:56
Operator : CG/JU
Sample : PB151313BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK313

Quant Time: Mar 11 00:07:27 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 03:43:59 2023
Response via : Initial Calibration




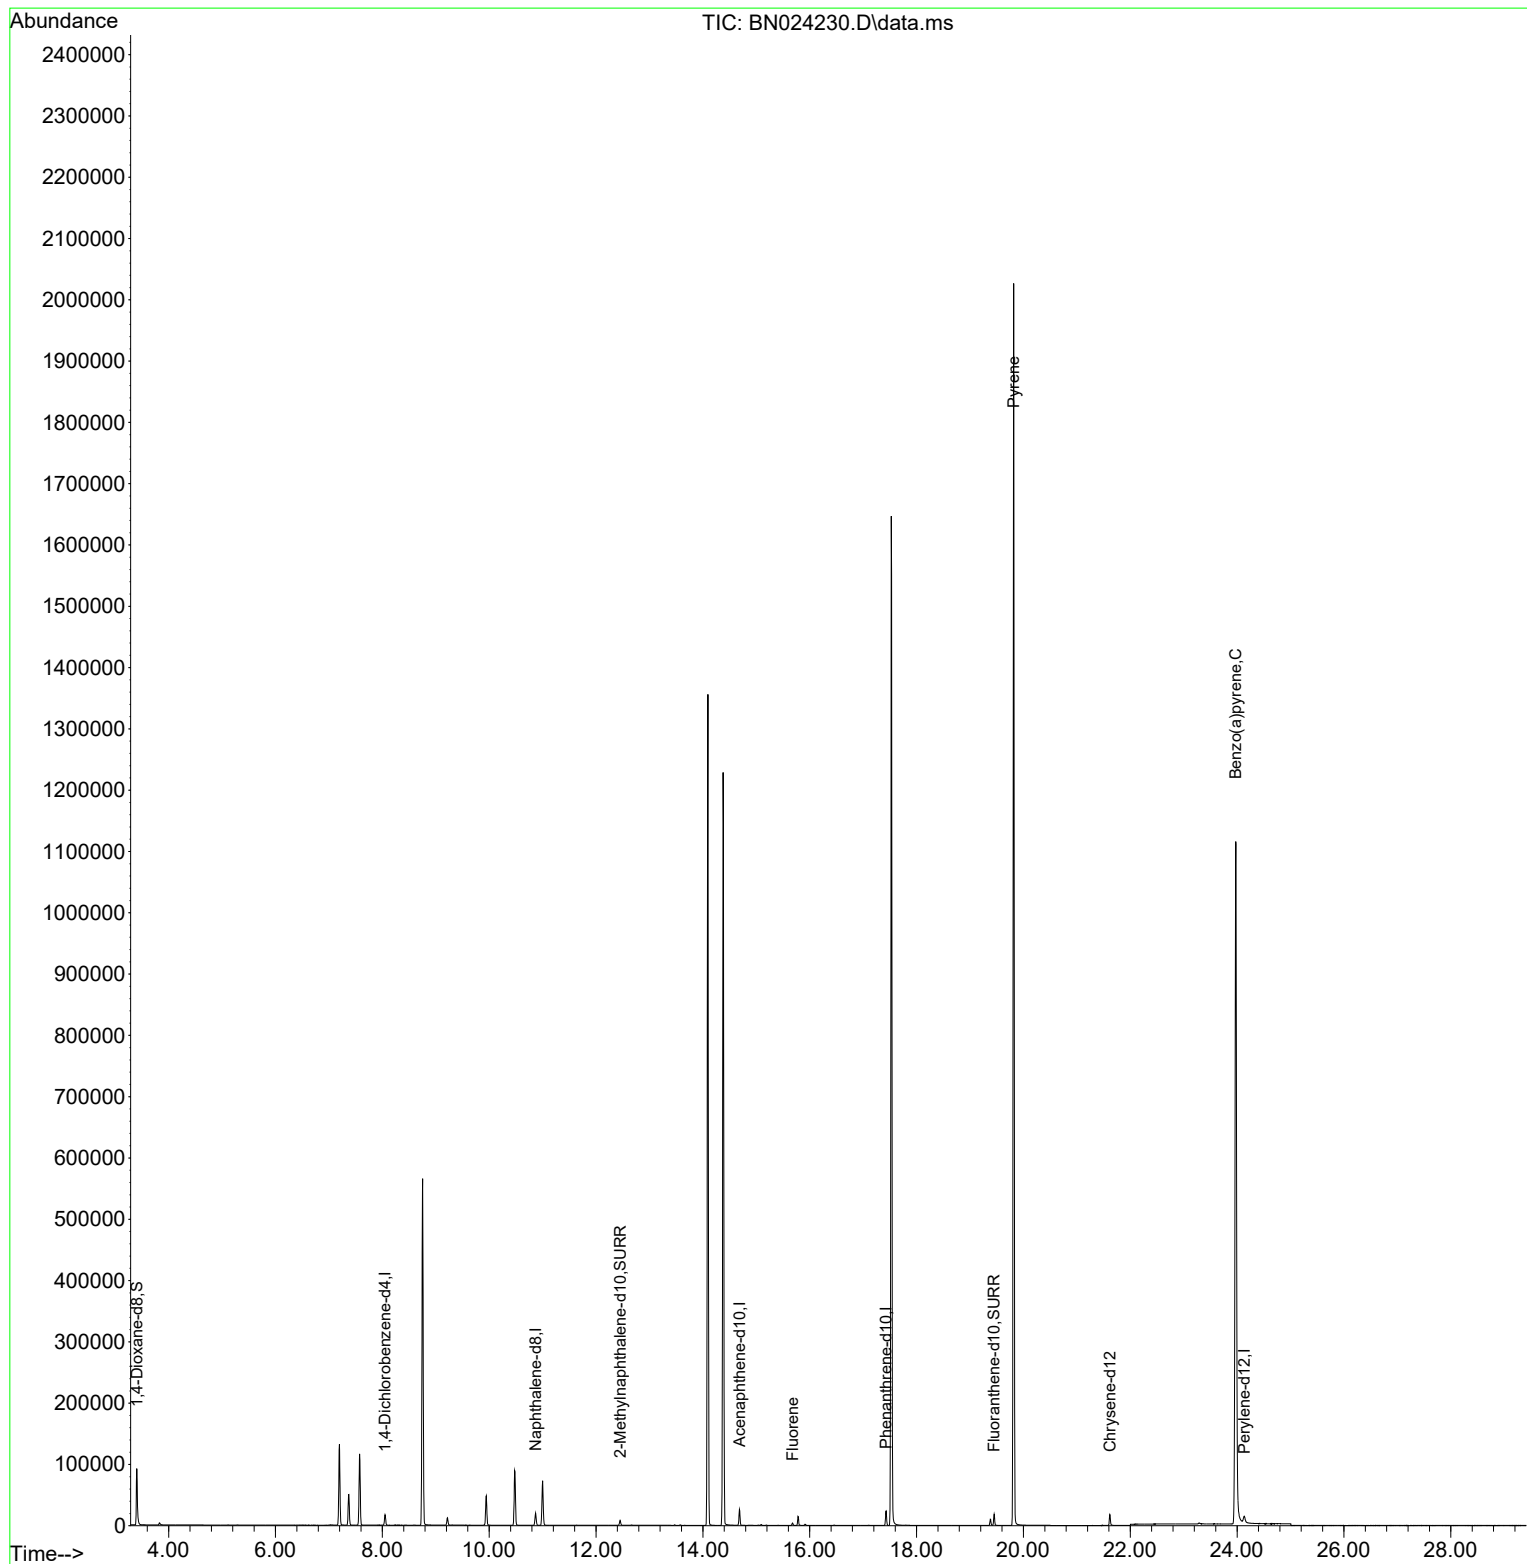


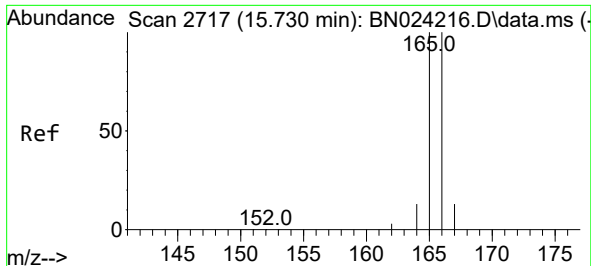

#12
Fluorene
Concen: 0.069 ng/ul
RT: 15.679 min Scan# 21
Delta R.T. -0.051 min
Lab File: BN024230.D
Acq: 10 Mar 2023 10:56




Instrument :
BNA_N
ClientSampleId :
SBLK313


Tgt Ion:166 Resp: 3409
Ion Ratio Lower Upper
166 100
165 6.9 77.4 116.0#
167 35.9 10.9 16.3#

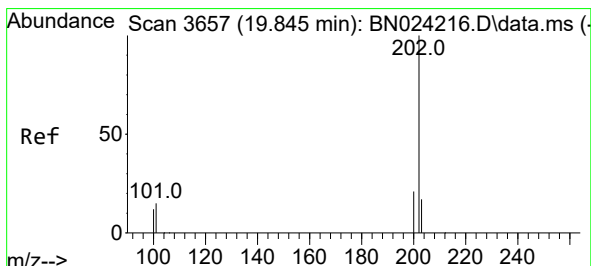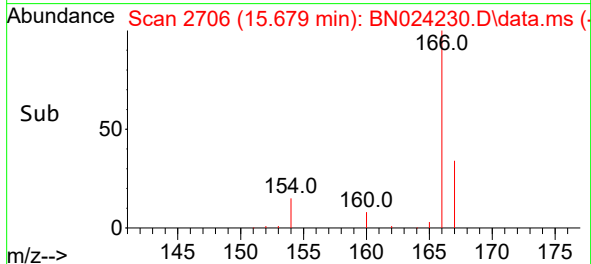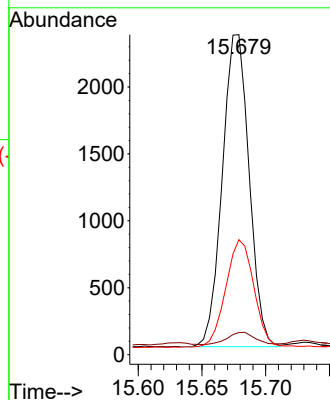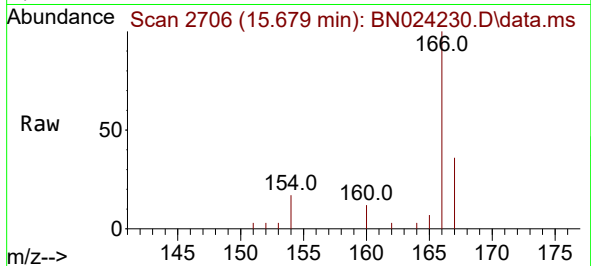

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.817 min Scan# 3651
Delta R.T. -0.028 min
Lab File: BN024230.D
Acq: 10 Mar 2023 10:56

Tgt Ion:202 Resp: 3049
Ion Ratio Lower Upper
202 100
101 171.2 12.1 18.1#
100 1247.4 9.4 14.0#

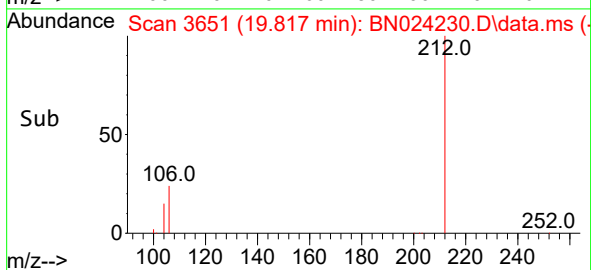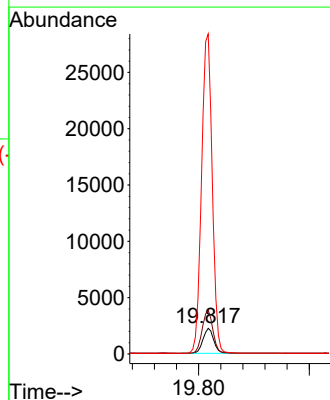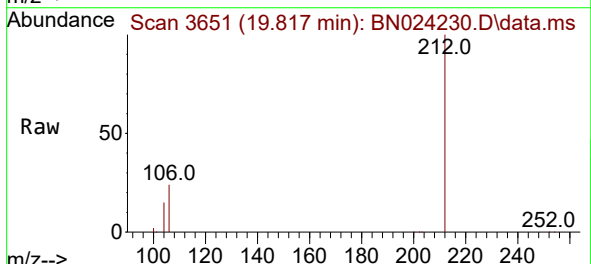

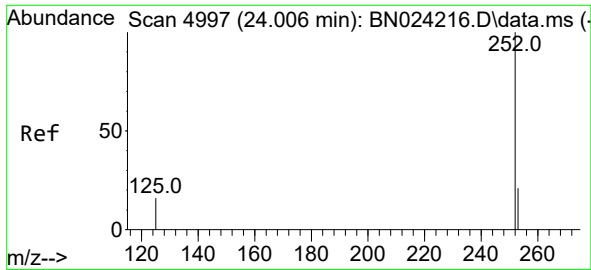

#26

Benzo(a)pyrene

Concen: 0.105 ng/ul

RT: 23.974 min Scan# 49

Delta R.T. -0.032 min

Lab File: BN024230.D


Acq: 10 Mar 2023 10:56

Instrument :

BNA_N

ClientSampleId :

SBLK313

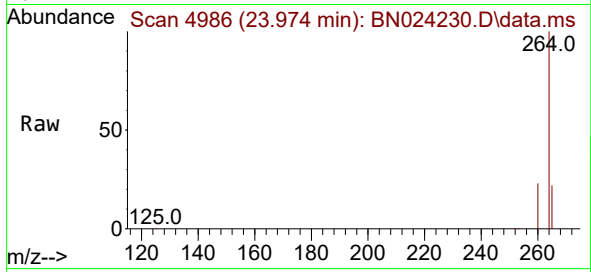

Tgt Ion:252 Resp: 6428

Ion Ratio Lower Upper

252 100

253 37.0 19.2 28.8#

125 35.9 15.8 23.6#

