




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024182.D
 Acq On : 09 Mar 2023 00:12
 Operator : CG/JU
 Sample : 01746-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAE1

Manual IntegrationsAPPROVED

Quant Time: Mar 09 03:52:26 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 03:48:21 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
 Supervised By :Jagrut Upadhyay 03/09/2023

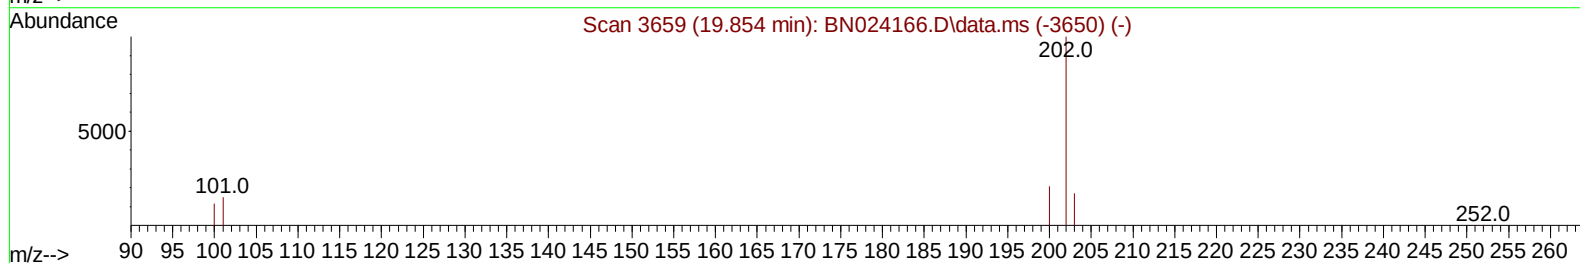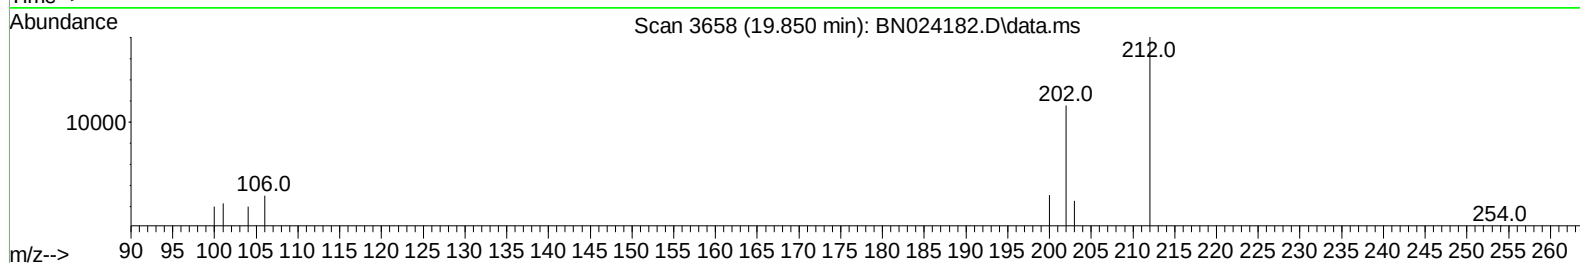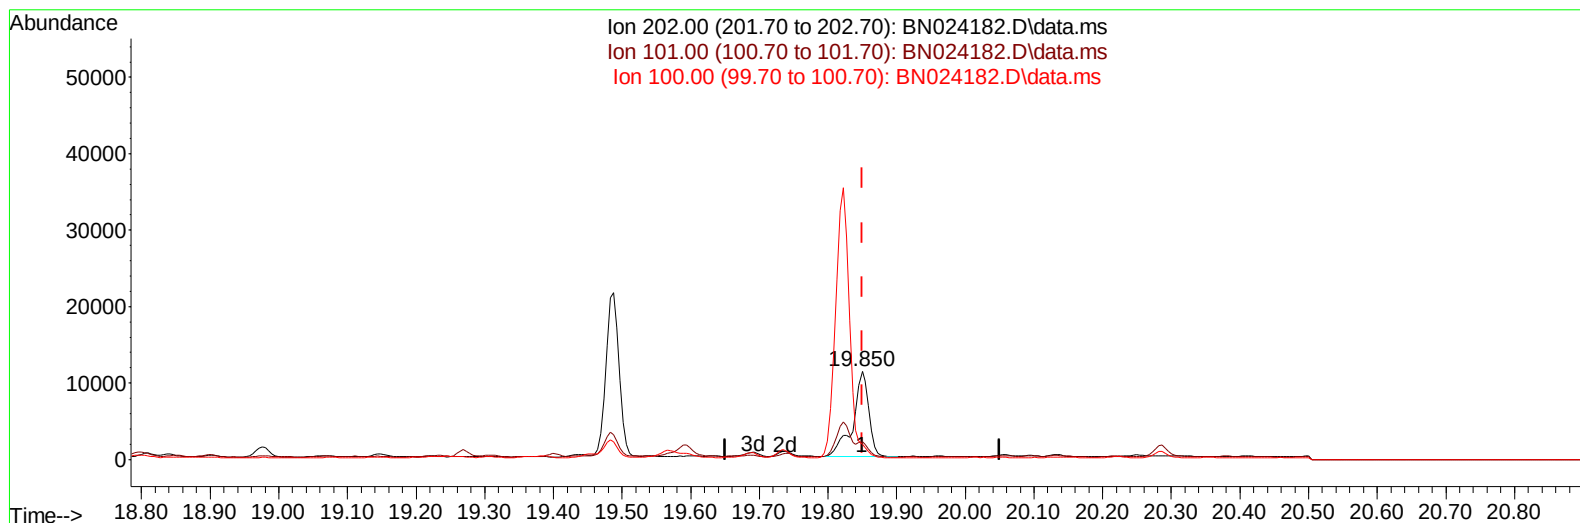

TIC: BN024182.D\data.ms

(20) Pyrene

19.850min (-0.000) 0.16 ng/u1

response 18095

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	19.97#
100.00	11.70	17.06#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024182.D
 Acq On : 09 Mar 2023 00:12
 Operator : CG/JU
 Sample : 01746-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAE1

Manual IntegrationsAPPROVED

Quant Time: Mar 09 03:52:26 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 03:48:21 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
 Supervised By :Jagrut Upadhyay 03/09/2023

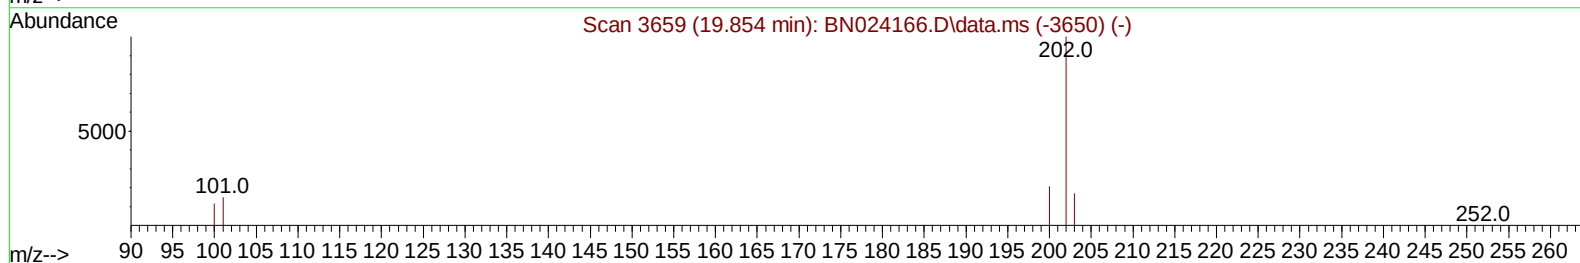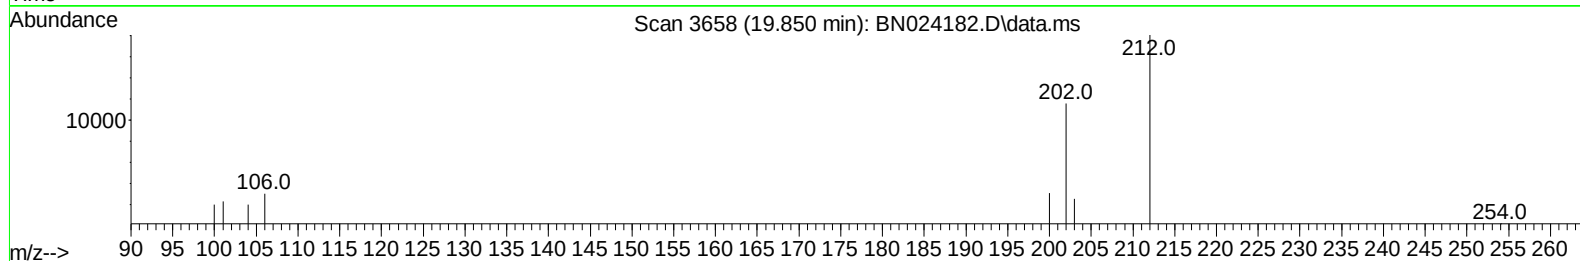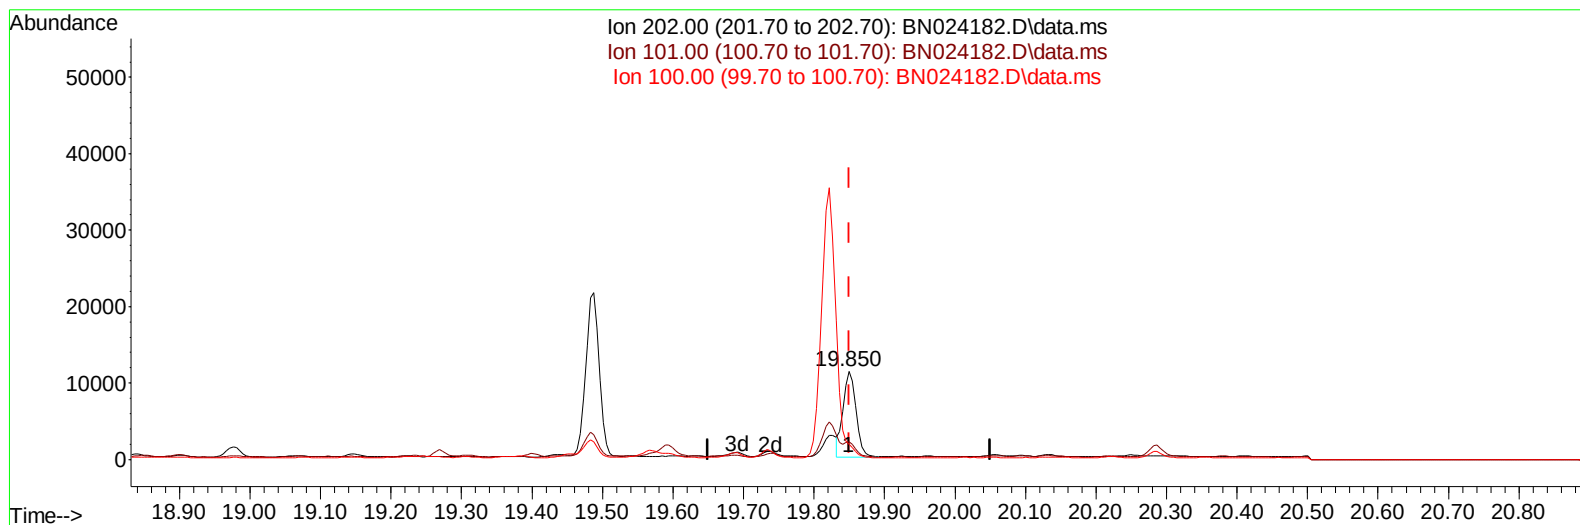

TIC: BN024182.D\data.ms

(20) Pyrene

19.850min (-0.000) 0.13 ng/ul m

response 14504

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	19.97#
100.00	11.70	17.06#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024182.D
 Acq On : 09 Mar 2023 00:12
 Operator : CG/JU
 Sample : 01746-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAE1

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/09/2023
 Supervised By :Jagrut Upadhyay 03/09/2023

Quant Time: Mar 09 03:52:26 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 03:48:21 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.055	152		9743	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136		30667	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164		19186	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.434	188		37253	0.400	ng/ul	0.00
17) Chrysene-d12	21.615	240		27526	0.400	ng/ul	-0.01
23) Perylene-d12	24.132	264		23899	0.400	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.405	96		40786	3.804	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152		13034	0.358	ng/ul	0.00
18) Fluoranthene-d10	19.455	212		31115	0.425	ng/ul	0.00
Target Compounds							Qvalue
5) Naphthalene	10.927	128		1752915	22.900	ng/ul	99
7) 2-Methylnaphthalene	12.527	142		63175	1.360	ng/ul	100
8) 1-Methylnaphthalene	12.747	142		192262	3.939	ng/ul	100
10) Acenaphthylene	14.411	152		106126	1.326	ng/ul	99
11) Acenaphthene	14.754	153		1643399	26.647	ng/ul	97
12) Fluorene	15.739	166		361798	5.253	ng/ul	100
14) Pentachlorophenol	17.080	266		25763	2.490	ng/ul#	73
15) Phenanthrene	17.477	178		342833	3.213	ng/ul	100
16) Anthracene	17.569	178		48108	0.514	ng/ul	96
19) Fluoranthene	19.487	202		28262	0.258	ng/ul	96
20) Pyrene	19.850	202		14504m	0.131	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024182.D
Acq On : 09 Mar 2023 00:12
Operator : CG/JU
Sample : 01746-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAE1

Manual IntegrationsAPPROVED

Quant Time: Mar 09 03:52:26 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 03:48:21 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
Supervised By :Jagrut Upadhyay 03/09/2023

