




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024183.D
 Acq On : 09 Mar 2023 00:49
 Operator : CG/JU
 Sample : 01746-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAE3

Manual IntegrationsAPPROVED

Quant Time: Mar 09 03:52:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 03:48:21 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
 Supervised By :Jagrut Upadhyay 03/09/2023

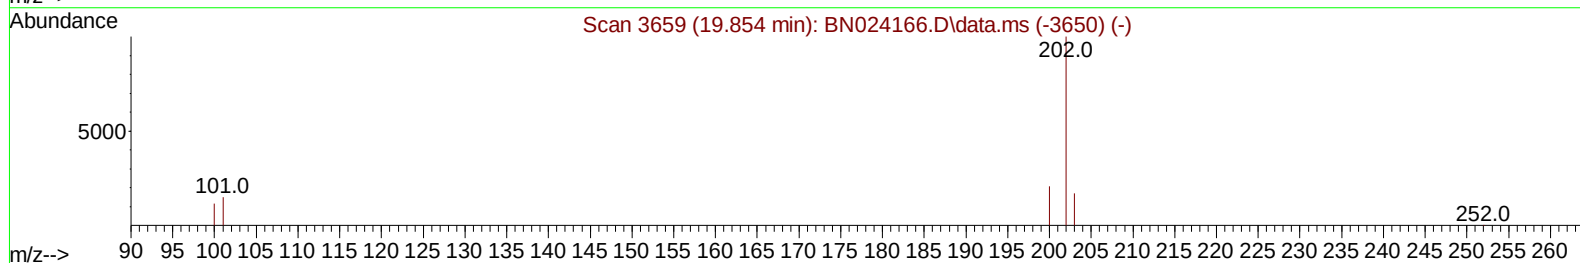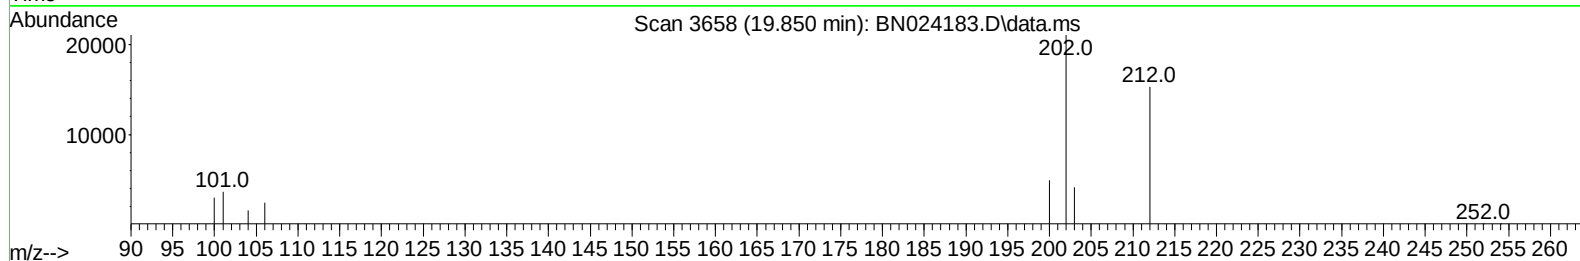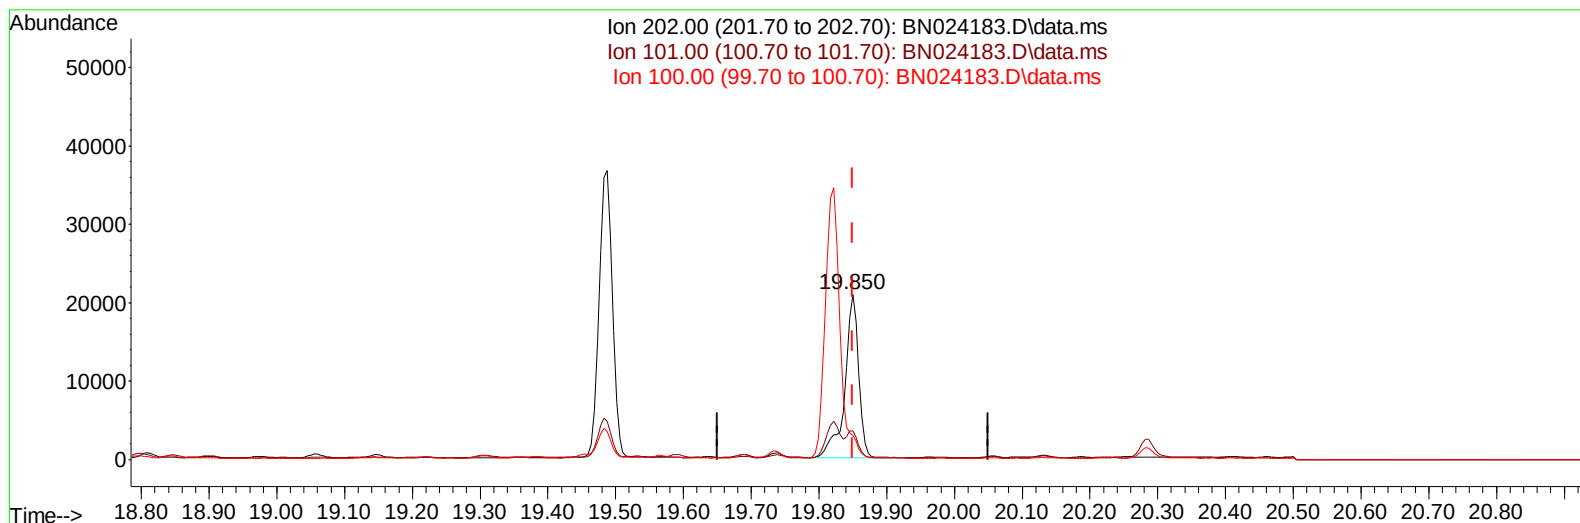

TIC: BN024183.D\data.ms

(20) Pyrene

19.850min (-0.000) 0.29 ng/u1

response 29750

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	17.34
100.00	11.70	14.45#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024183.D
 Acq On : 09 Mar 2023 00:49
 Operator : CG/JU
 Sample : 01746-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAE3

Manual IntegrationsAPPROVED

Quant Time: Mar 09 03:52:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 03:48:21 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
 Supervised By :Jagrut Upadhyay 03/09/2023

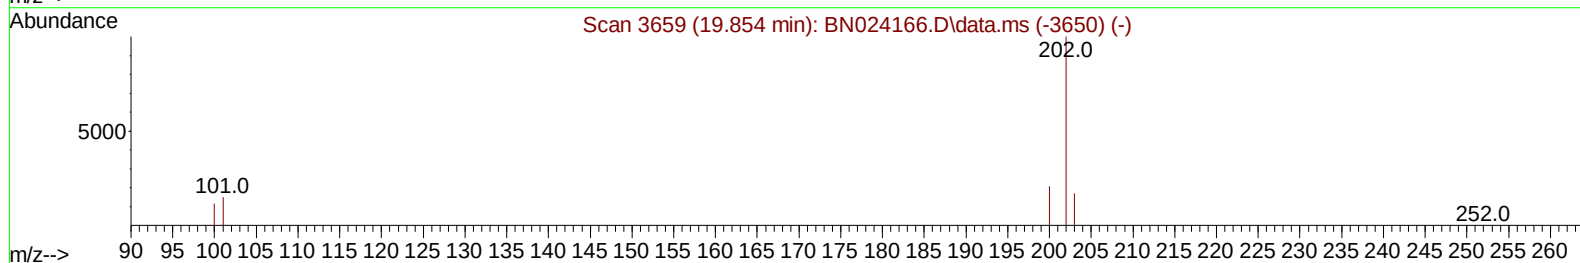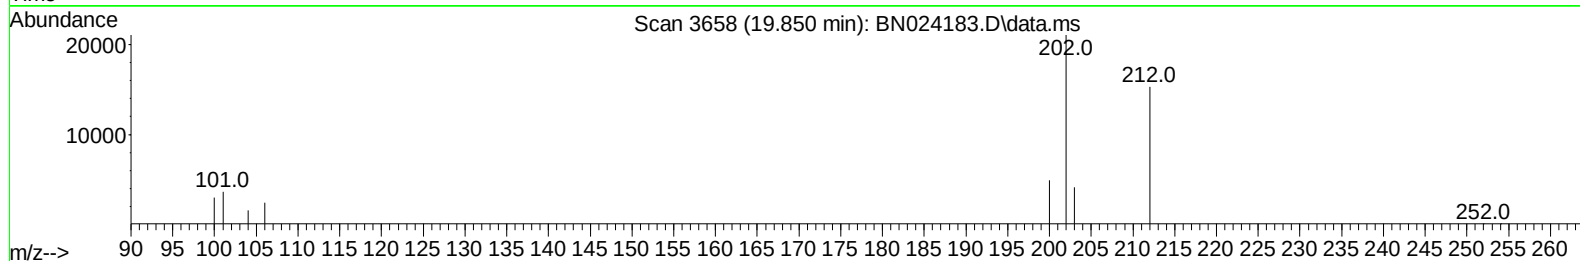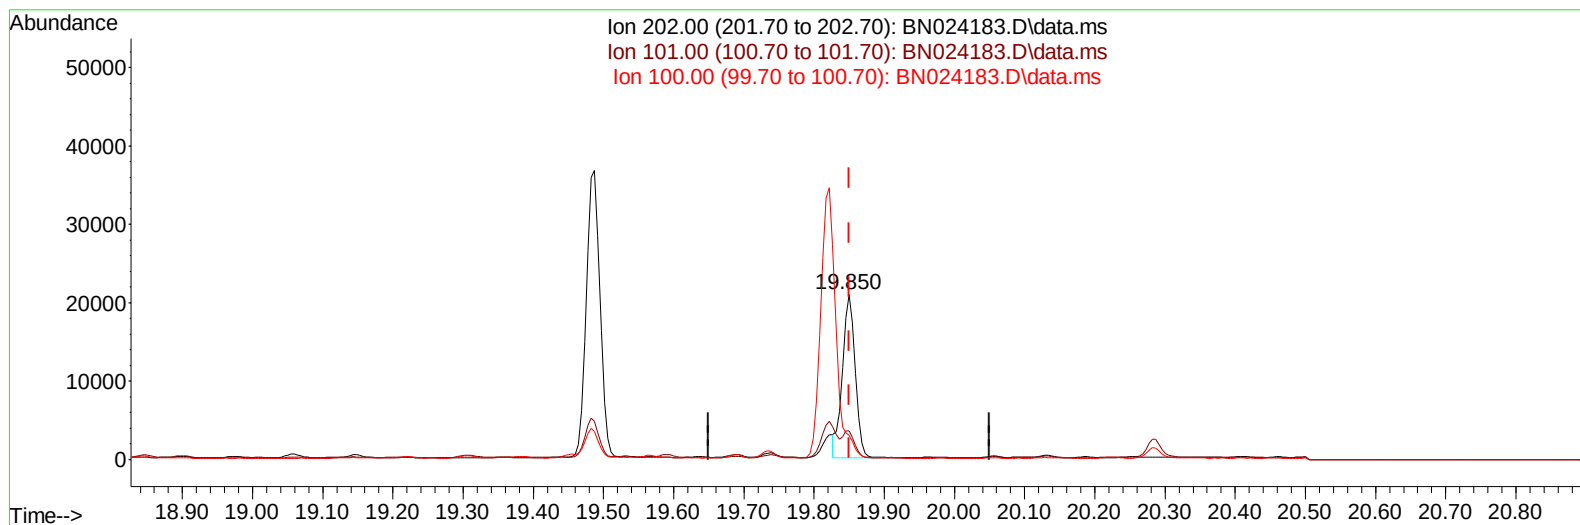

TIC: BN024183.D\data.ms

(20) Pyrene

19.850min (-0.000) 0.26 ng/ul m

response 26654

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	17.34
100.00	11.70	14.45#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024183.D
 Acq On : 09 Mar 2023 00:49
 Operator : CG/JU
 Sample : 01746-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAE3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/09/2023
 Supervised By :Jagrut Upadhyay 03/09/2023

Quant Time: Mar 09 03:52:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 03:48:21 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.055	152		8836	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136		27913	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164		17855	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.434	188		33875	0.400	ng/ul	0.00
17) Chrysene-d12	21.621	240		24987	0.400	ng/ul	0.00
23) Perylene-d12	24.123	264		22570	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.405	96		44602	4.587	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152		12731	0.384	ng/ul	0.00
18) Fluoranthene-d10	19.455	212		29762	0.448	ng/ul	0.00
Target Compounds							
						Qvalue	
5) Naphthalene	10.922	128		4389	0.063	ng/ul#	80
7) 2-Methylnaphthalene	12.527	142		85124	2.014	ng/ul	100
8) 1-Methylnaphthalene	12.742	142		130310	2.933	ng/ul	100
10) Acenaphthylene	14.411	152		42500	0.570	ng/ul#	94
11) Acenaphthene	14.754	153		771104	13.435	ng/ul	96
12) Fluorene	15.734	166		871649	13.600	ng/ul	98
14) Pentachlorophenol	17.080	266		31114	3.307	ng/ul#	73
15) Phenanthrene	17.477	178		1389226	14.318	ng/ul	100
16) Anthracene	17.565	178		139344	1.637	ng/ul	99
19) Fluoranthene	19.487	202		49962	0.502	ng/ul	100
20) Pyrene	19.850	202		26654m	0.264	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024183.D
Acq On : 09 Mar 2023 00:49
Operator : CG/JU
Sample : 01746-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAE3

Manual IntegrationsAPPROVED

Quant Time: Mar 09 03:52:34 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 03:48:21 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/09/2023
Supervised By :Jagrut Upadhyay 03/09/2023

