




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024198.D
 Acq On : 09 Mar 2023 14:07
 Operator : CG/JU
 Sample : 01746-16
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAF5

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:23:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

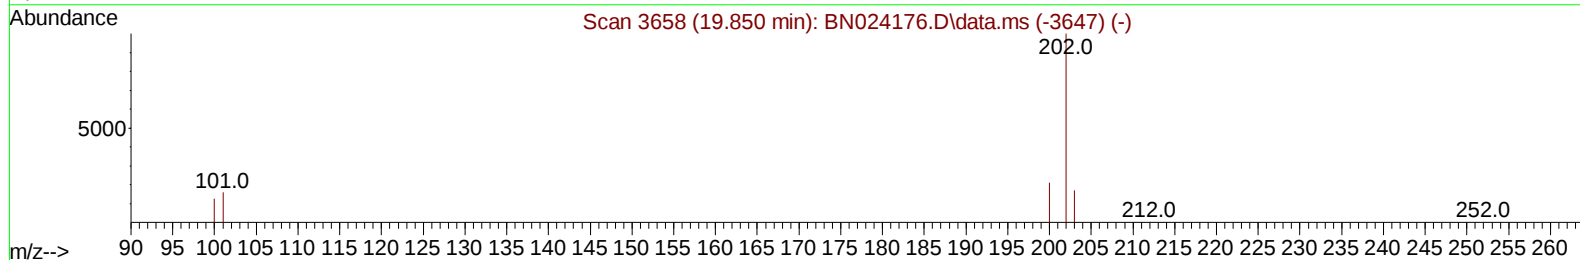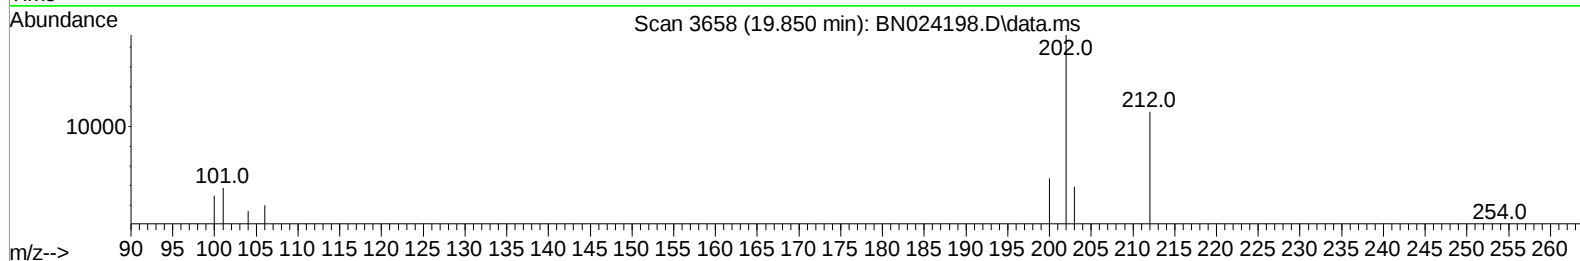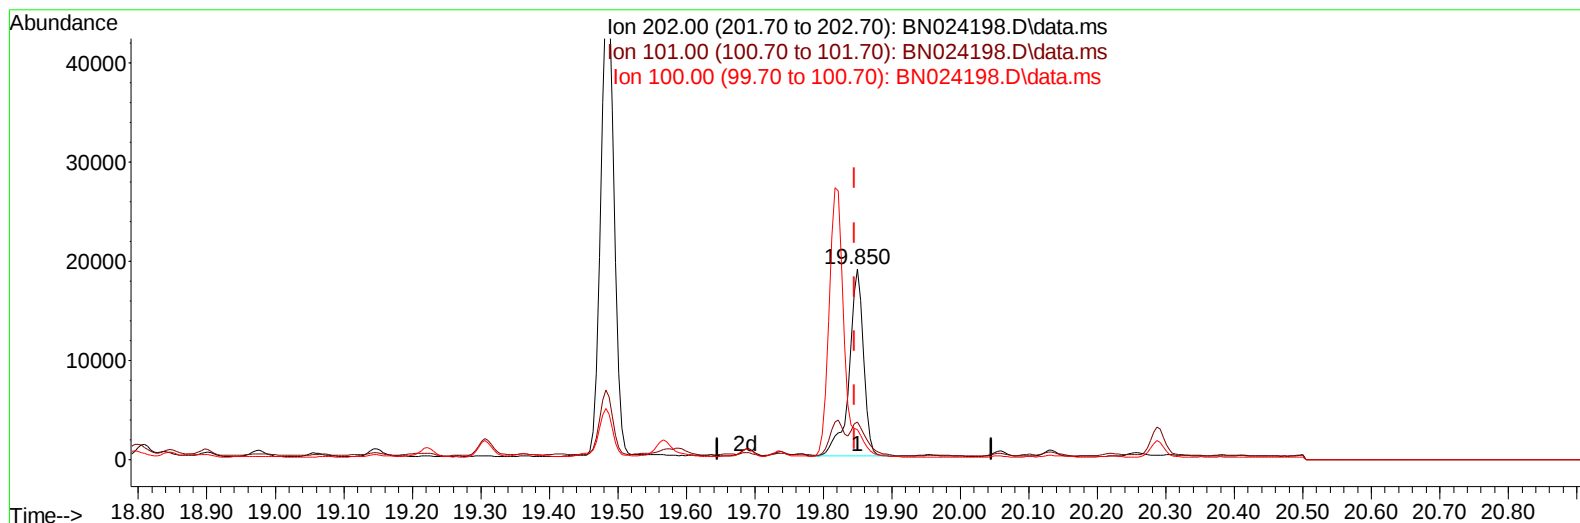

TIC: BN024198.D\data.ms

(20) Pyrene

19.850min (+ 0.005) 0.28 ng/u1

response 27455

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	19.74#
100.00	11.70	15.52#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024198.D
 Acq On : 09 Mar 2023 14:07
 Operator : CG/JU
 Sample : 01746-16
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAF5

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:23:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

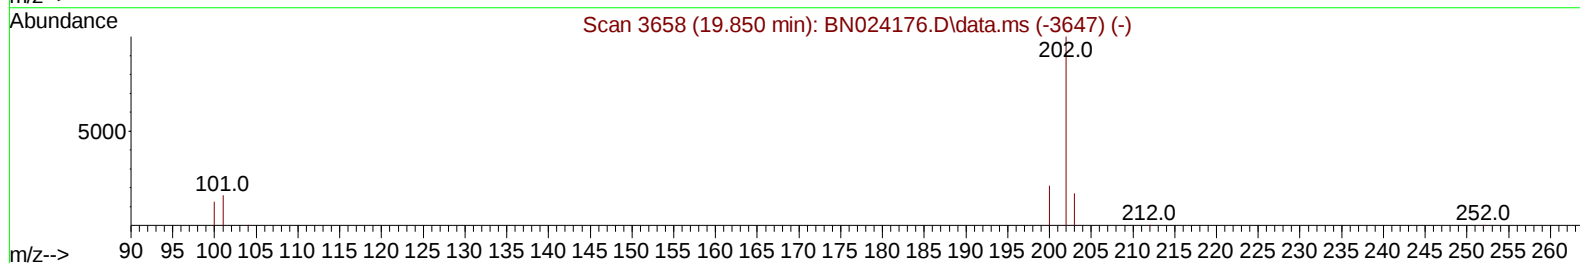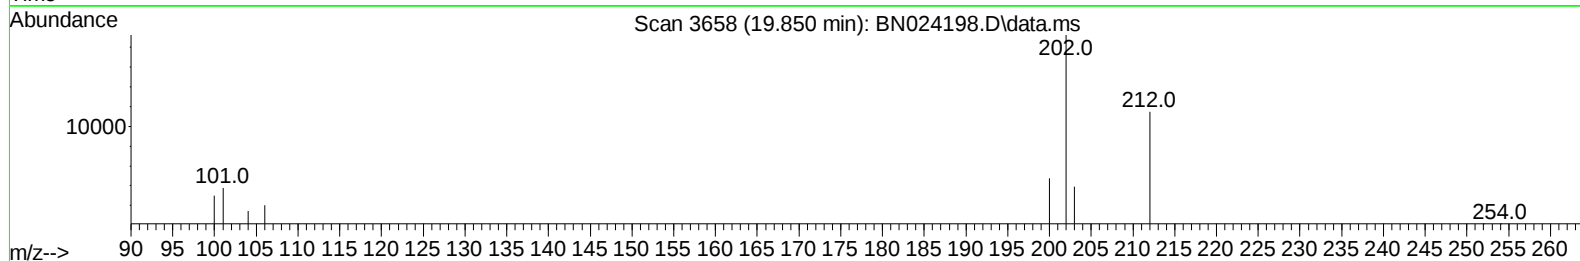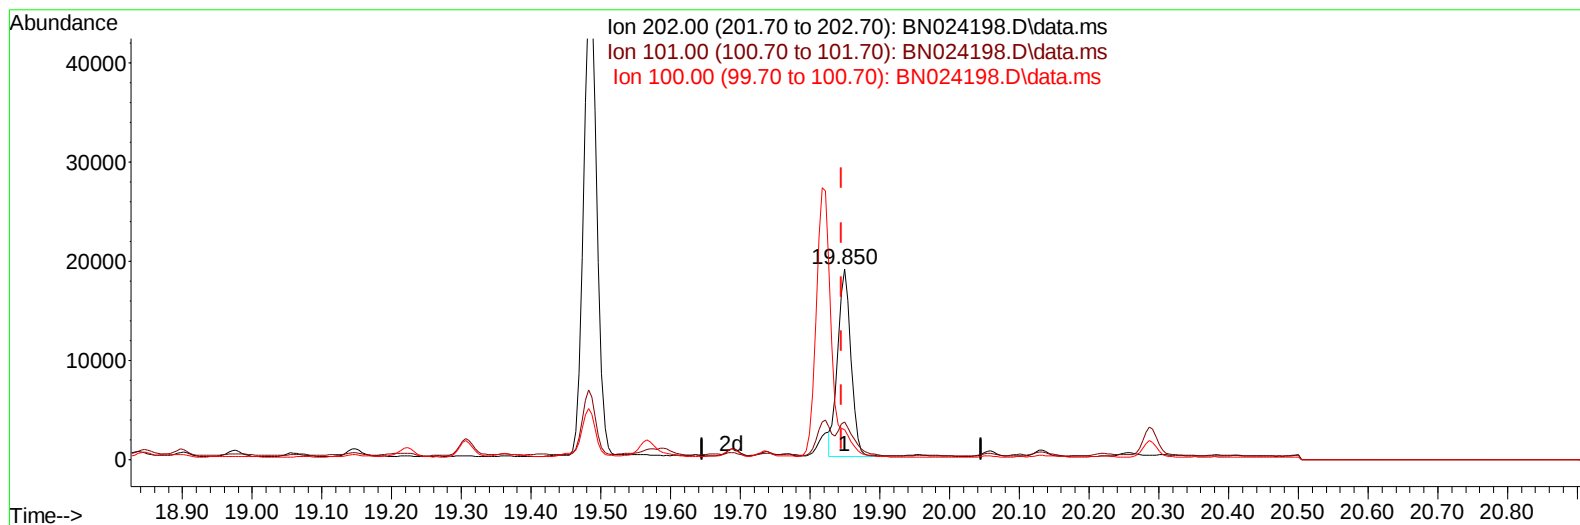

TIC: BN024198.D\data.ms

(20) Pyrene

19.850min (+ 0.005) 0.26 ng/ul m

response 24885

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	19.74#
100.00	11.70	15.52#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024198.D
 Acq On : 09 Mar 2023 14:07
 Operator : CG/JU
 Sample : 01746-16
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAF5

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 02:23:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.055	152		9026	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136		28196	0.400	ng/ul	0.01
9) Acenaphthene-d10	14.689	164		19539	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.434	188		33451	0.400	ng/ul	0.00
17) Chrysene-d12	21.621	240		23865	0.400	ng/ul	0.00
23) Perylene-d12	24.138	264		17816	0.400	ng/ul	0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.405	96		37410	3.766	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152		10982	0.328	ng/ul	0.00
18) Fluoranthene-d10	19.455	212		24745	0.390	ng/ul	0.00
Target Compounds							Qvalue
5) Naphthalene	10.955	128	25197130		358.020	ng/ul	95
7) 2-Methylnaphthalene	12.533	142	3066346		71.816	ng/ul	99
8) 1-Methylnaphthalene	12.747	142	2086038		46.489	ng/ul	99
10) Acenaphthylene	14.411	152	350056		4.294	ng/ul	98
11) Acenaphthene	14.754	153	2668943		42.494	ng/ul	97
12) Fluorene	15.734	166	1347462		19.212	ng/ul	99
14) Pentachlorophenol	17.080	266	384078		41.338	ng/ul#	73
15) Phenanthrene	17.477	178	1670917		17.440	ng/ul	99
16) Anthracene	17.565	178	139385		1.658	ng/ul	98
19) Fluoranthene	19.483	202	63492		0.668	ng/ul	96
20) Pyrene	19.850	202	24885m		0.258	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024198.D
Acq On : 09 Mar 2023 14:07
Operator : CG/JU
Sample : 01746-16
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAF5

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:23:55 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

