




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024204.D
 Acq On : 09 Mar 2023 17:49
 Operator : CG/JU
 Sample : 01746-21
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:24:49 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

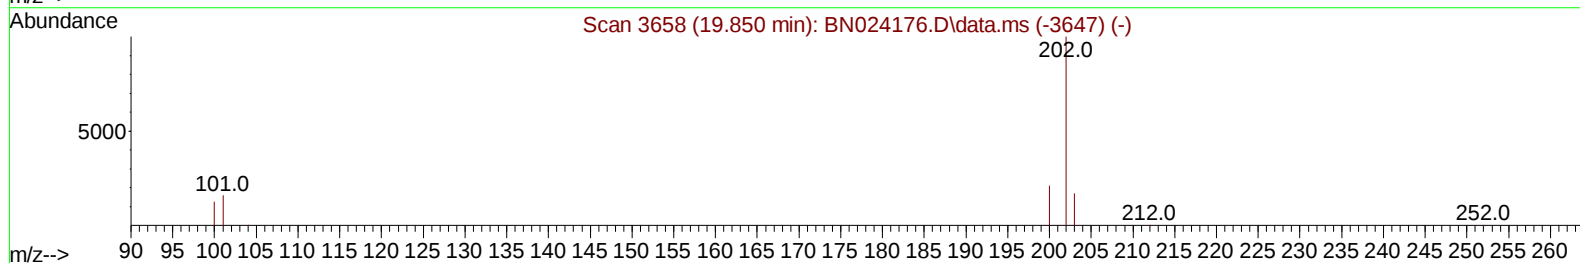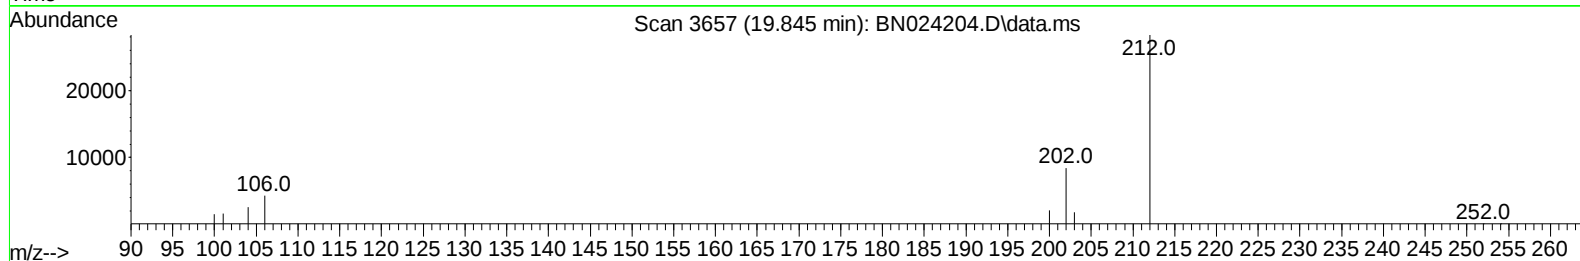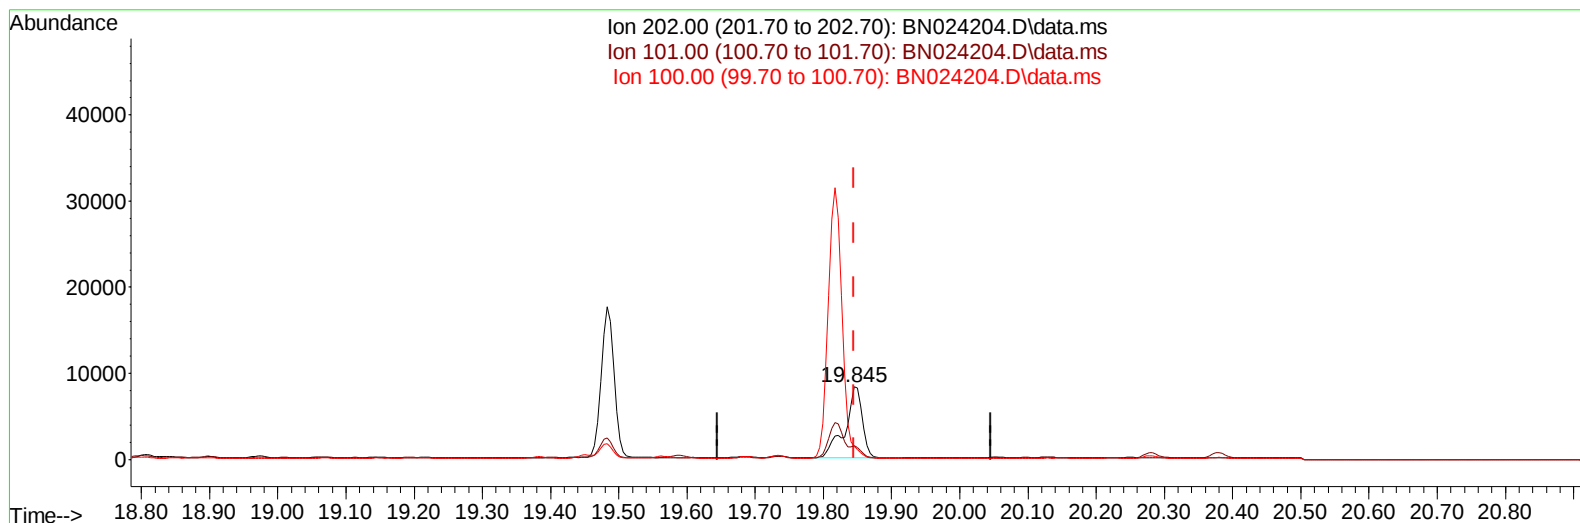

TIC: BN024204.D\data.ms

(20) Pyrene

19.845min (+ 0.000) 0.18 ng/u1

response 14446

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	18.93#
100.00	11.70	17.89#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024204.D
 Acq On : 09 Mar 2023 17:49
 Operator : CG/JU
 Sample : 01746-21
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:24:49 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

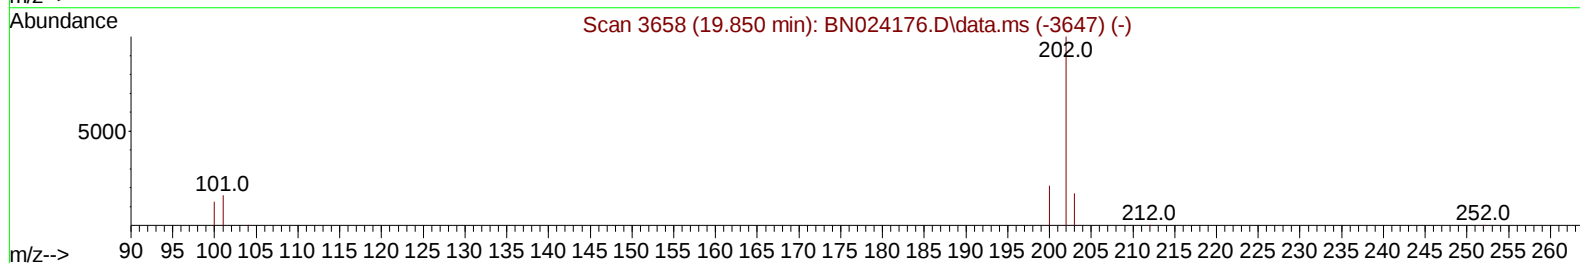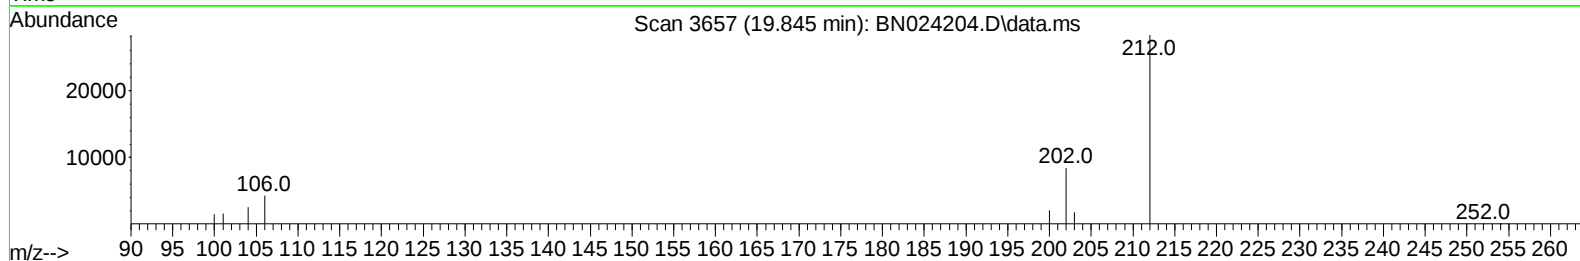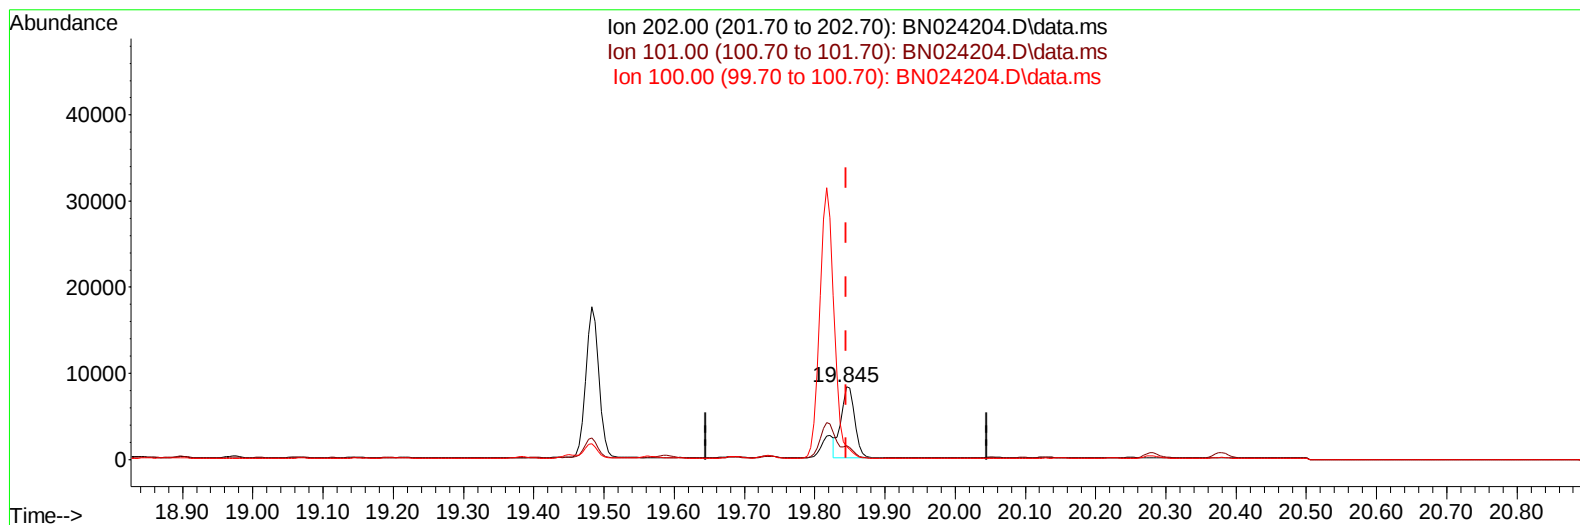

TIC: BN024204.D\data.ms

(20) Pyrene

19.845min (+ 0.000) 0.14 ng/ul m

response 11309

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	18.93#
100.00	11.70	17.89#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024204.D
 Acq On : 09 Mar 2023 17:49
 Operator : CG/JU
 Sample : 01746-21
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 02:24:49 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.055	152		7748	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136		24476	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164		14432	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.430	188		29173	0.400	ng/ul	0.00
17) Chrysene-d12	21.621	240		20382	0.400	ng/ul	0.00
23) Perylene-d12	24.138	264		15766	0.400	ng/ul	0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.406	96		41133	4.824	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152		11267	0.387	ng/ul	0.00
18) Fluoranthene-d10	19.455	212		27184	0.501	ng/ul	0.00
Target Compounds							
							Qvalue
5) Naphthalene	10.922	128		277725	4.546	ng/ul	100
7) 2-Methylnaphthalene	12.528	142		3313	0.089	ng/ul	100
8) 1-Methylnaphthalene	12.742	142		12484	0.320	ng/ul	100
10) Acenaphthylene	14.411	152		43118	0.716	ng/ul#	97
11) Acenaphthene	14.754	153		1499965	32.333	ng/ul	97
12) Fluorene	15.735	166		675997	13.049	ng/ul	99
14) Pentachlorophenol	17.076	266		511	0.063	ng/ul#	74
15) Phenanthrene	17.472	178		49915	0.597	ng/ul	98
16) Anthracene	17.565	178		13072	0.178	ng/ul#	92
19) Fluoranthene	19.483	202		22922	0.283	ng/ul	97
20) Pyrene	19.845	202		11309m	0.137	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024204.D
Acq On : 09 Mar 2023 17:49
Operator : CG/JU
Sample : 01746-21
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAC6

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:24:49 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

