




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024207.D
 Acq On : 09 Mar 2023 19:41
 Operator : CG/JU
 Sample : 01746-03DL 5X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC7DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:25:16 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

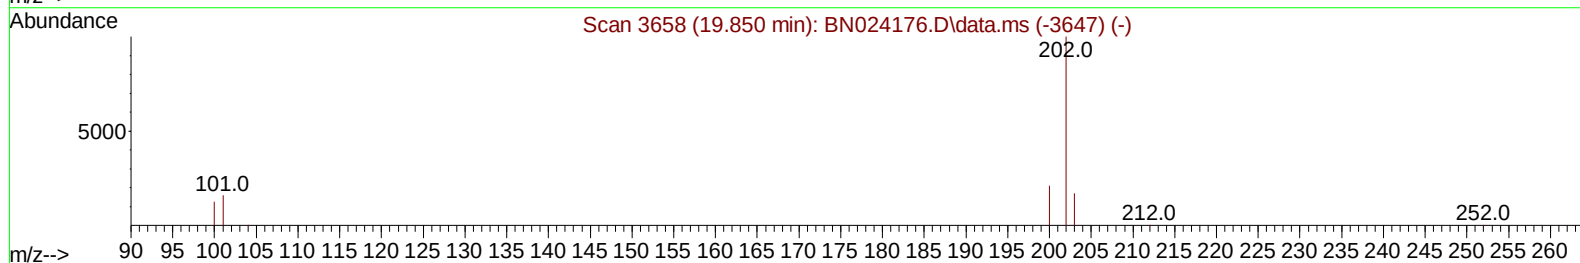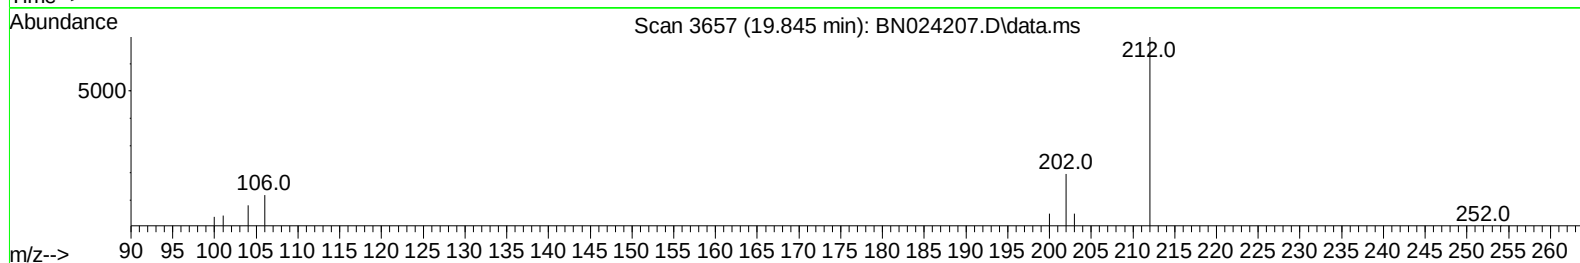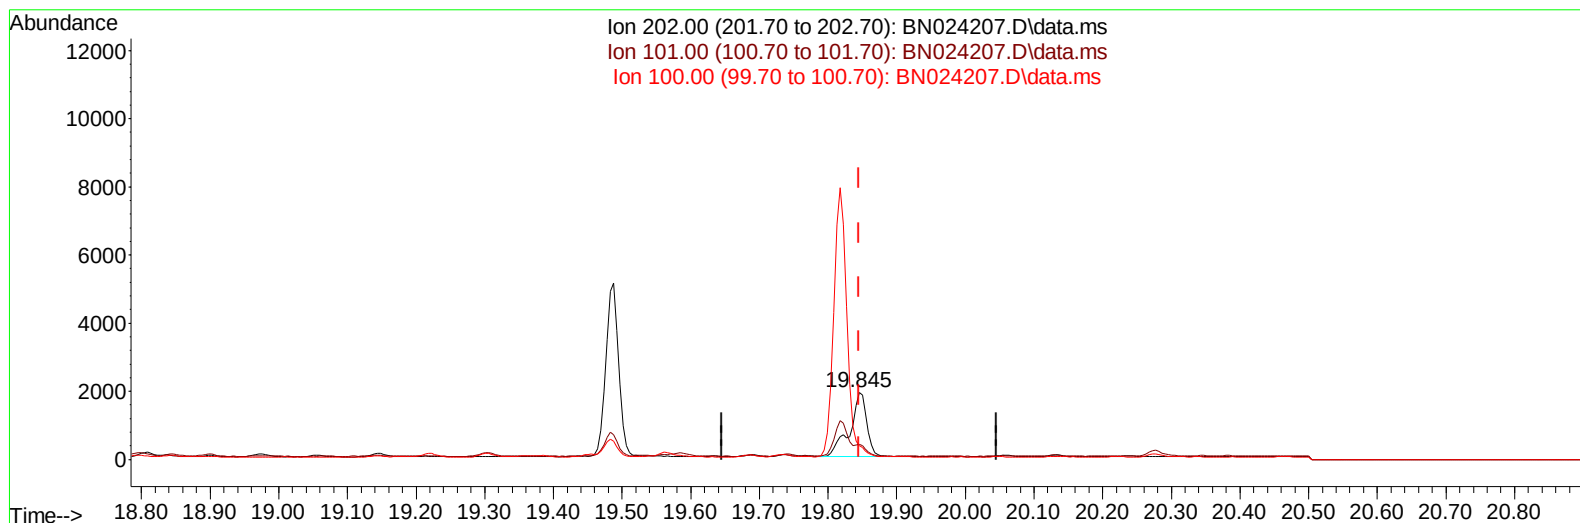

TIC: BN024207.D\data.ms

(20) Pyrene

19.845min (-0.000) 0.04 ng/u1

response 3315

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	22.87#
100.00	11.70	20.54#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024207.D
 Acq On : 09 Mar 2023 19:41
 Operator : CG/JU
 Sample : 01746-03DL 5X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC7DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:25:16 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

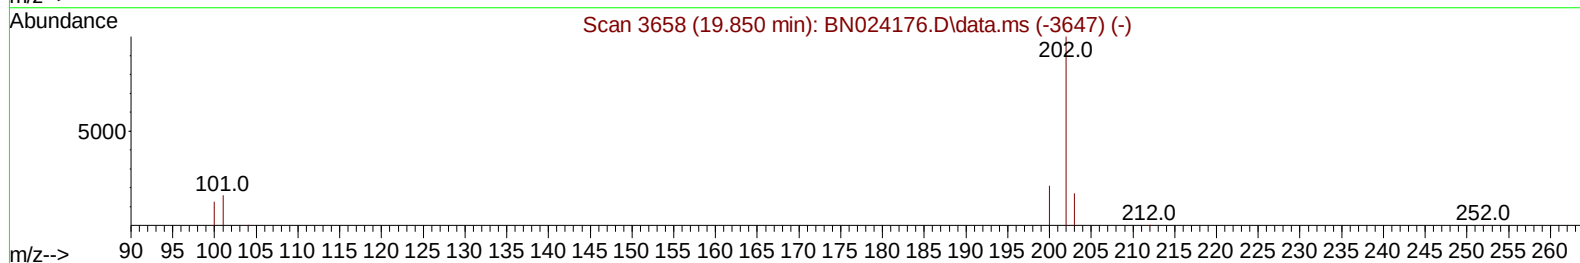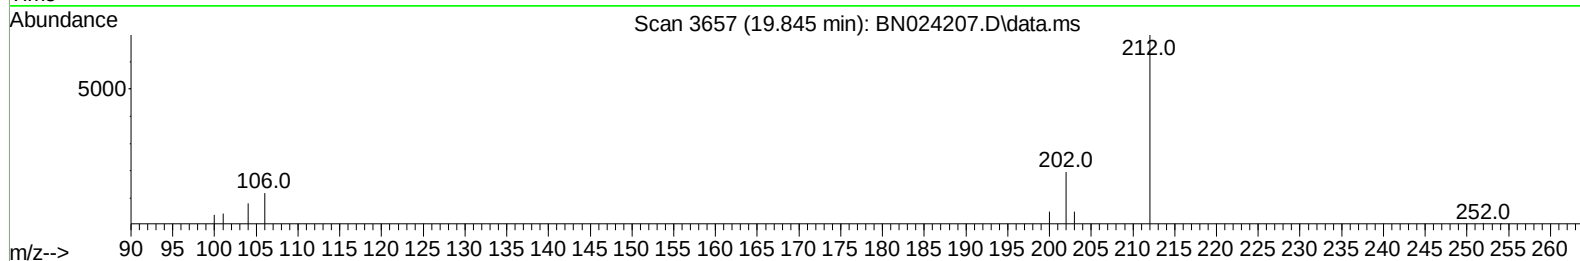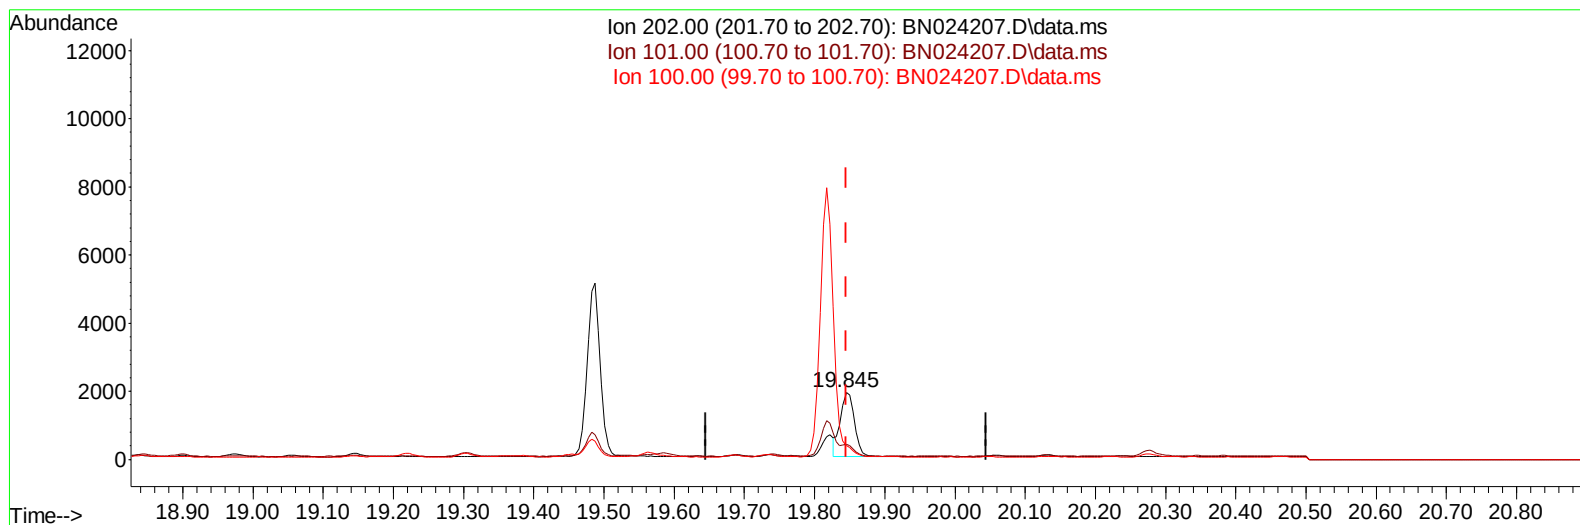

TIC: BN024207.D\data.ms

(20) Pyrene

19.845min (-0.000) 0.03 ng/ul m

response 2617

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	22.87#
100.00	11.70	20.54#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024207.D
 Acq On : 09 Mar 2023 19:41
 Operator : CG/JU
 Sample : 01746-03DL 5X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC7DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 02:25:16 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.055	152		9085	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136		27439	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164		15642	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188		31661	0.400	ng/ul	0.00
17) Chrysene-d12	21.621	240		20799	0.400	ng/ul	0.00
23) Perylene-d12	24.138	264		14908	0.400	ng/ul	0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.410	96		4317	0.432	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152		2464	0.076	ng/ul	0.00
18) Fluoranthene-d10	19.455	212		5283	0.095	ng/ul	0.00
Target Compounds							
							Qvalue
5) Naphthalene	10.927	128		4424429	64.600	ng/ul	100
7) 2-Methylnaphthalene	12.527	142		297072	7.150	ng/ul	100
8) 1-Methylnaphthalene	12.742	142		215647	4.938	ng/ul	100
10) Acenaphthylene	14.411	152		38453	0.589	ng/ul	98
11) Acenaphthene	14.754	153		329420	6.552	ng/ul	98
12) Fluorene	15.734	166		162246	2.890	ng/ul	99
14) Pentachlorophenol	17.075	266		45118	5.131	ng/ul#	73
15) Phenanthrene	17.472	178		245491	2.707	ng/ul	100
16) Anthracene	17.565	178		18913	0.238	ng/ul	99
19) Fluoranthene	19.487	202		6548	0.079	ng/ul	97
20) Pyrene	19.845	202		2617m	0.031	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024207.D
Acq On : 09 Mar 2023 19:41
Operator : CG/JU
Sample : 01746-03DL 5X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAC7DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:25:16 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

