




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024208.D
Acq On : 09 Mar 2023 20:18
Operator : CG/JU
Sample : 01746-01DL 5X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

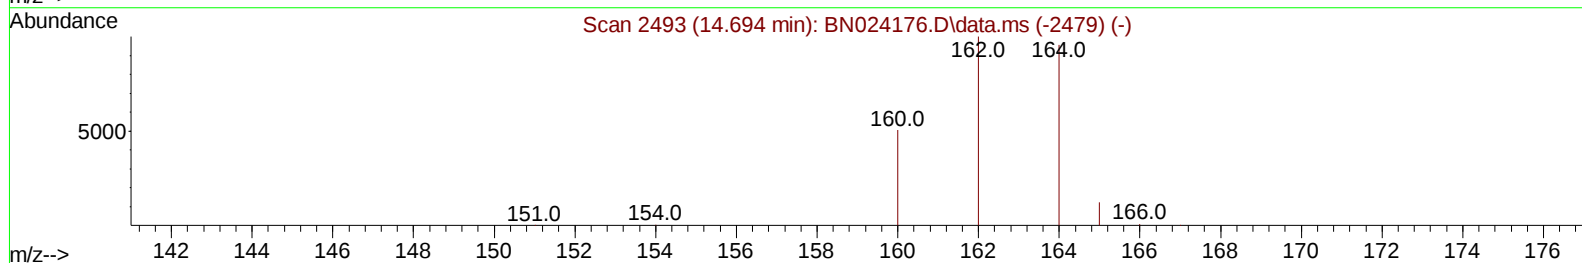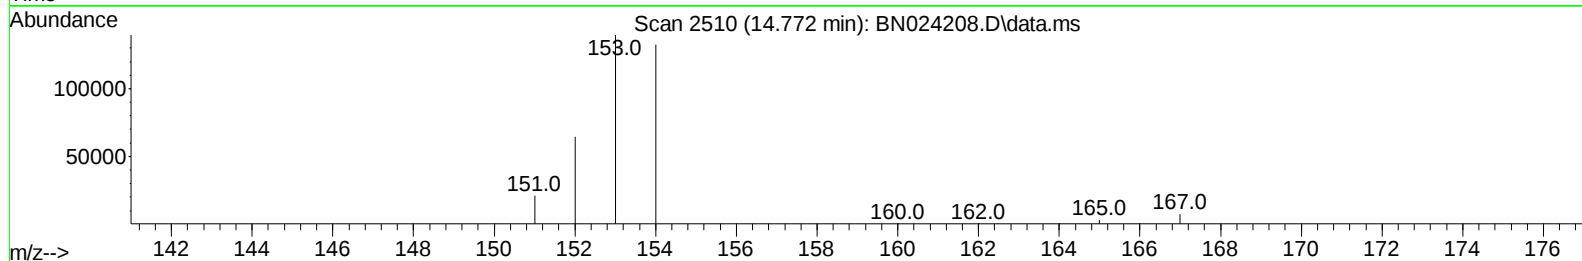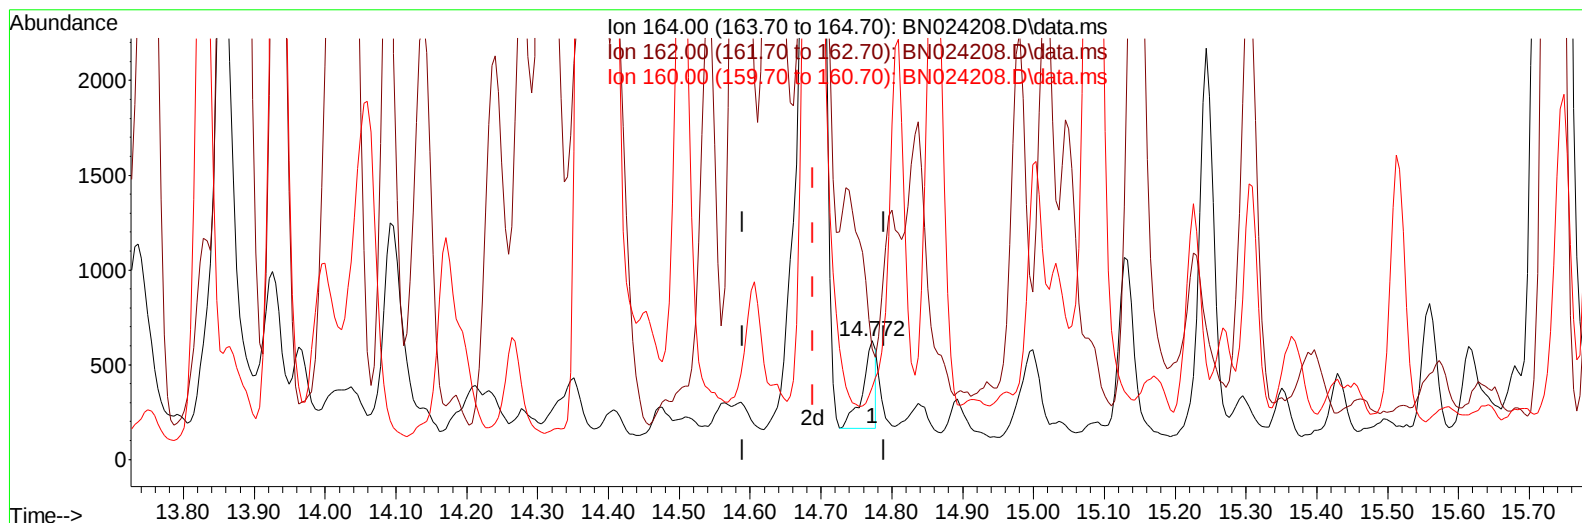

TIC: BN024208.D\data.ms

(9) Acenaphthene-d10 (I)

14.772min (+ 0.083) 0.40 ng/u1

response 607

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	103.80	92.97
160.00	52.10	61.02
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

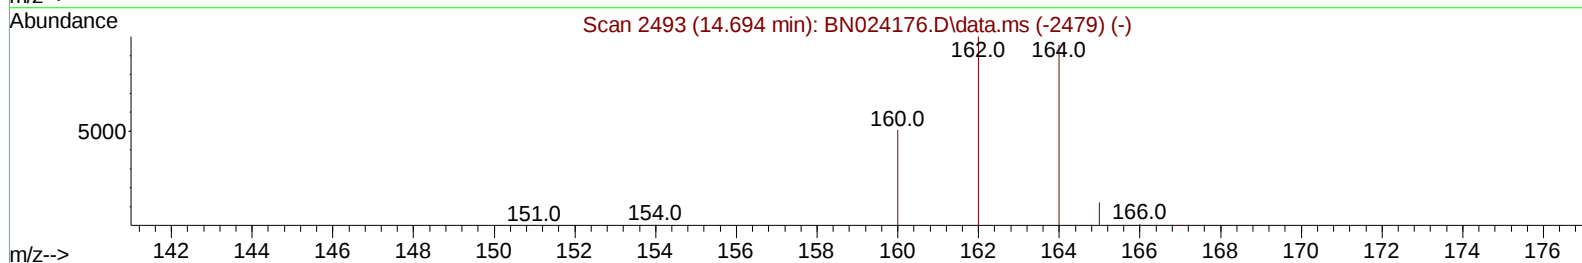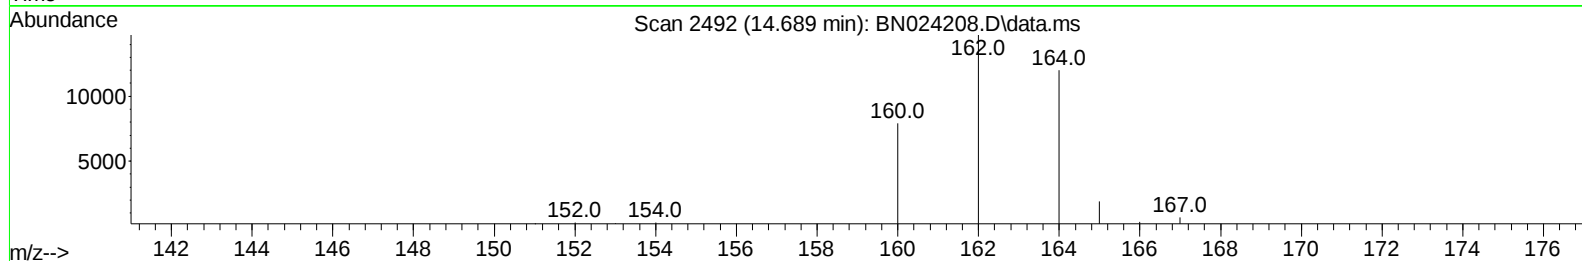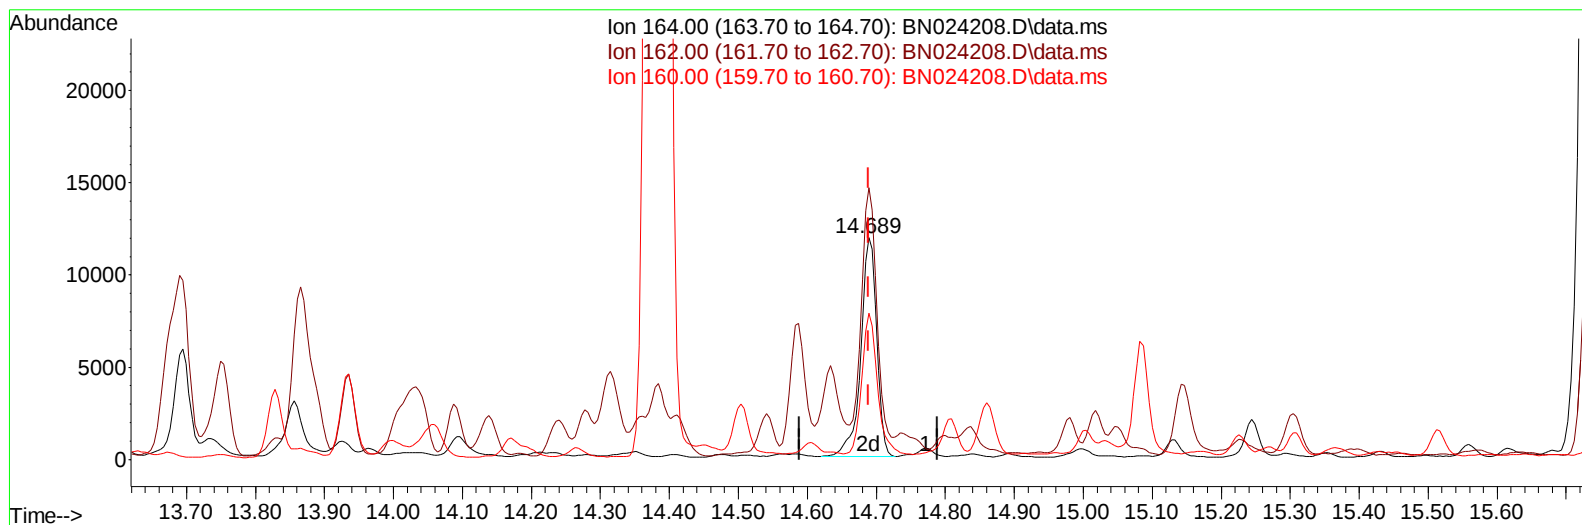

TIC: BN024208.D\data.ms

(9) Acenaphthene-d10 (I)

14.689min (+ 0.000) 0.40 ng/ul m

response 19052

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	103.80	122.33
160.00	52.10	65.95#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

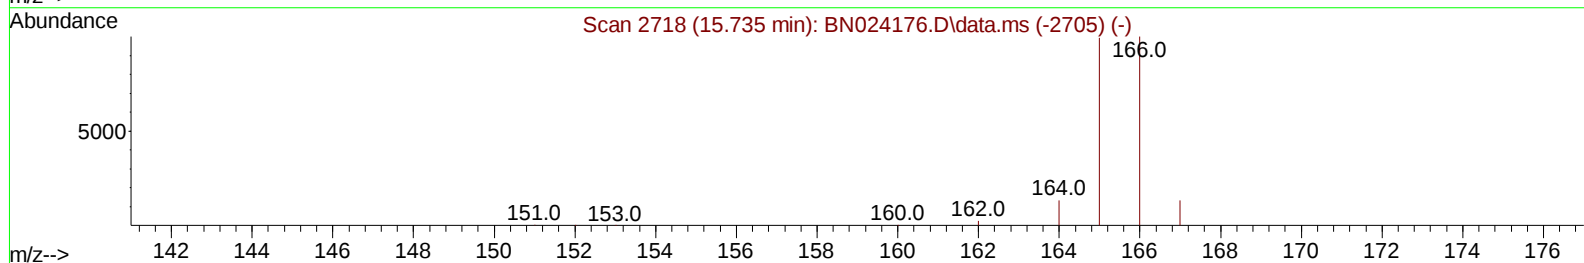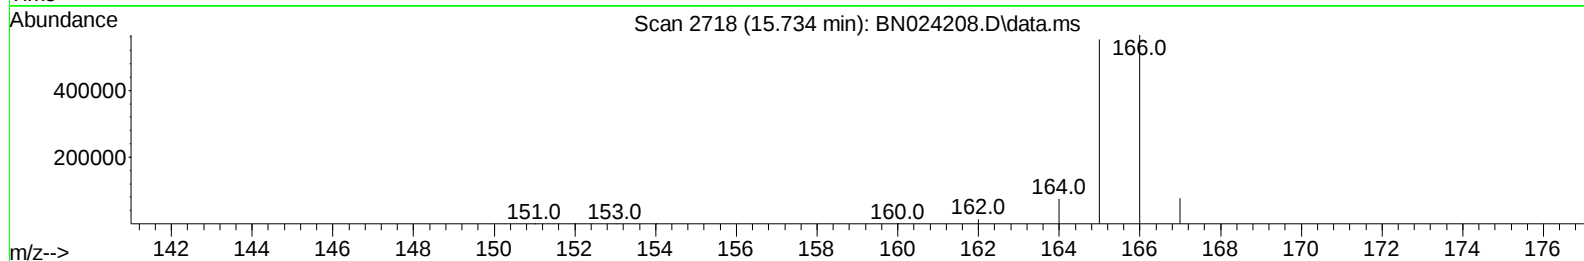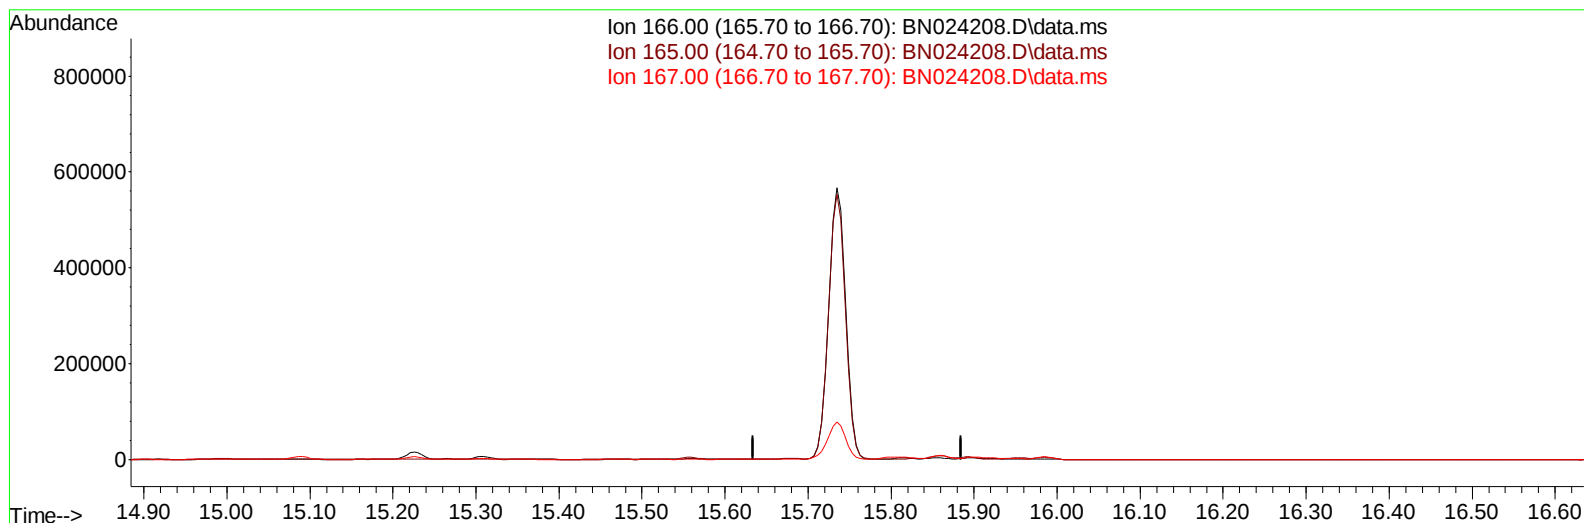

TIC: BN024208.D\data.ms

(12) Fluorene

15.734min (-15.734) 0.00 ng/ul

response 0

Ion	Exp%	Act%
166.00	100.00	0.00
165.00	96.70	0.00#
167.00	13.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

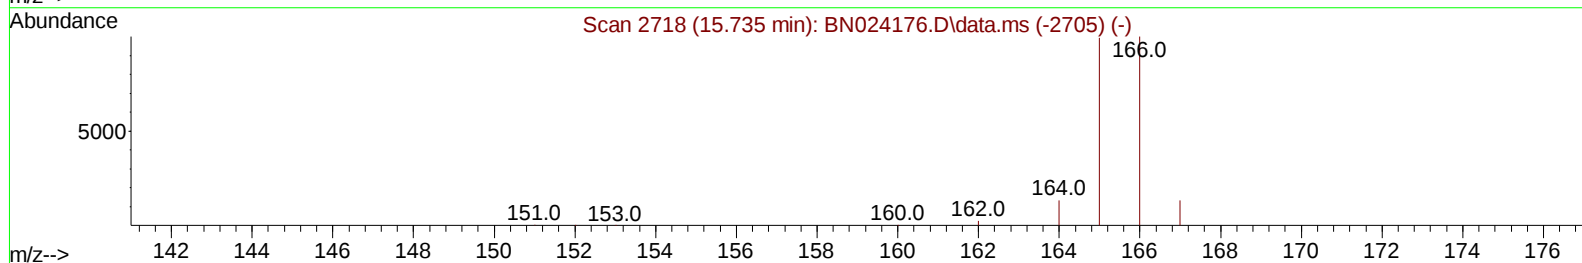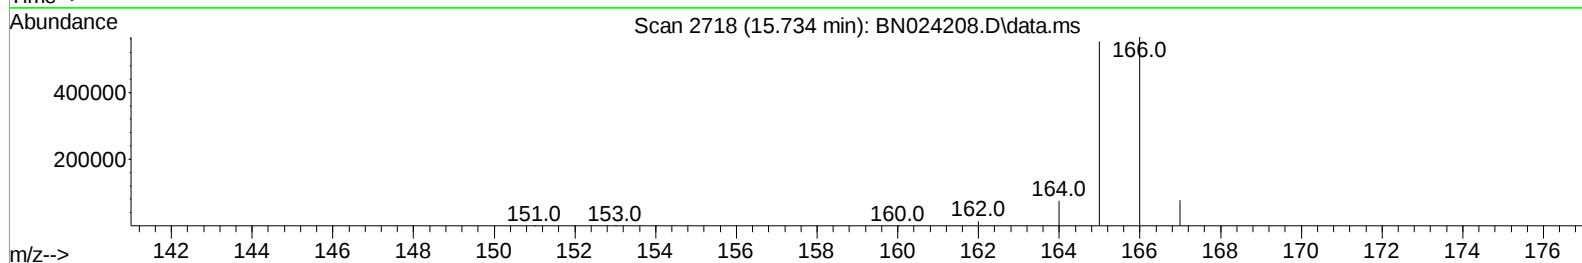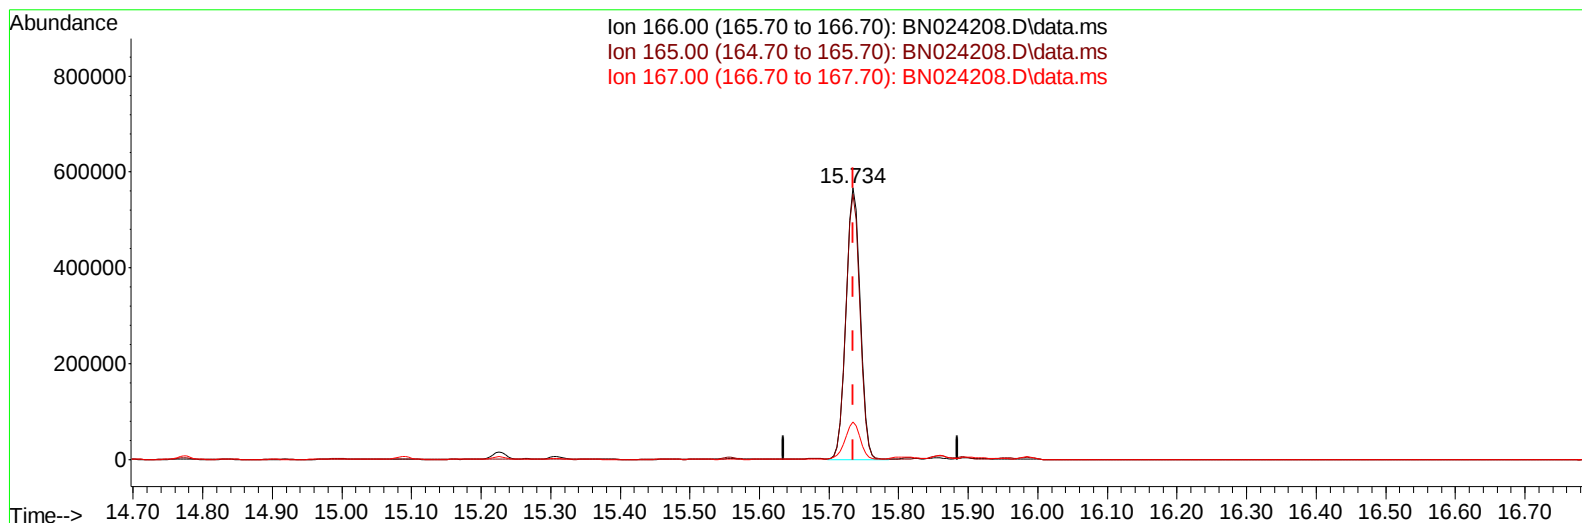

TIC: BN024208.D\data.ms

(12) Fluorene

15.734min (+ 0.000) 11.86 ng/ul m

response 810780

Ion	Exp%	Act%
166.00	100.00	100.00
165.00	96.70	97.64
167.00	13.60	13.74
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

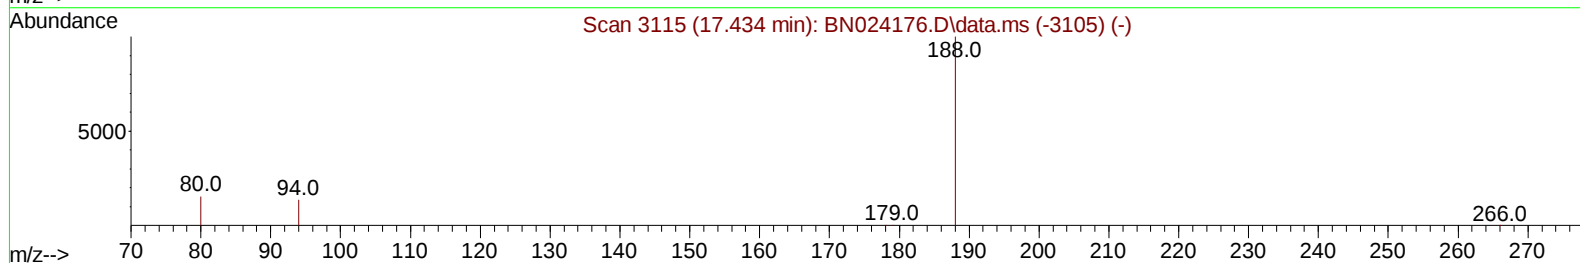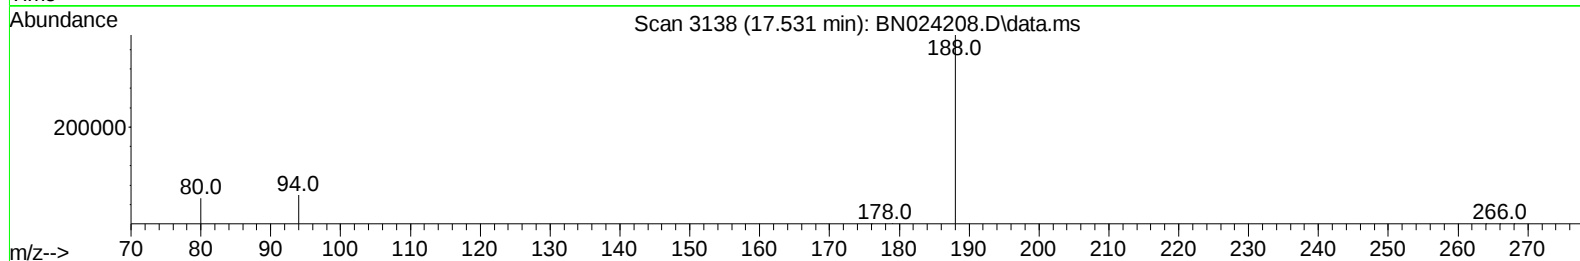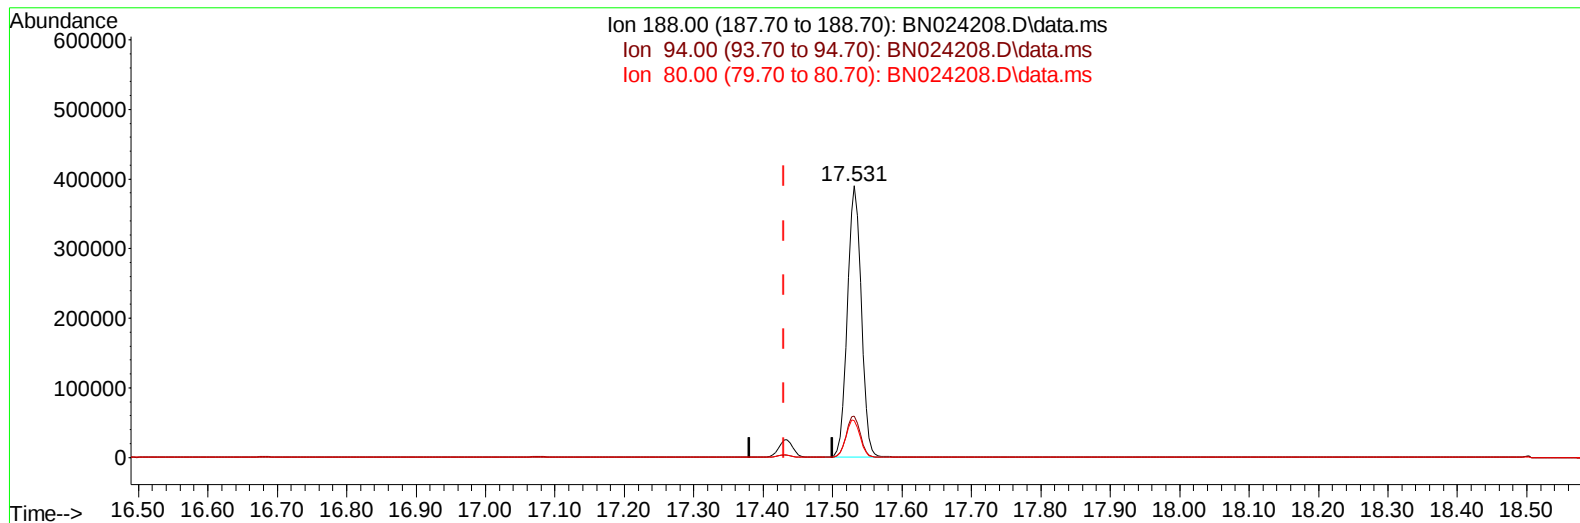

TIC: BN024208.D\data.ms

(13) Phenanthrene-d10 (I)

17.531min (+ 0.101) 0.40 ng/u1

response 541829

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.00	15.25
80.00	14.30	13.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

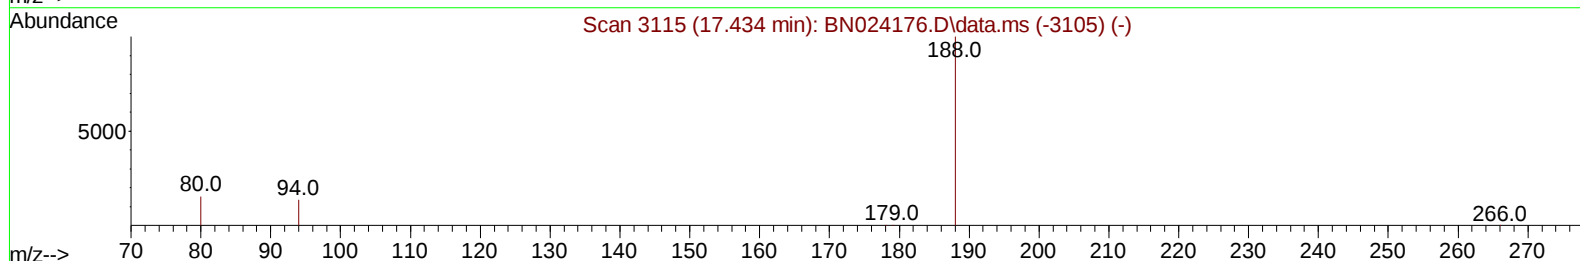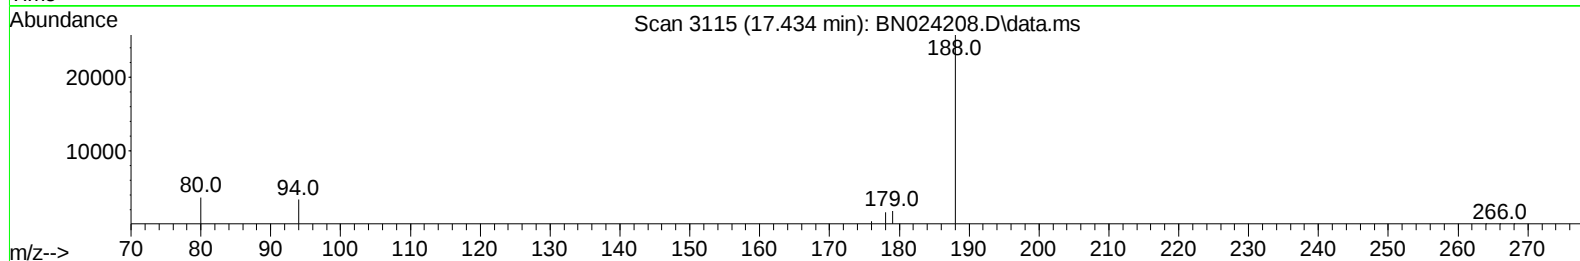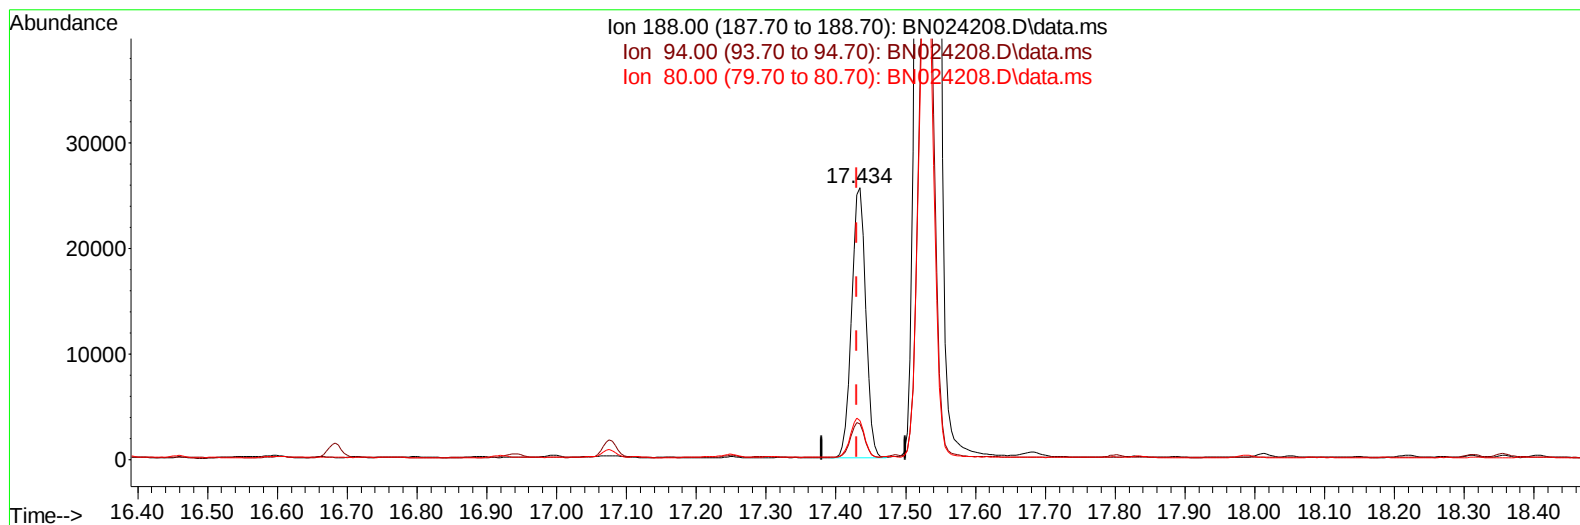

TIC: BN024208.D\data.ms

(13) Phenanthrene-d10 (I)

17.434min (+ 0.004) 0.40 ng/ul m

response 36055

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	13.00	13.01
80.00	14.30	14.17
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

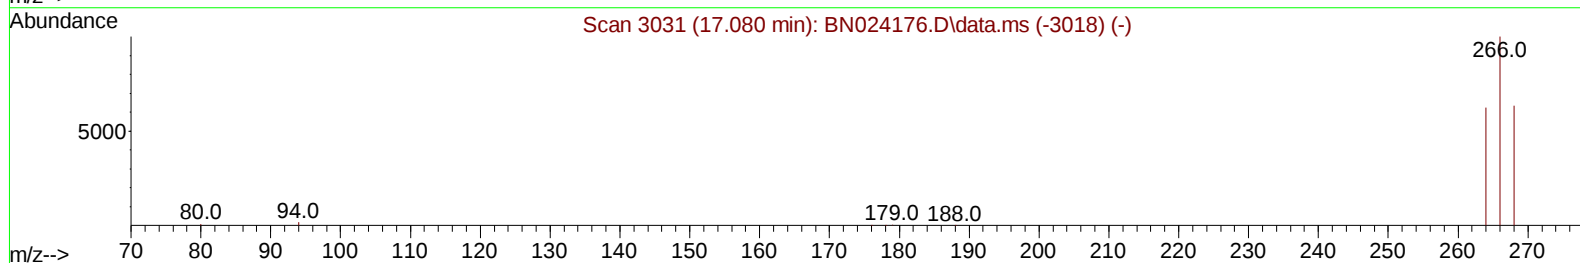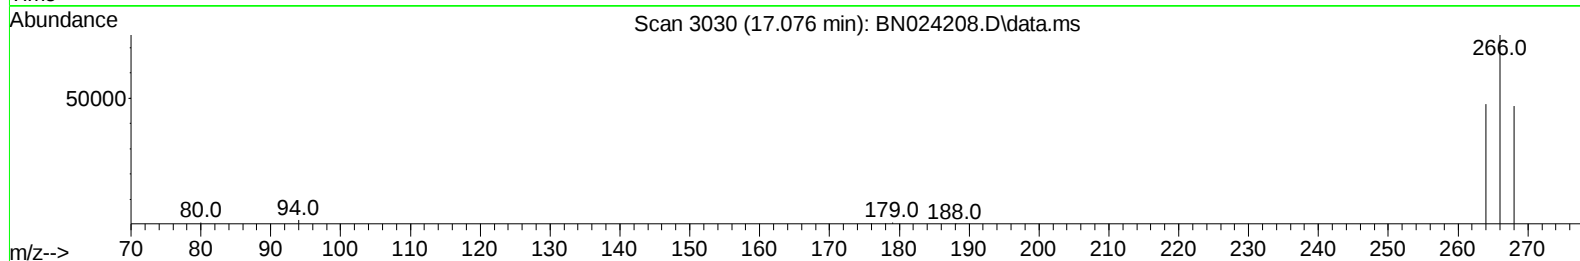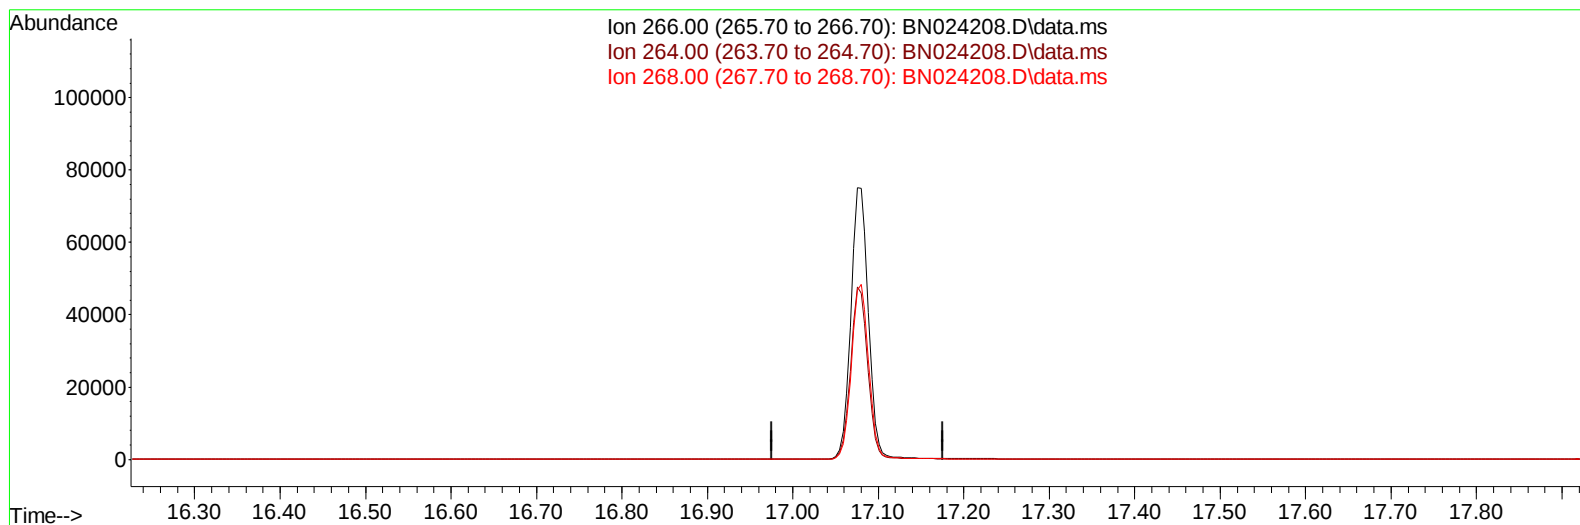

TIC: BN024208.D\data.ms

(14) Pentachlorophenol

17.075min (-17.075) 0.00 ng/u1

response 0

Ion	Exp%	Act%
266.00	100.00	0.00
264.00	0.00	0.00
268.00	0.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

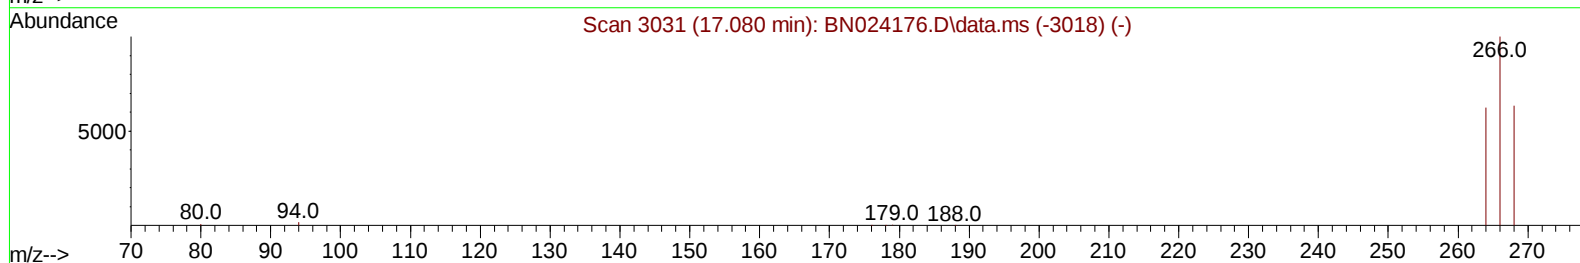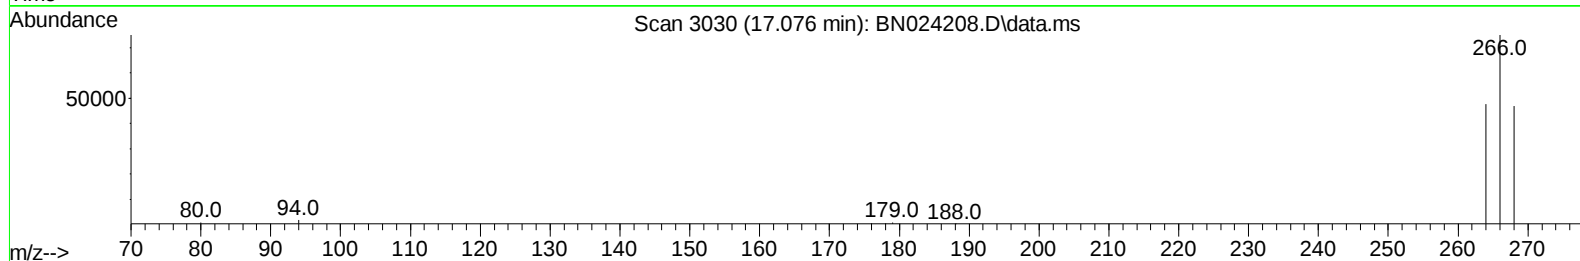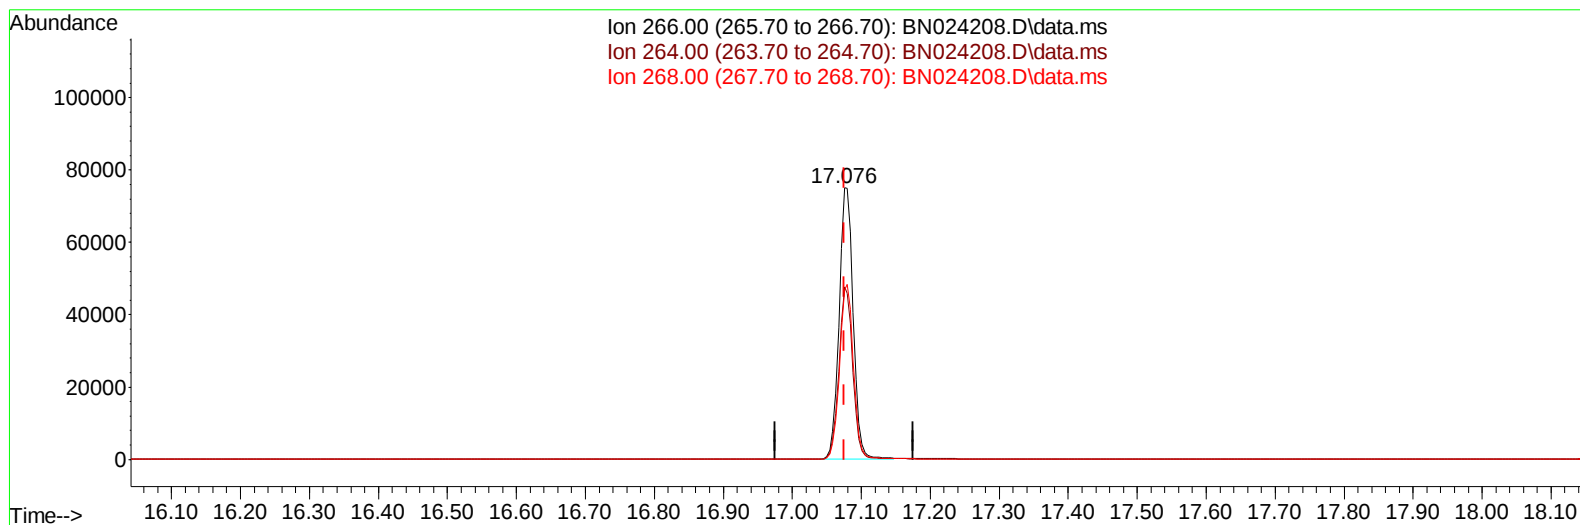

TIC: BN024208.D\data.ms

(14) Pentachlorophenol

17.076min (+ 0.000) 10.64 ng/ul m

response 106583

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	0.00	0.00
268.00	0.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

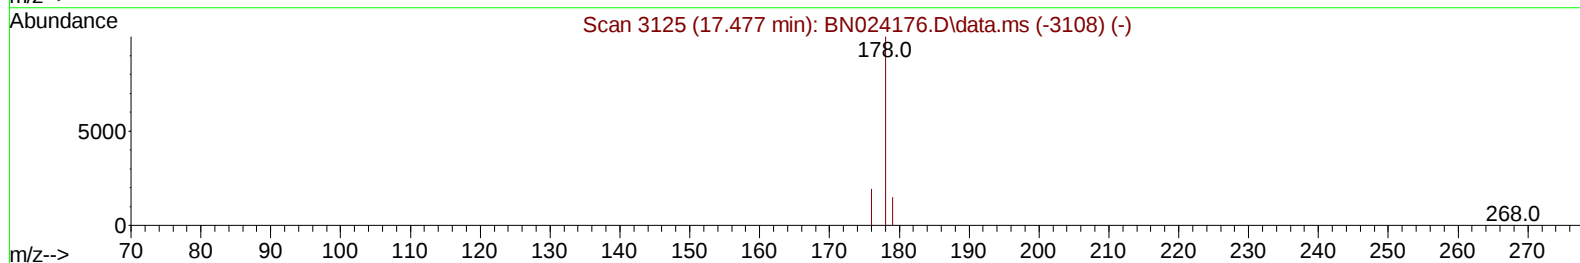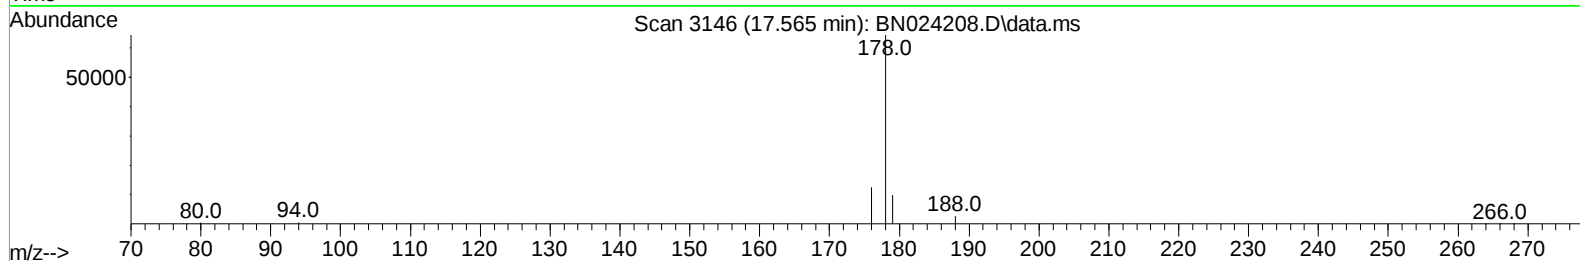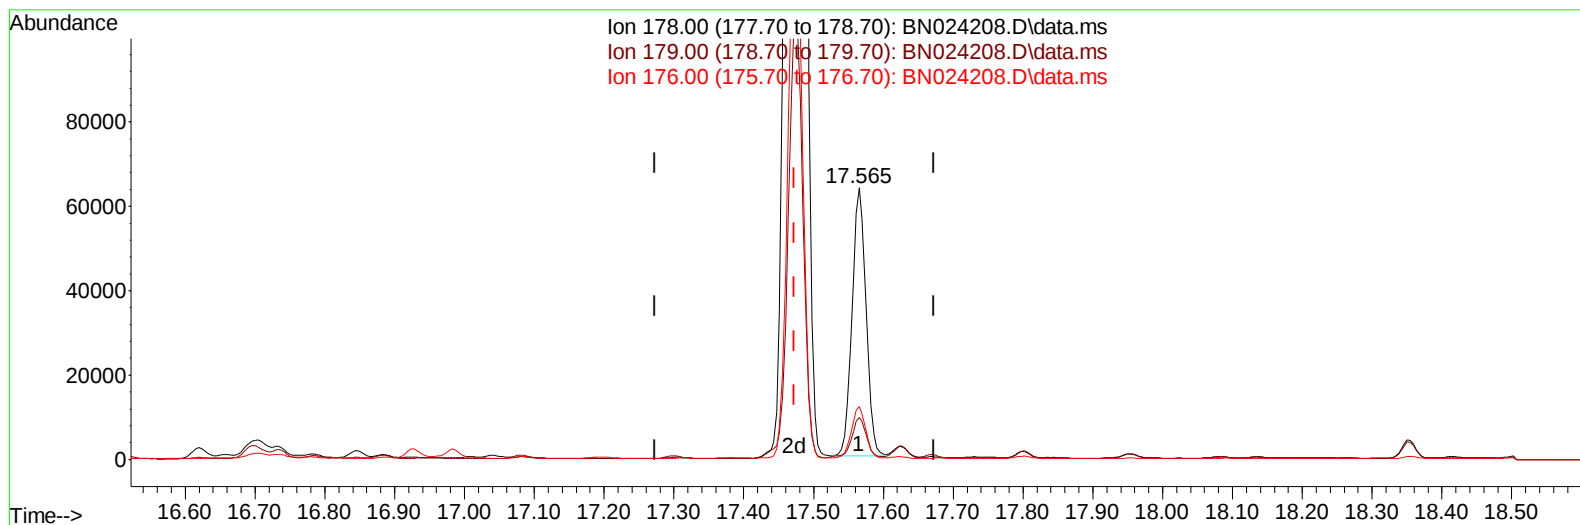

TIC: BN024208.D\data.ms

(15) Phenanthrene

17.565min (+ 0.093) 0.85 ng/u1

response 88059

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.20	15.48
176.00	19.60	19.46
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

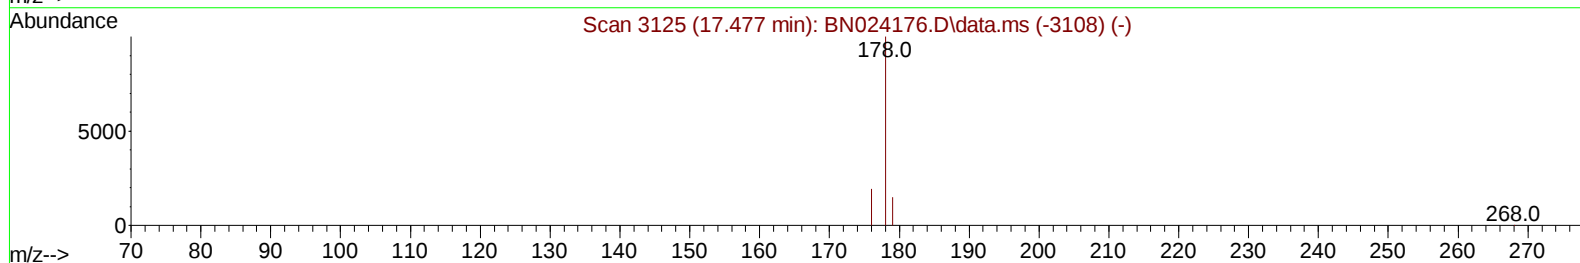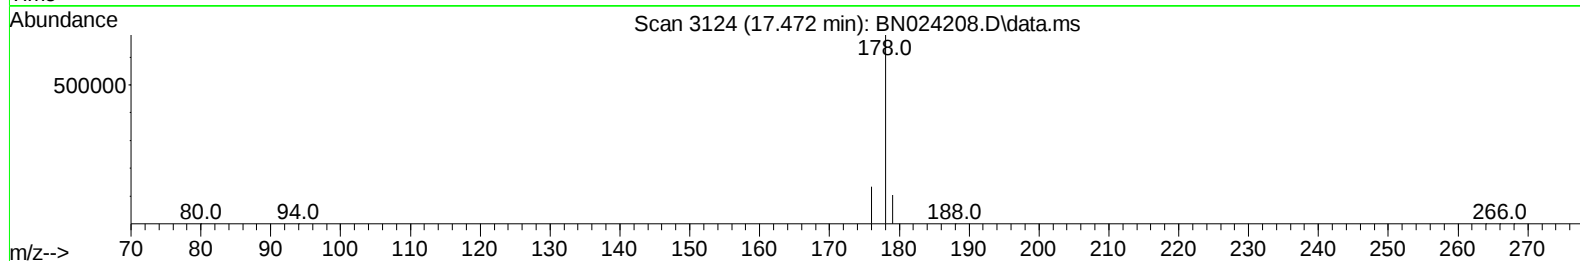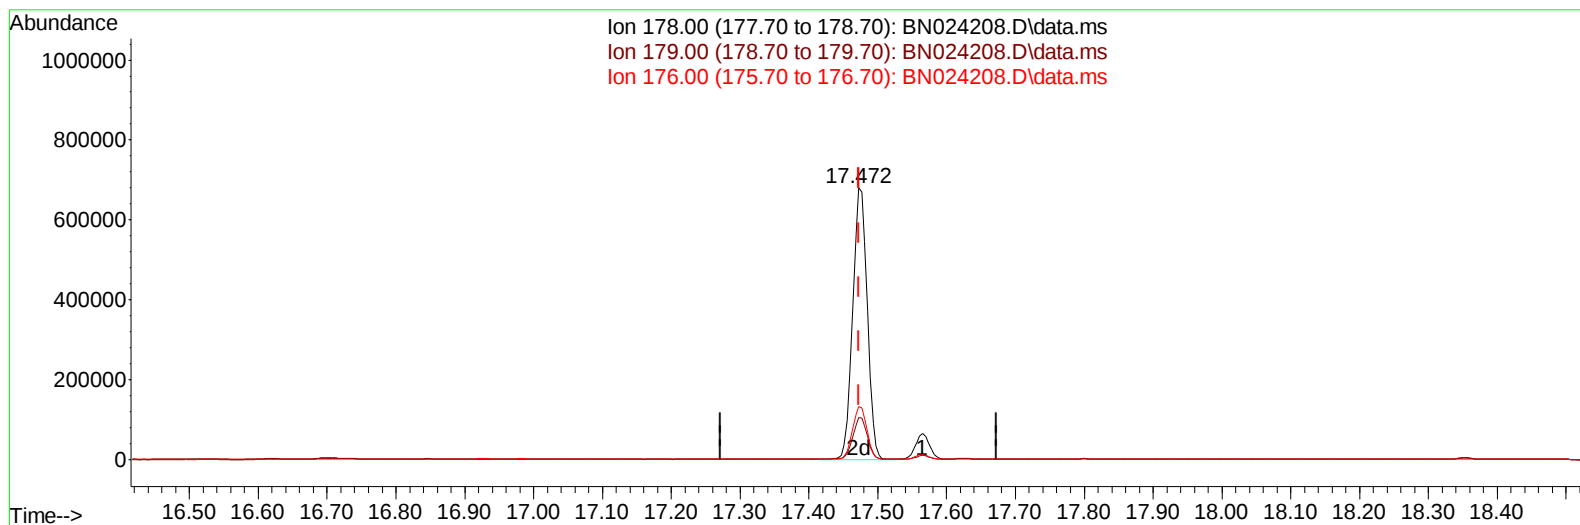

TIC: BN024208.D\data.ms

(15) Phenanthrene

17.472min (+ 0.000) 9.64 ng/ul m

response 995902

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.20	15.39
176.00	19.60	19.58
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024208.D
Acq On : 09 Mar 2023 20:18
Operator : CG/JU
Sample : 01746-01DL 5X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

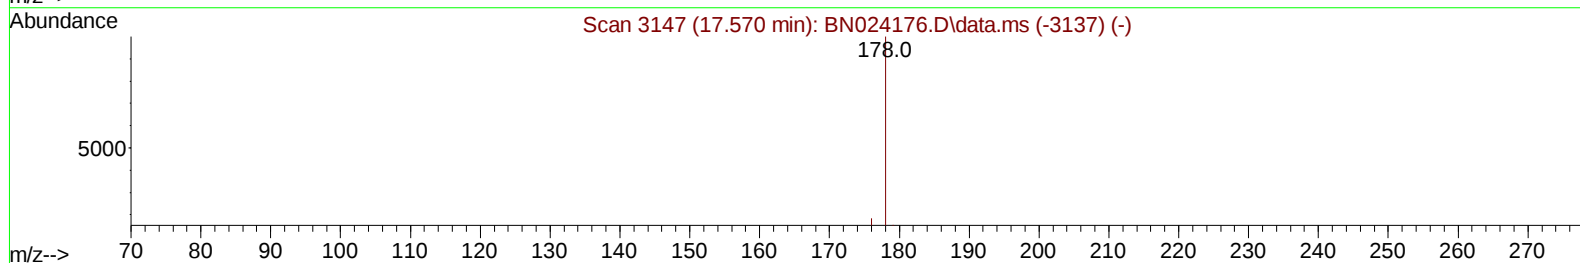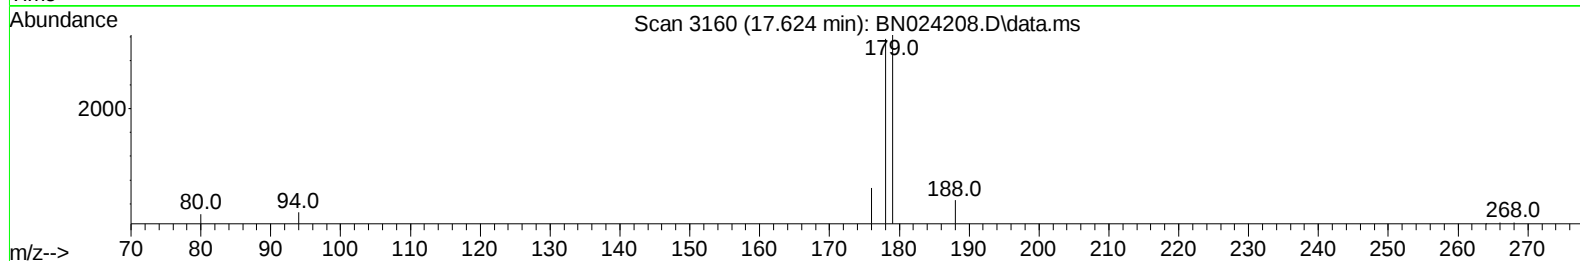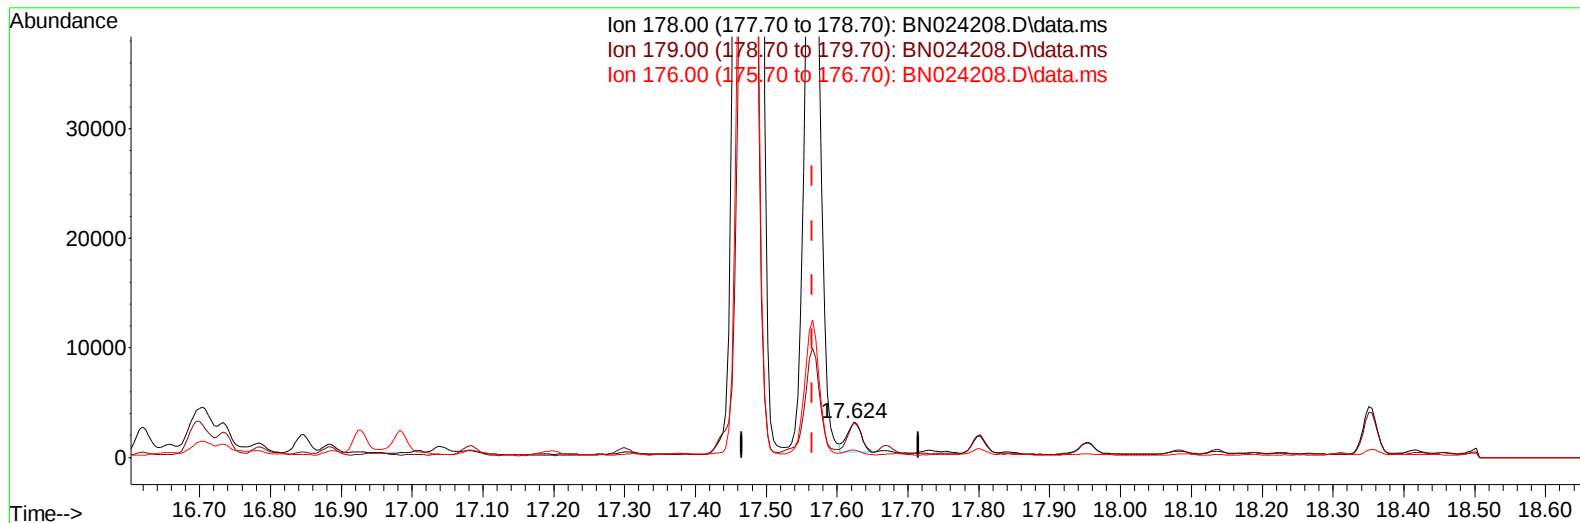

TIC: BN024208.D\data.ms

(16) Anthracene

17.624min (+ 0.059) 0.04 ng/u1

response 3697

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.40	101.86#
176.00	19.10	21.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024208.D
Acq On : 09 Mar 2023 20:18
Operator : CG/JU
Sample : 01746-01DL 5X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

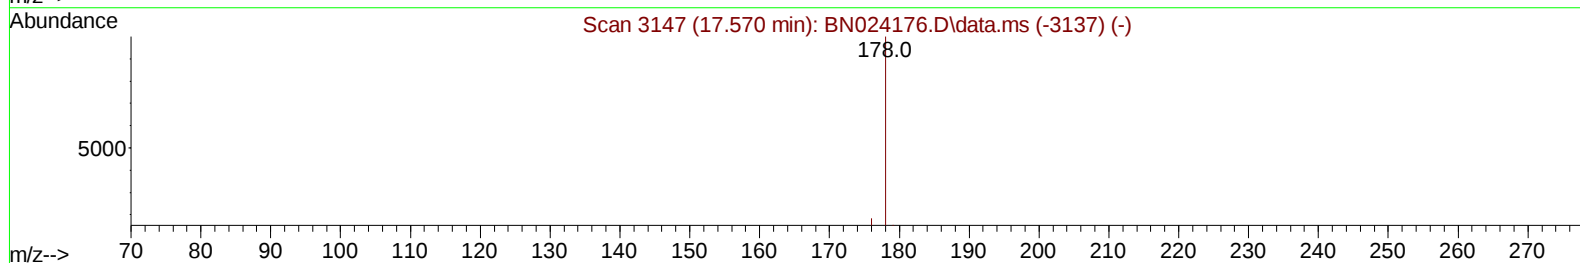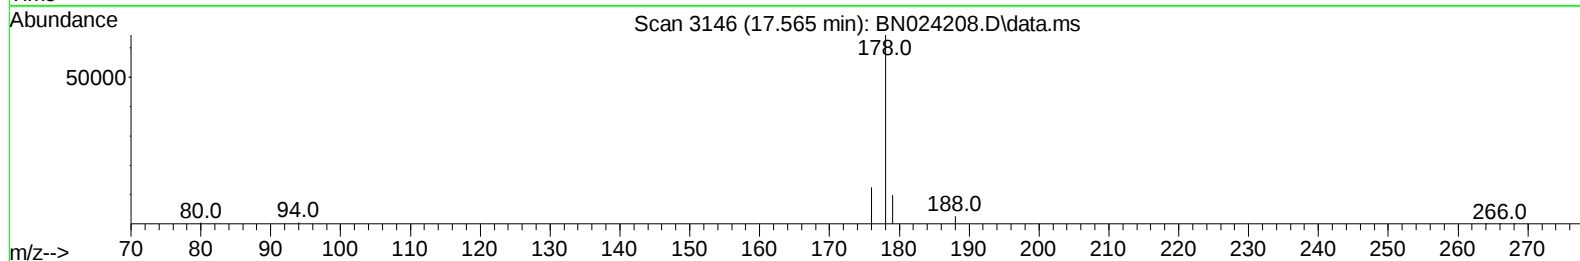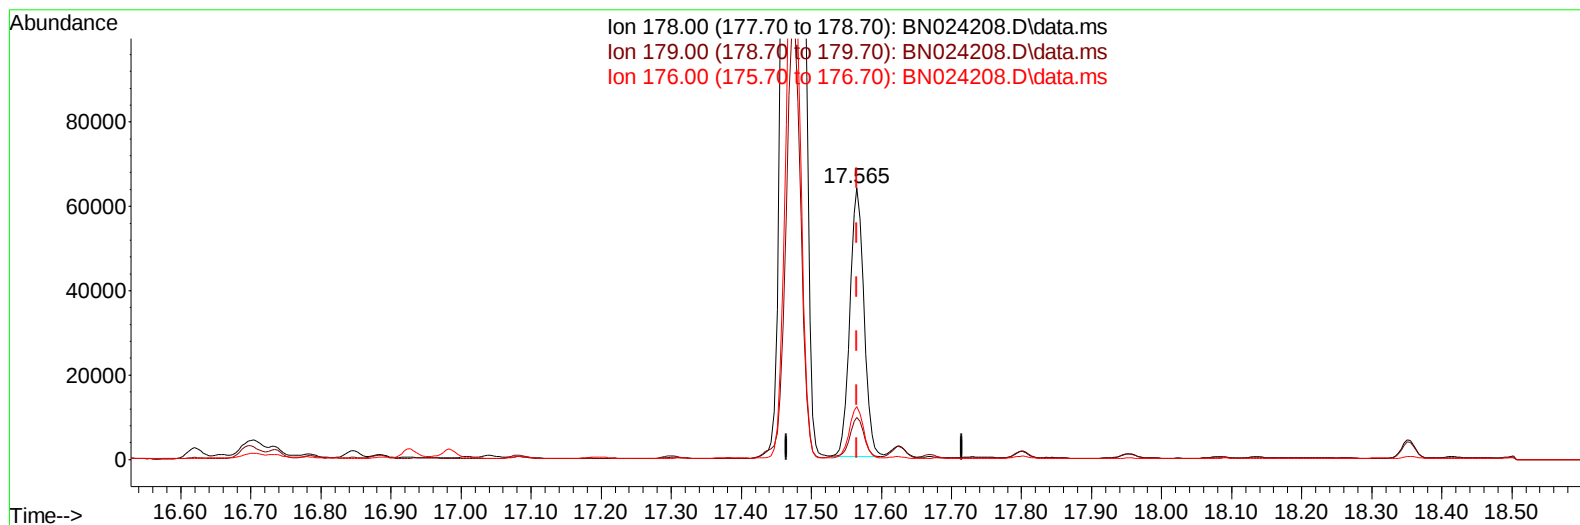

TIC: BN024208.D\data.ms

(16) Anthracene

17.565min (+ 0.000) 0.98 ng/ul m

response 88923

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.40	15.48
176.00	19.10	19.46
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

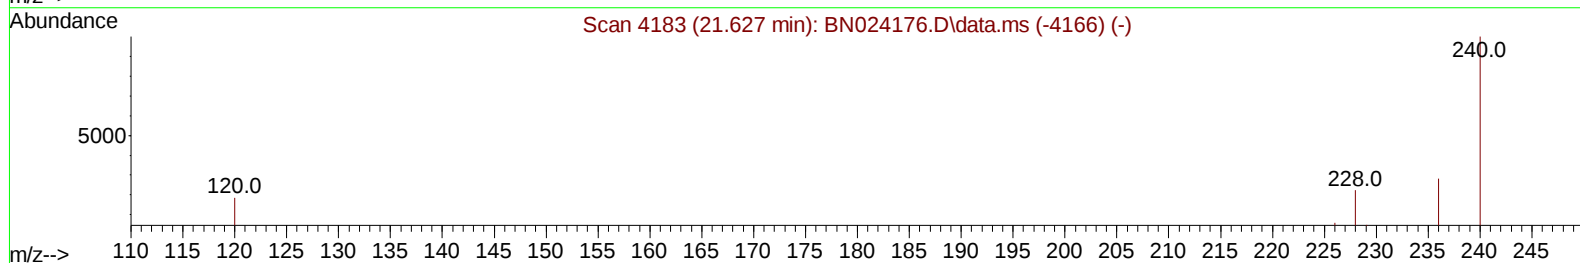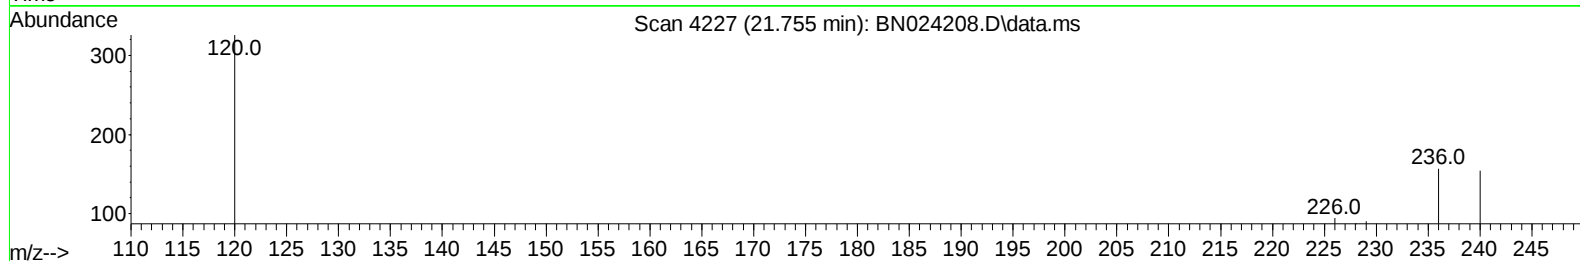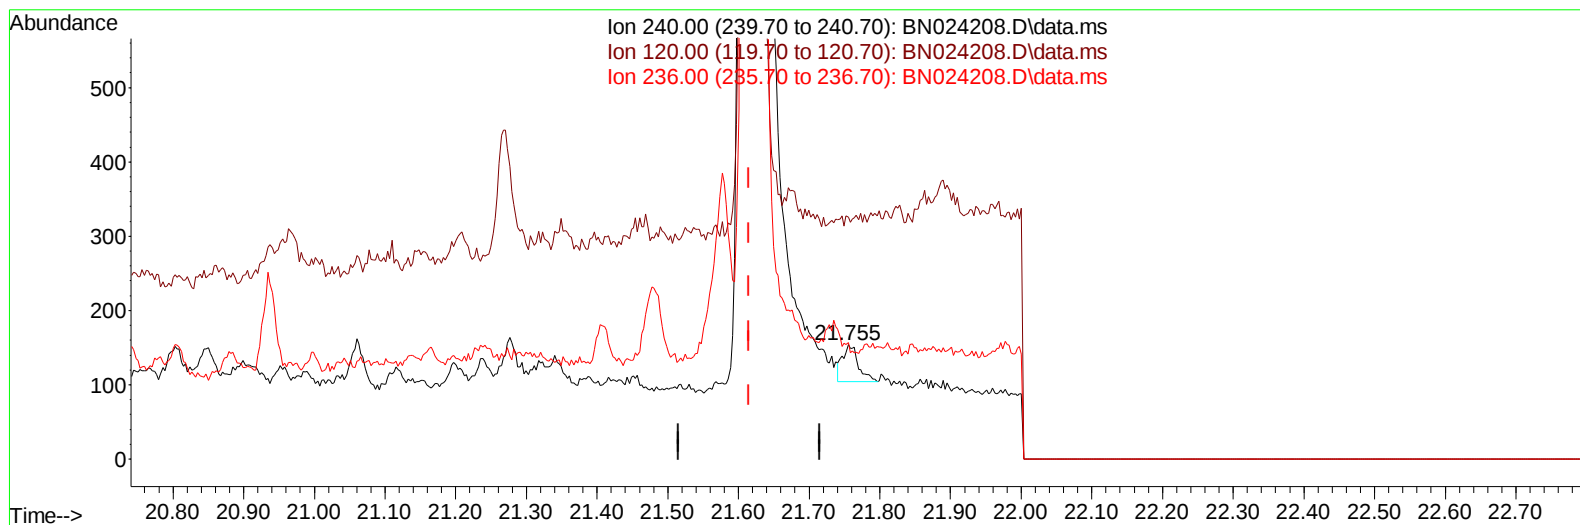

TIC: BN024208.D\data.ms

(17) Chrysene-d12

21.755min (+ 0.140) 0.40 ng/u1

response 78

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.10	211.69#
236.00	28.10	101.95#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

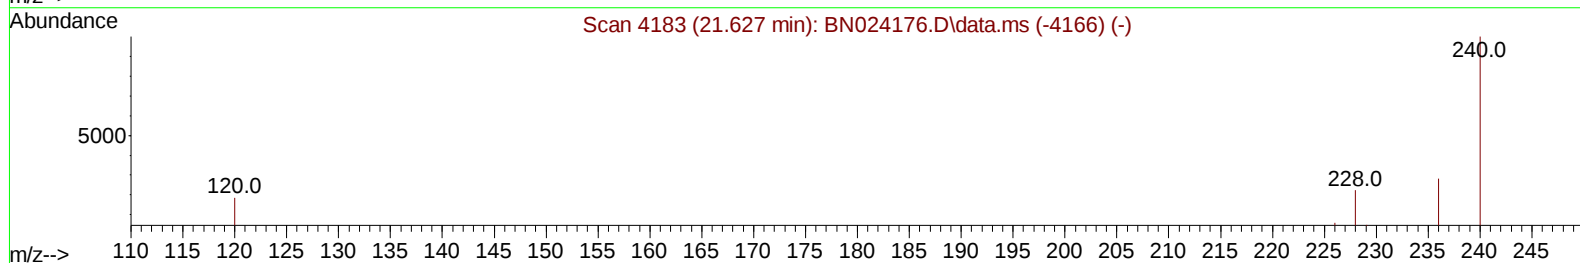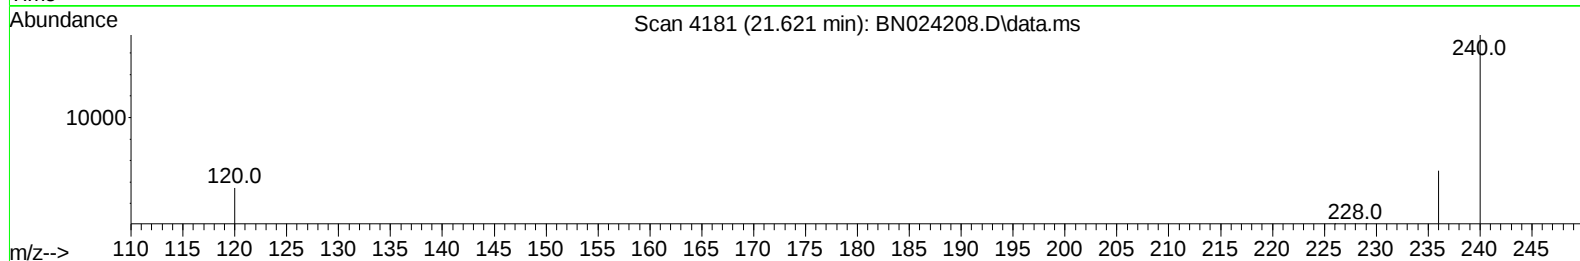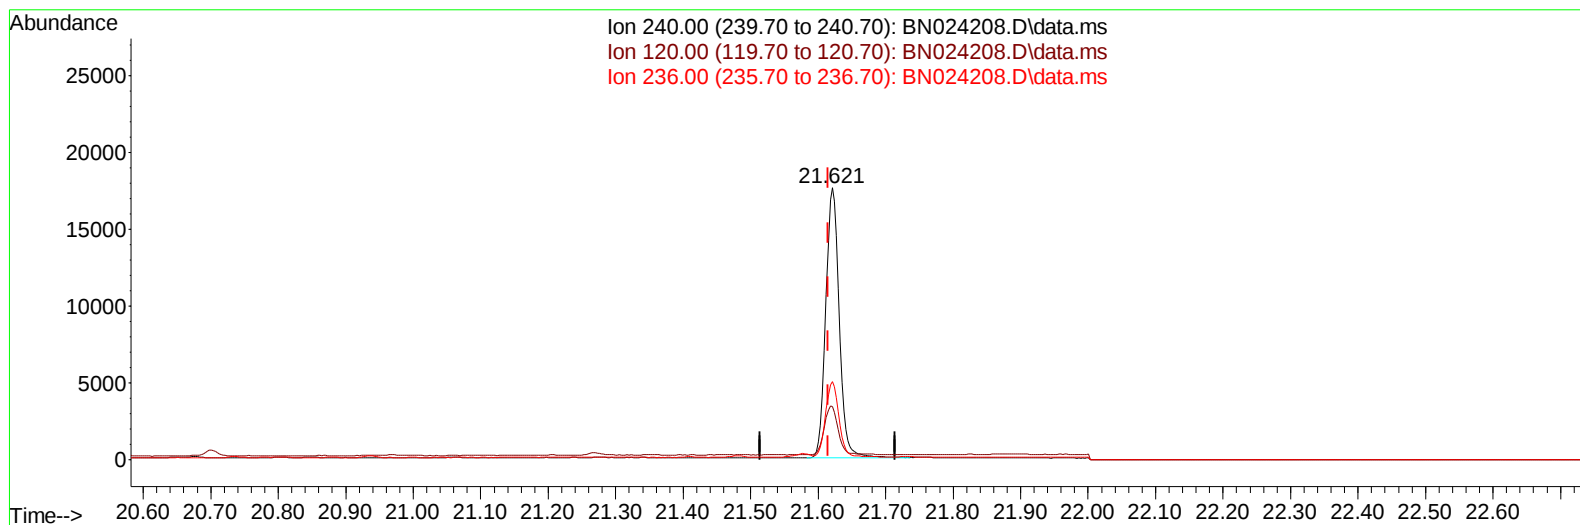

TIC: BN024208.D\data.ms

(17) Chrysene-d12

21.621min (+ 0.006) 0.40 ng/ul m

response 24513

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.10	19.40
236.00	28.10	28.56
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

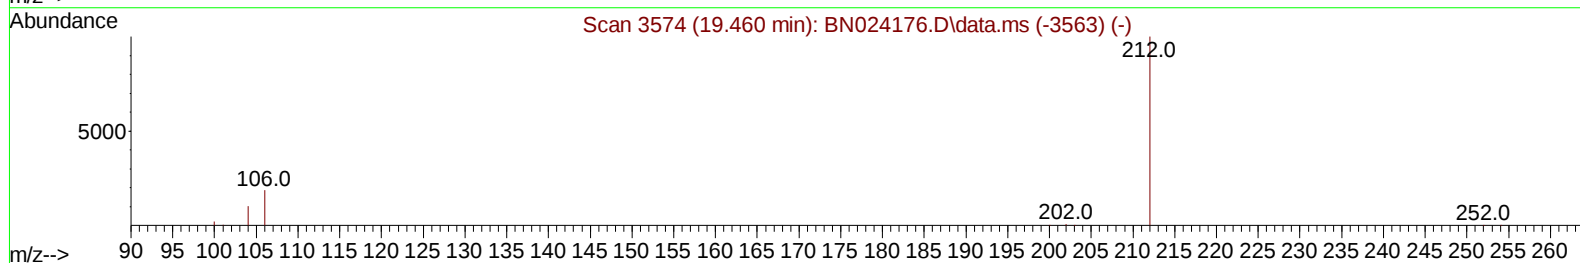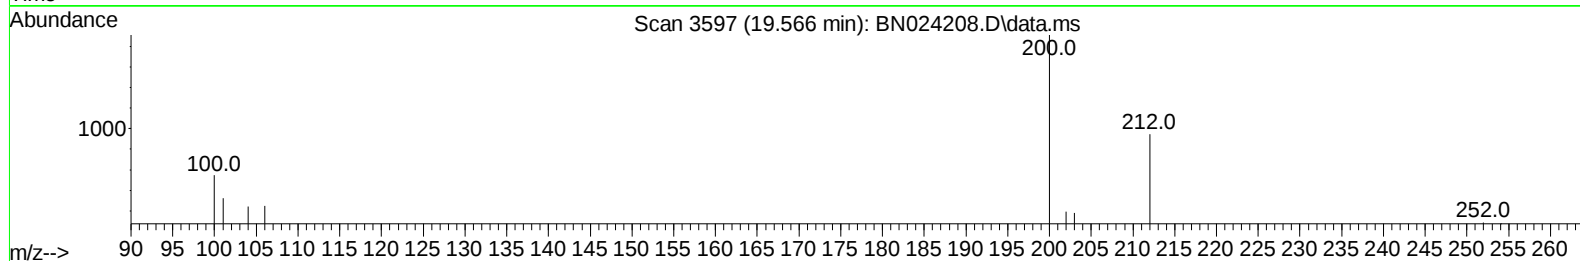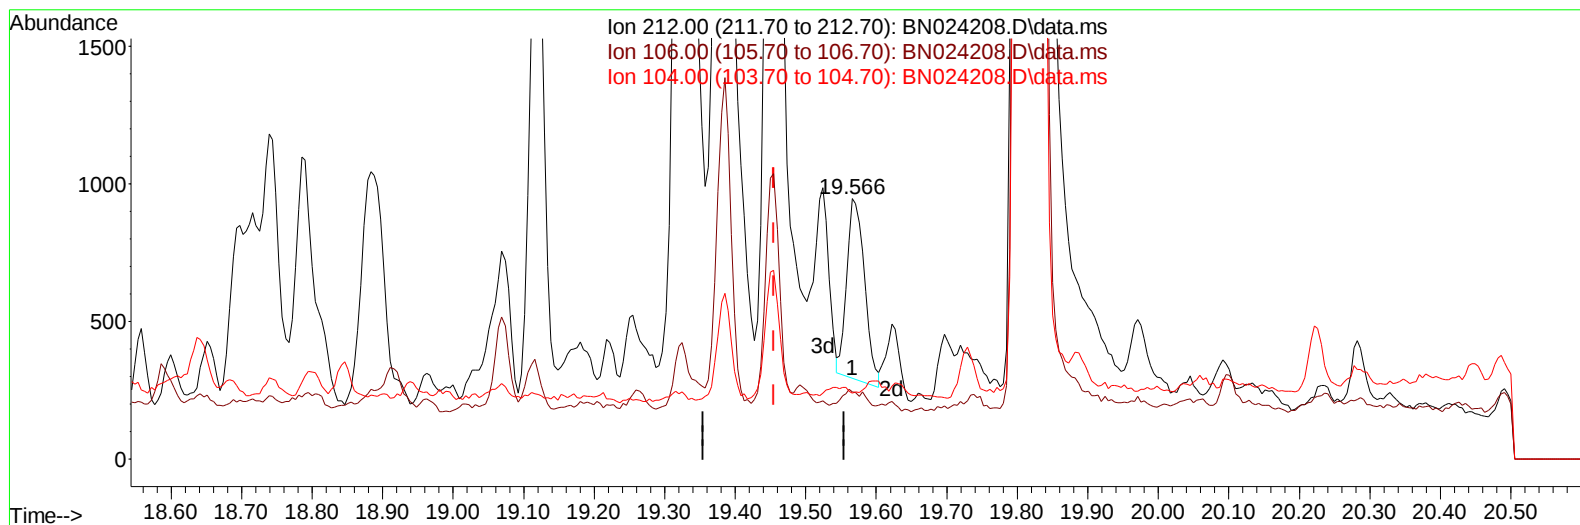

TIC: BN024208.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.566min (+ 0.112) 0.02 ng/u1

response 1142

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	0.00	11.82#
104.00	0.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024208.D
Acq On : 09 Mar 2023 20:18
Operator : CG/JU
Sample : 01746-01DL 5X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

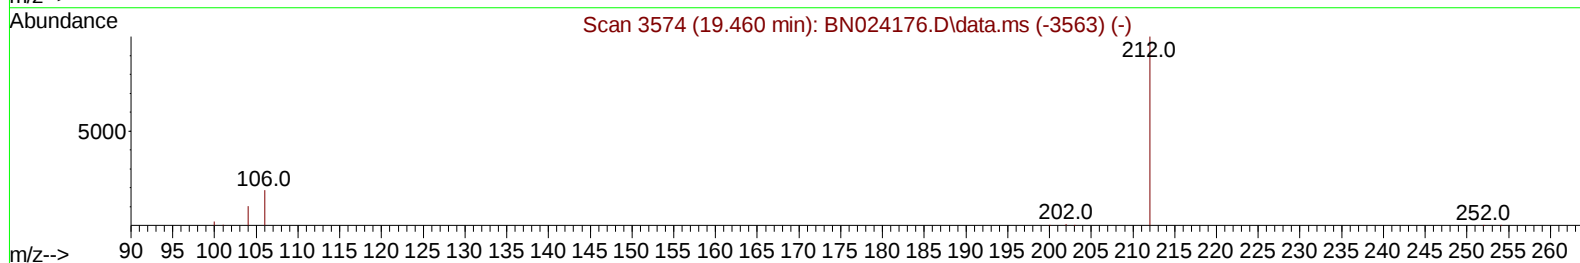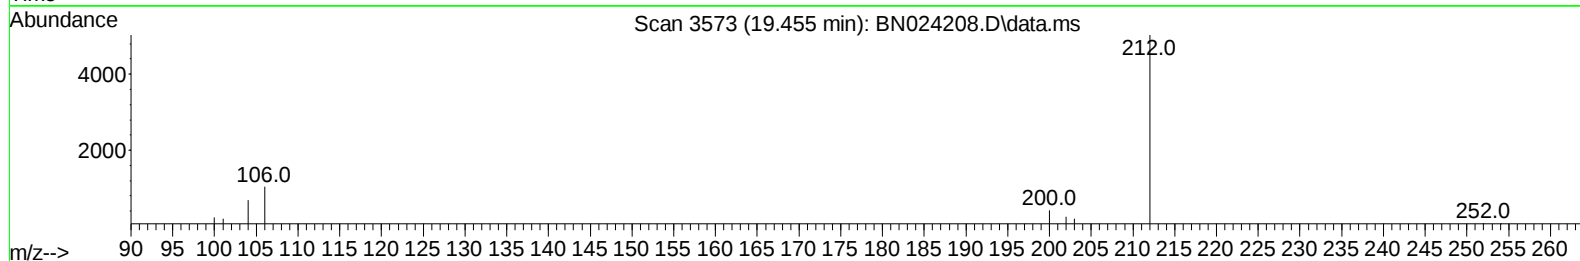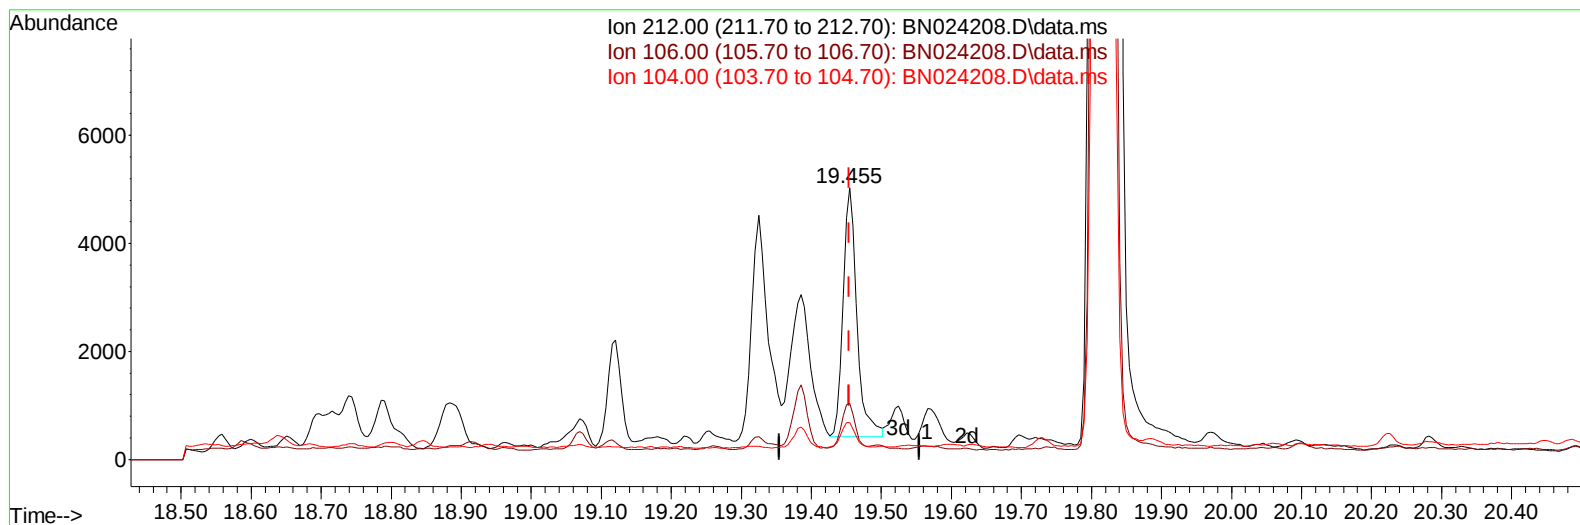

TIC: BN024208.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.455min (+ 0.000) 0.10 ng/u1 m

response 6396

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	0.00	2.11#
104.00	0.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024208.D
Acq On : 09 Mar 2023 20:18
Operator : CG/JU
Sample : 01746-01DL 5X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

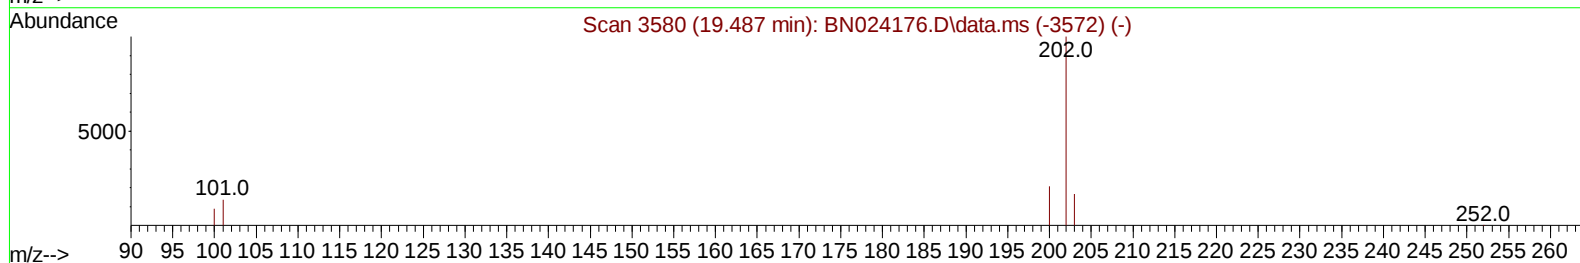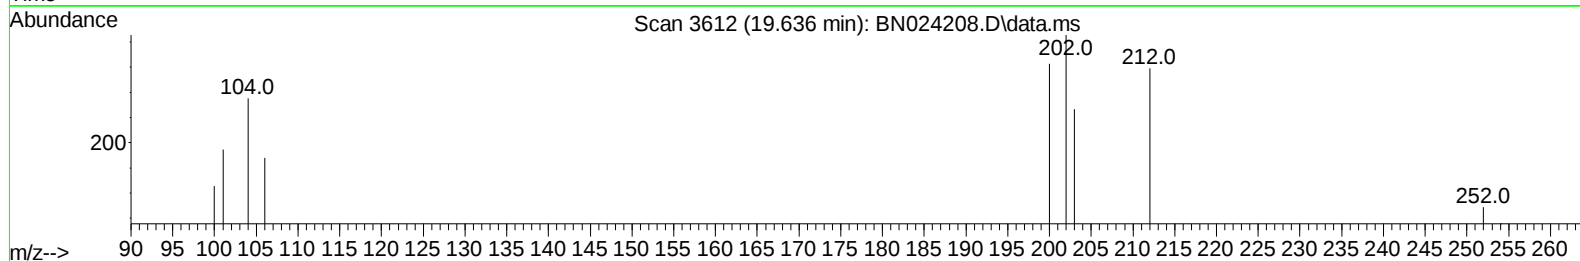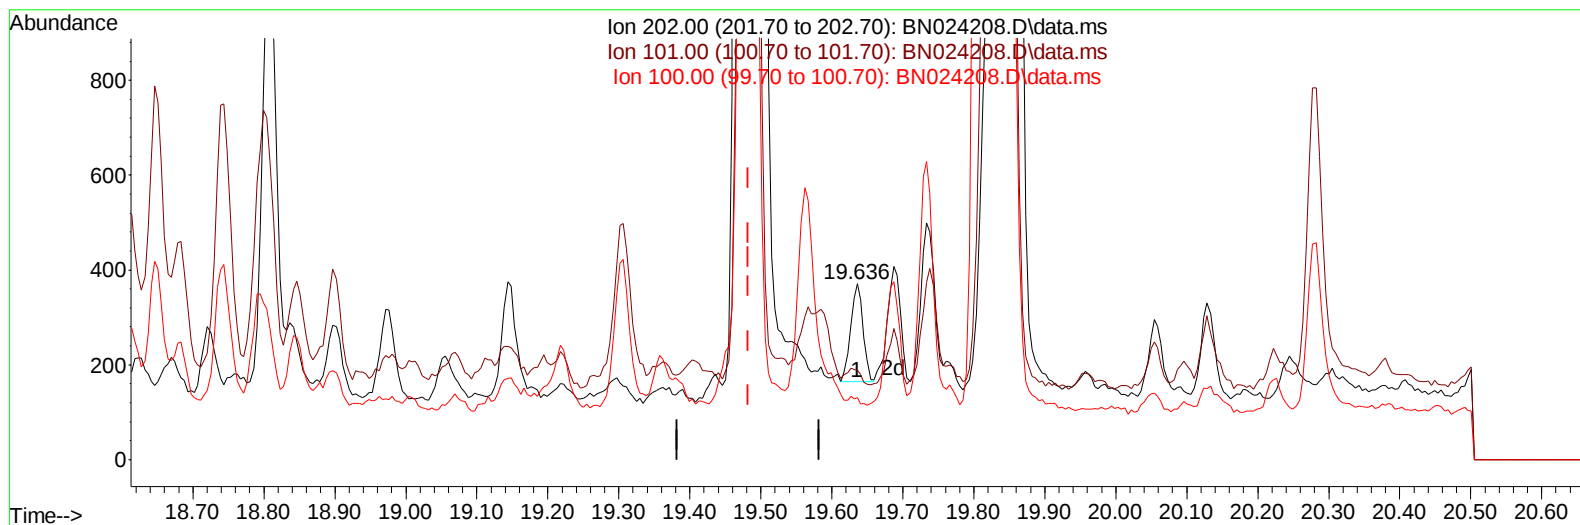

TIC: BN024208.D\data.ms

(19) Fluoranthene (C)

19.636min (+ 0.153) 0.00 ng/u1

response 253

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.00	50.94#
100.00	9.60	35.31#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

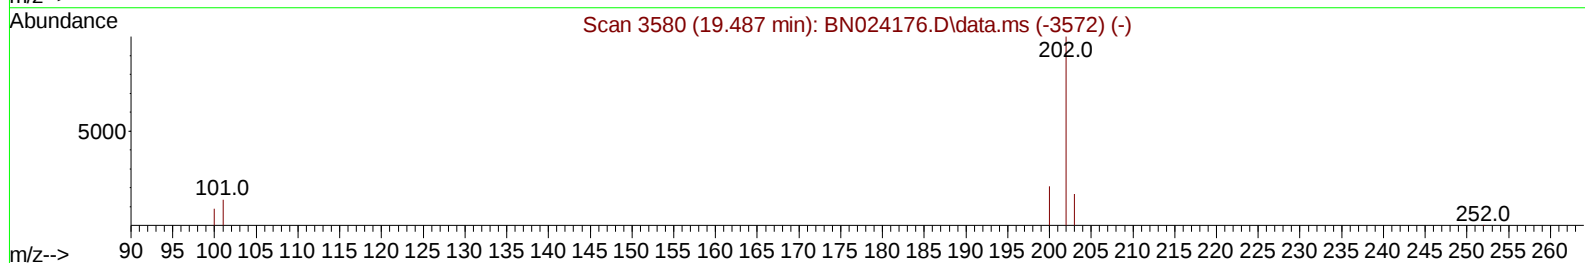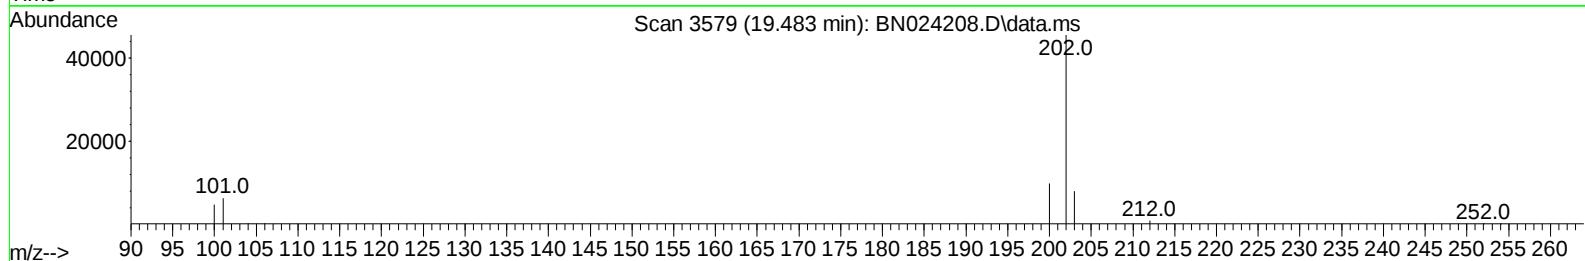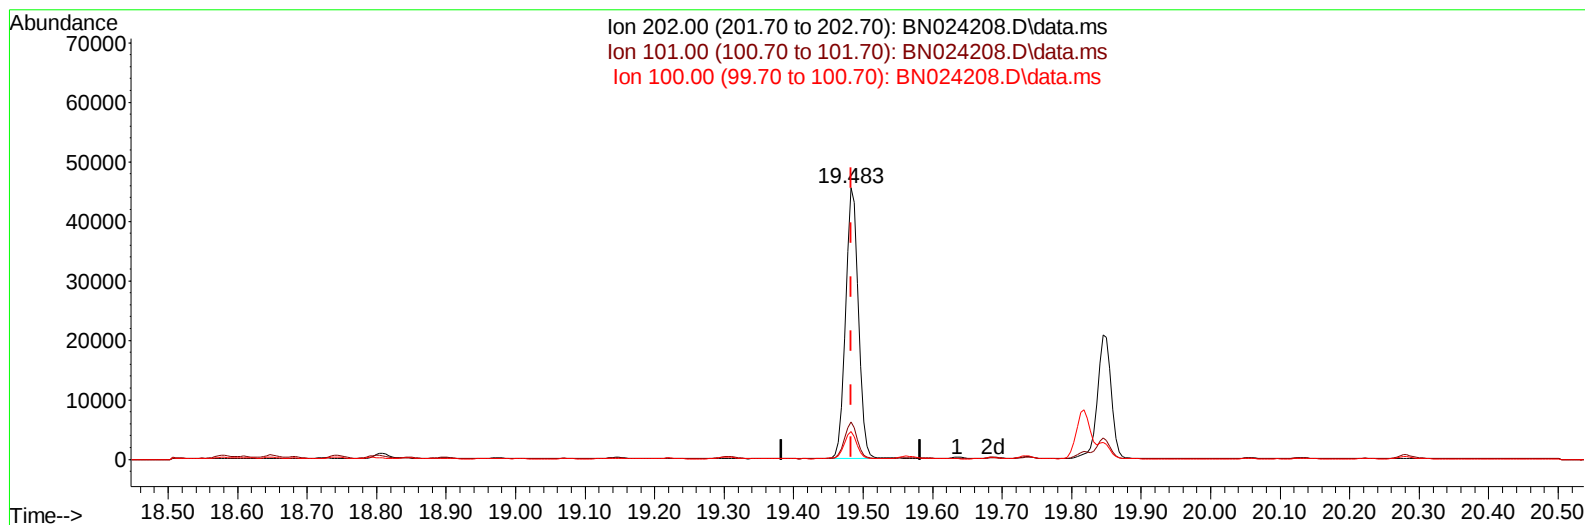

TIC: BN024208.D\data.ms

(19) Fluoranthene (C)

19.483min (+ 0.000) 0.60 ng/ul m

response 58602

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.00	13.84
100.00	9.60	10.31
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

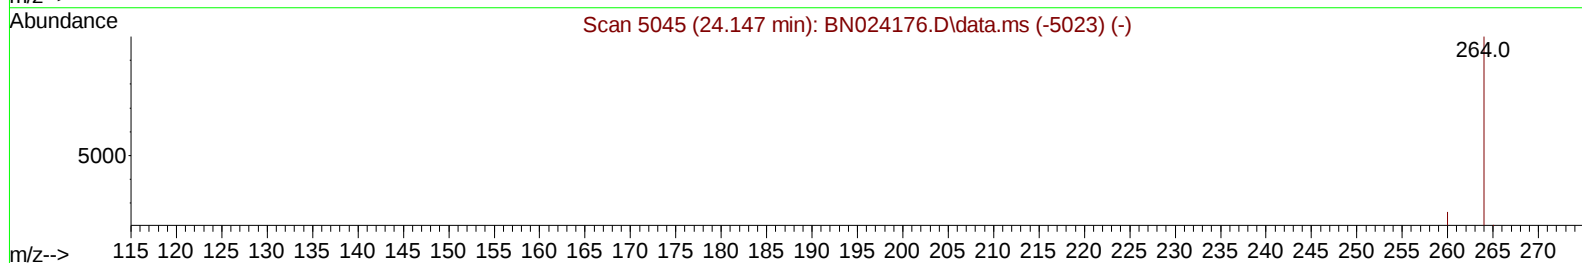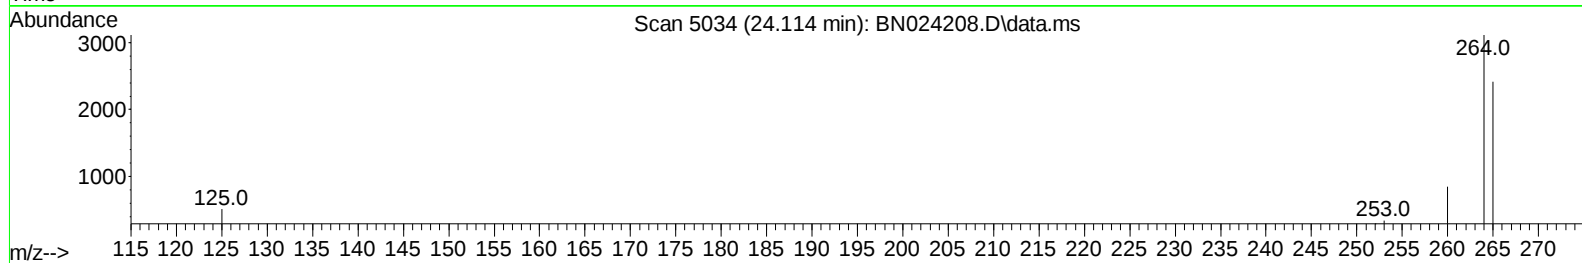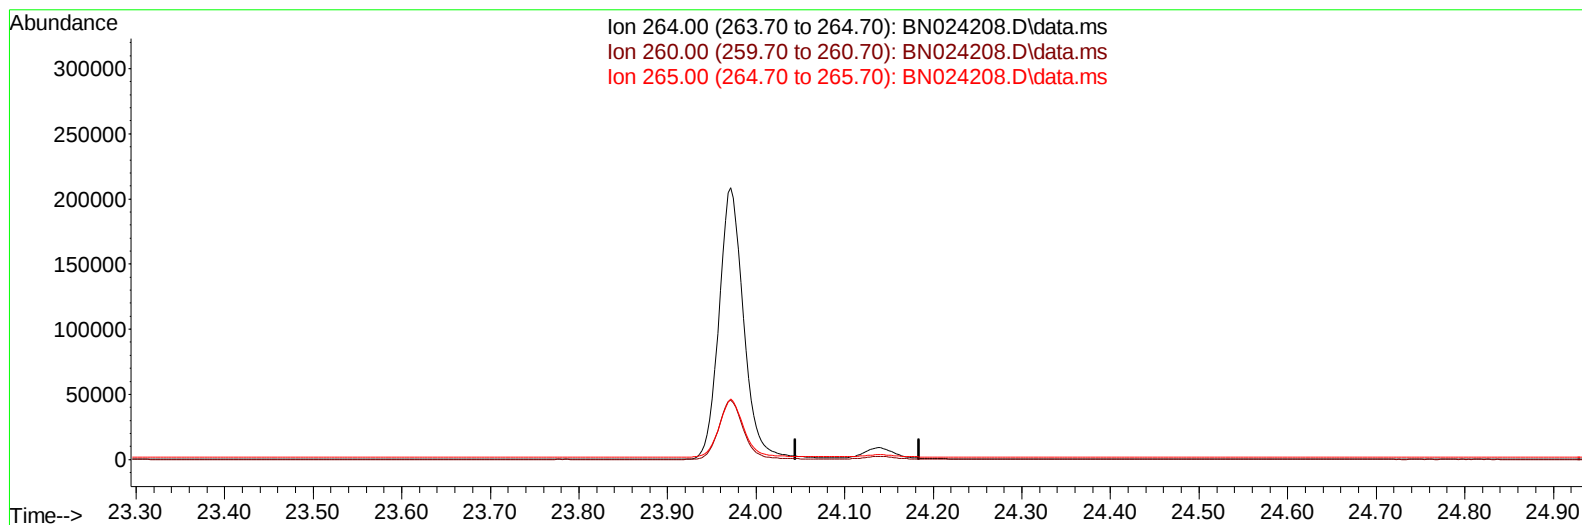

TIC: BN024208.D\data.ms

(23) Perylene-d12 (I)

24.114min (-24.114) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	26.80	0.00#
265.00	38.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

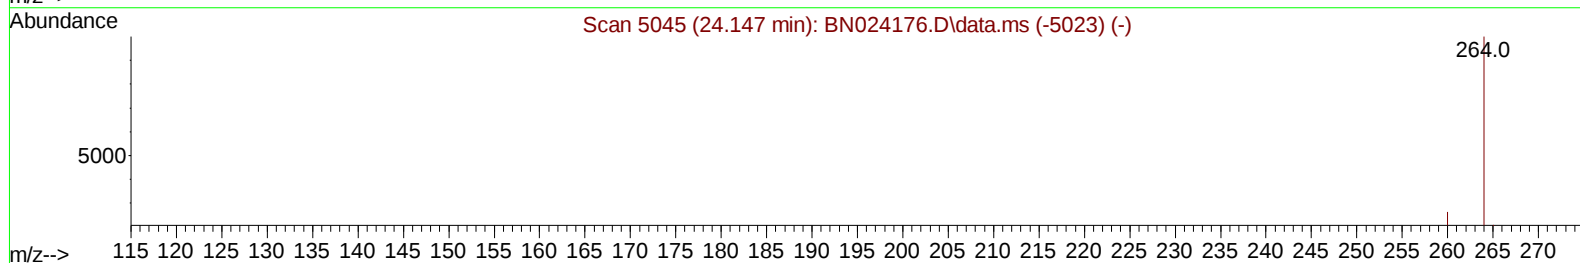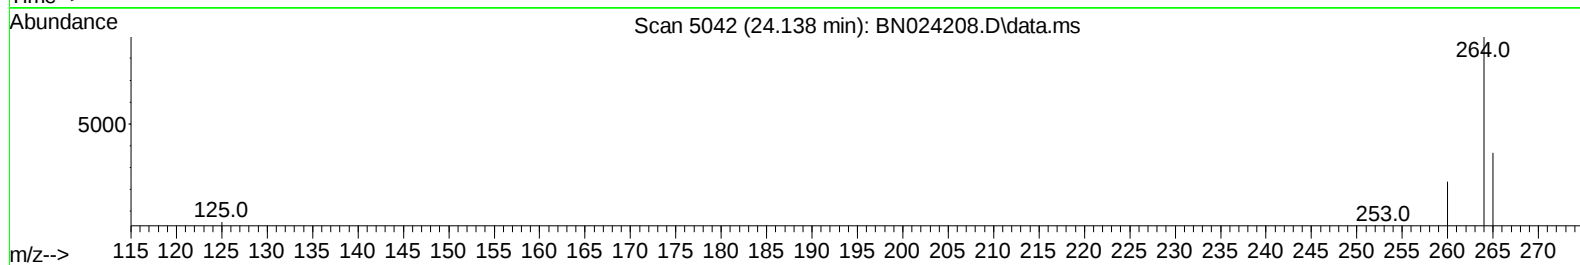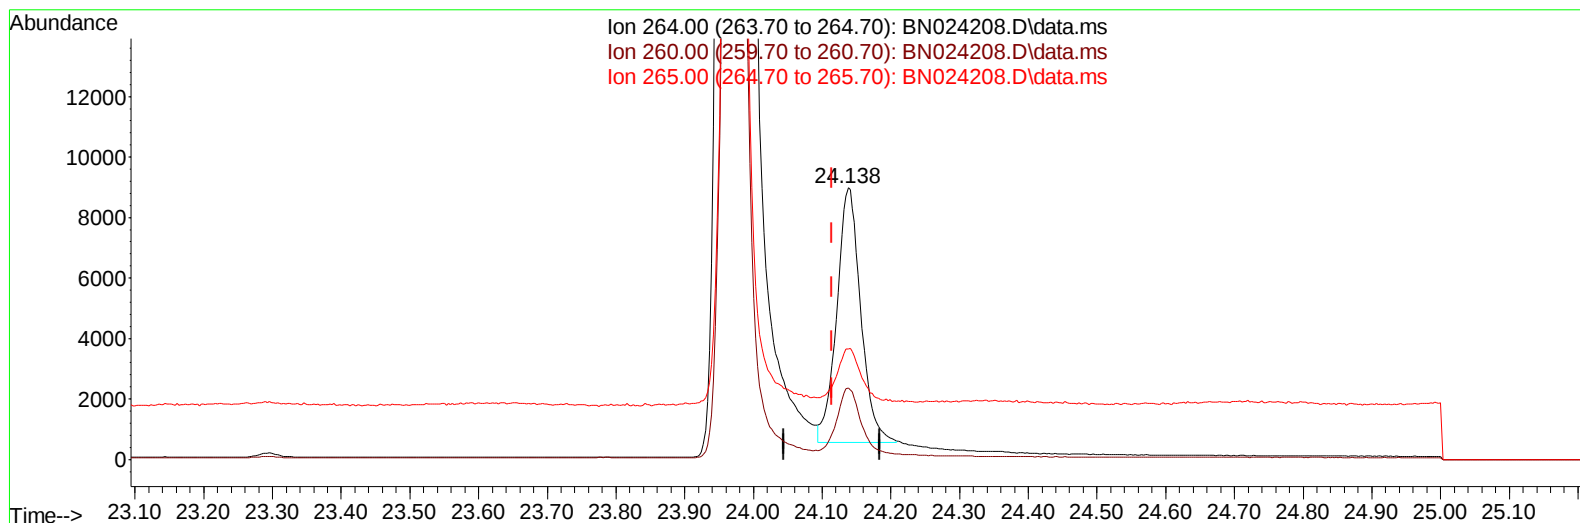

TIC: BN024208.D\data.ms

(23) Perylene-d12 (I)

24.138min (+ 0.023) 0.40 ng/ul m

response 20382

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	26.25
265.00	38.30	40.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024208.D
 Acq On : 09 Mar 2023 20:18
 Operator : CG/JU
 Sample : 01746-01DL 5X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC1DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 03:22:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.055	152		9865	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136		30494	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164		19052m	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188		36055m	0.400	ng/ul	0.00
17) Chrysene-d12	21.621	240		24513m	0.400	ng/ul	0.00
23) Perylene-d12	24.138	264		20382m	0.400	ng/ul	0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.410	96		5060	0.466	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152		3074	0.085	ng/ul	0.00
18) Fluoranthene-d10	19.455	212		6396m	0.098	ng/ul	0.00
Target Compounds							
							Qvalue
5) Naphthalene	10.938	128	15951263	209.568	ng/ul		97
7) 2-Methylnaphthalene	12.528	142	1462478	31.671	ng/ul		100
8) 1-Methylnaphthalene	12.748	142	1063000	21.904	ng/ul		100
10) Acenaphthylene	14.411	152	167801	2.111	ng/ul		98
11) Acenaphthene	14.754	153	1546149	25.247	ng/ul		97
12) Fluorene	15.734	166	810780m	11.855	ng/ul		
14) Pentachlorophenol	17.076	266	106583m	10.643	ng/ul		
15) Phenanthrene	17.472	178	995902m	9.644	ng/ul		
16) Anthracene	17.565	178	88923m	0.981	ng/ul		
19) Fluoranthene	19.483	202	58602m	0.601	ng/ul		
20) Pyrene	19.845	202	28971	0.293	ng/ul		95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024208.D
Acq On : 09 Mar 2023 20:18
Operator : CG/JU
Sample : 01746-01DL 5X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAC1DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:22:25 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

