




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024209.D
 Acq On : 09 Mar 2023 20:55
 Operator : CG/JU
 Sample : 01746-05DL 5X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAD5DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:25:33 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

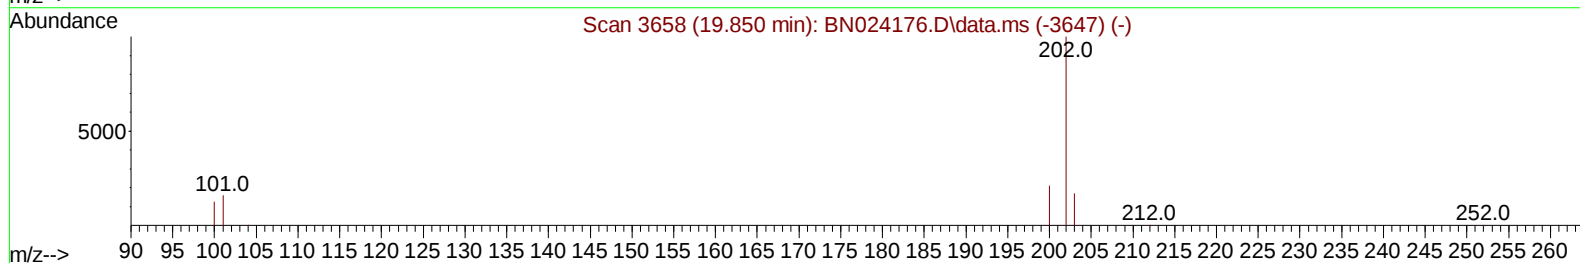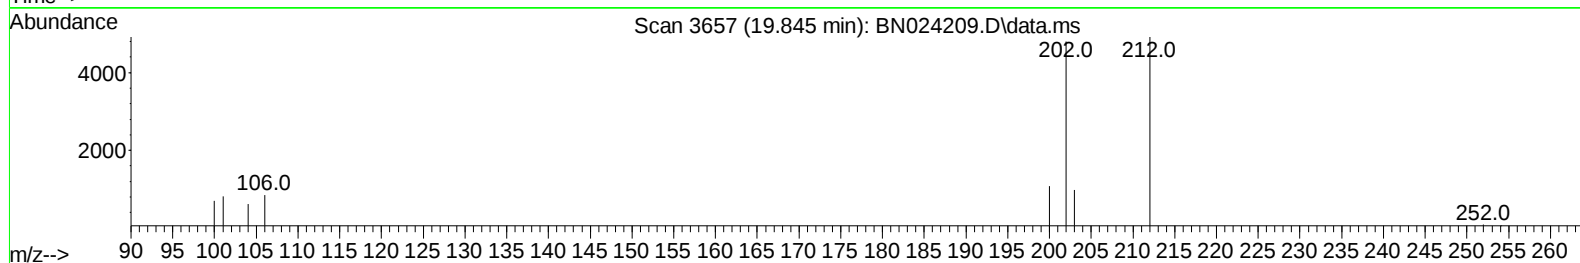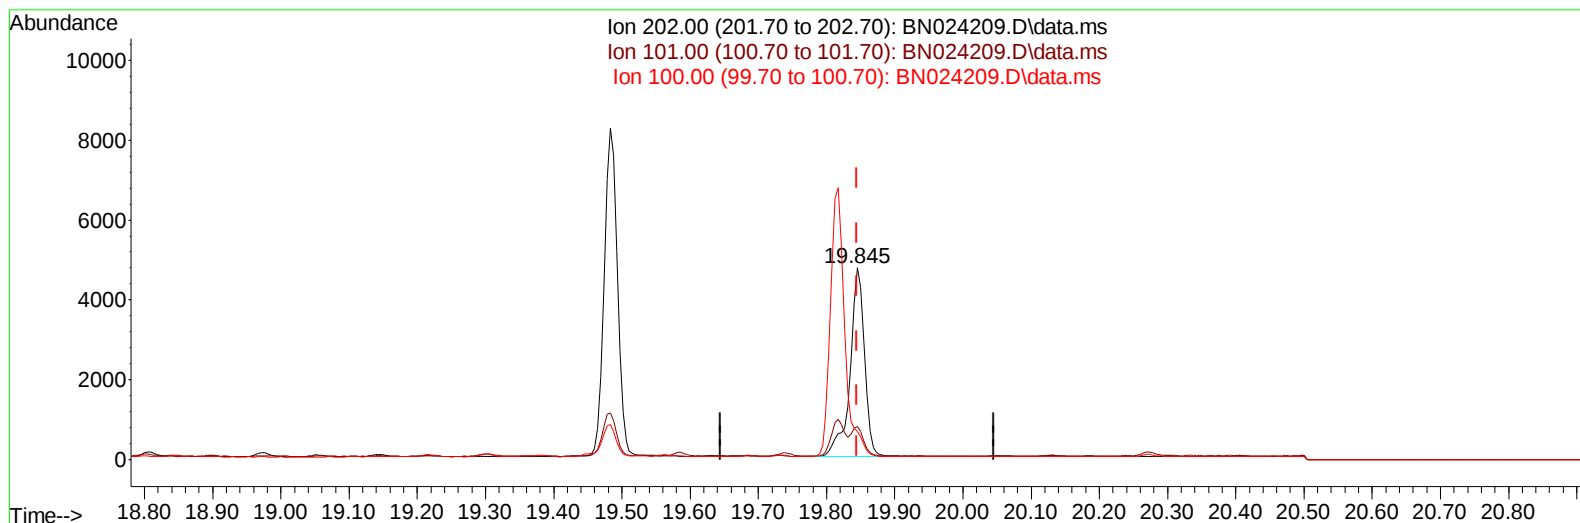

TIC: BN024209.D\data.ms

(20) Pyrene

19.845min (+ 0.000) 0.08 ng/u1

response 6891

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	17.10
100.00	11.70	14.62#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024209.D
Acq On : 09 Mar 2023 20:55
Operator : CG/JU
Sample : 01746-05DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAD5DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:25:33 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

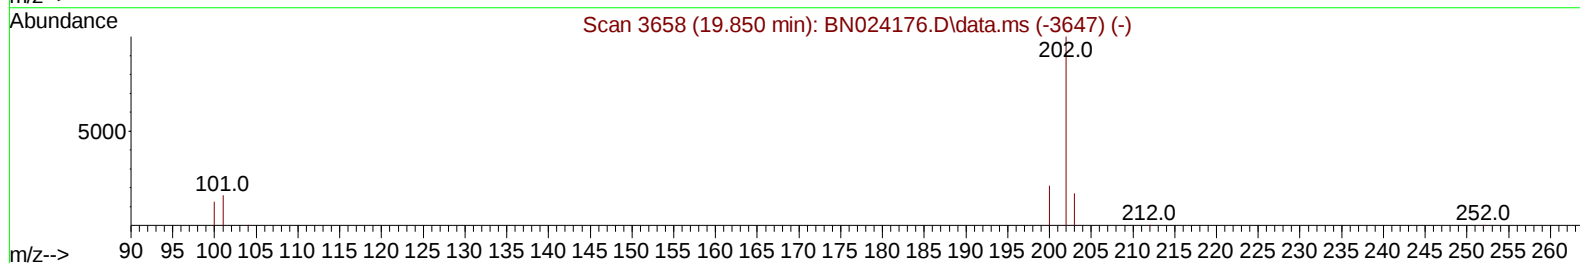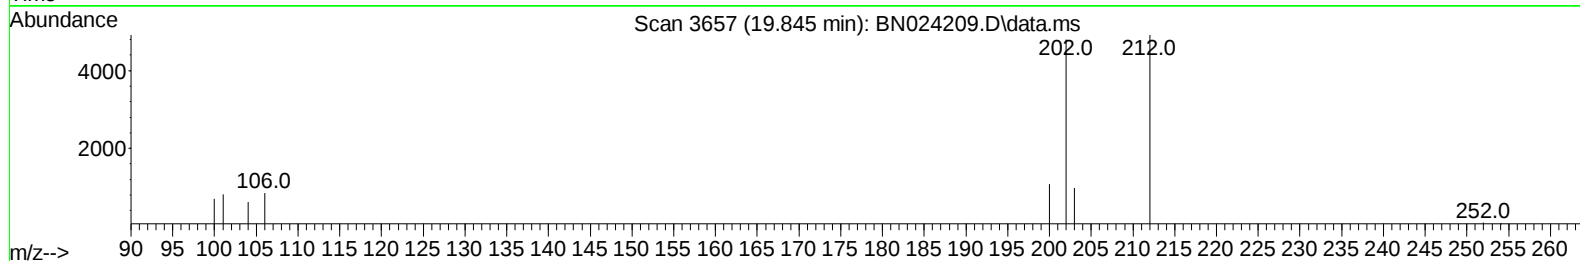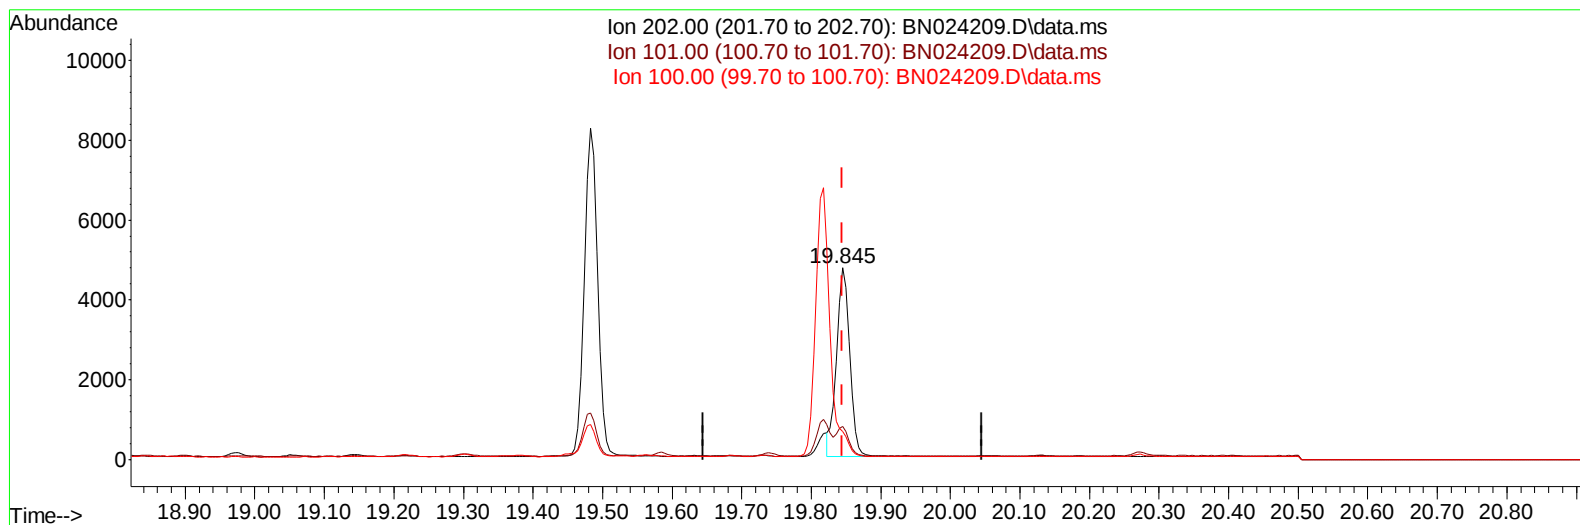

TIC: BN024209.D\data.ms

(20) Pyrene

19.845min (+ 0.000) 0.07 ng/ul m

response 6326

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	17.10
100.00	11.70	14.62#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024209.D
 Acq On : 09 Mar 2023 20:55
 Operator : CG/JU
 Sample : 01746-05DL 5X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAD5DL

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 02:25:33 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.055	152		9566	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136		28753	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164		16027	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188		32895	0.400	ng/ul	0.00
17) Chrysene-d12	21.615	240		22225	0.400	ng/ul	0.00
23) Perylene-d12	24.120	264		16791	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.410	96		4039	0.384	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152		2141	0.063	ng/ul	0.00
18) Fluoranthene-d10	19.455	212		4493	0.076	ng/ul	0.00
Target Compounds							
							Qvalue
5) Naphthalene	10.922	128		2565528	35.747	ng/ul	100
7) 2-Methylnaphthalene	12.528	142		150704	3.461	ng/ul	100
8) 1-Methylnaphthalene	12.742	142		92588	2.023	ng/ul	100
10) Acenaphthylene	14.407	152		33161	0.496	ng/ul	99
11) Acenaphthene	14.749	153		128094	2.486	ng/ul	98
12) Fluorene	15.735	166		173408	3.014	ng/ul	100
14) Pentachlorophenol	17.076	266		6172	0.676	ng/ul#	73
15) Phenanthrene	17.472	178		86017	0.913	ng/ul	100
16) Anthracene	17.565	178		6588	0.080	ng/ul	97
19) Fluoranthene	19.483	202		11009	0.124	ng/ul	97
20) Pyrene	19.845	202		6326m	0.070	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024209.D
Acq On : 09 Mar 2023 20:55
Operator : CG/JU
Sample : 01746-05DL 5X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAD5DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:25:33 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

