




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024210.D
 Acq On : 09 Mar 2023 21:32
 Operator : CG/JU
 Sample : 01746-11DL 5X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAE6DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:25:42 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian
 Giraldo

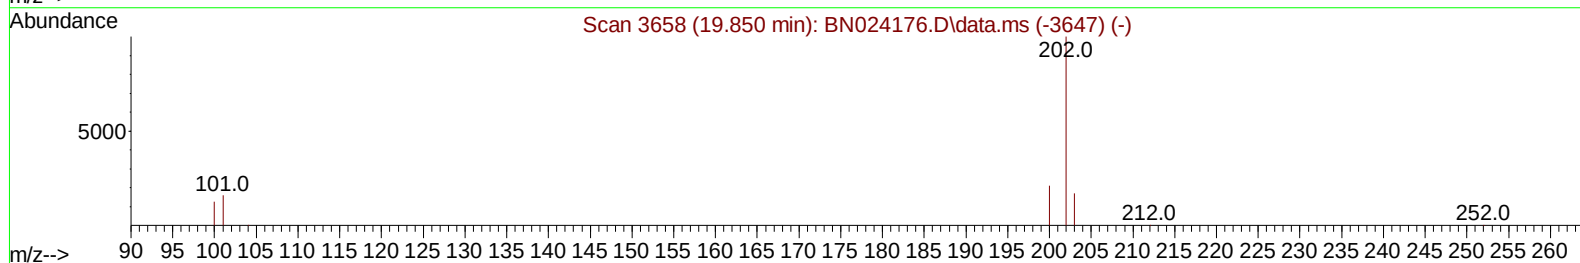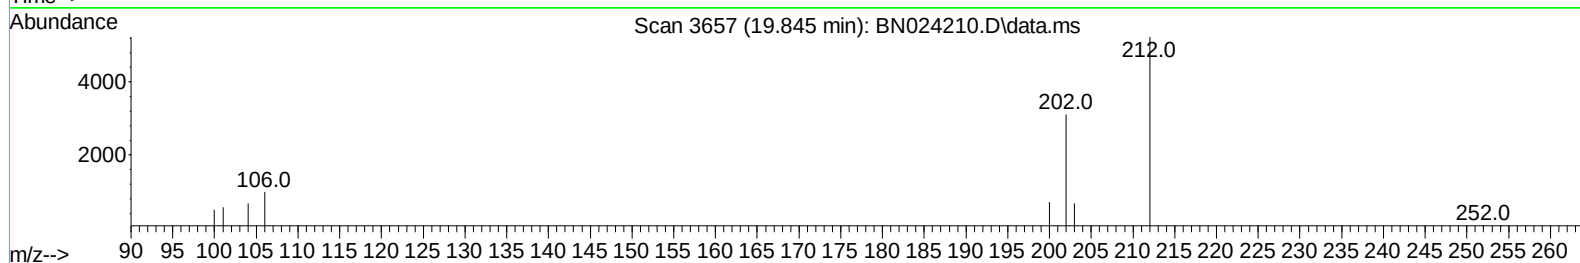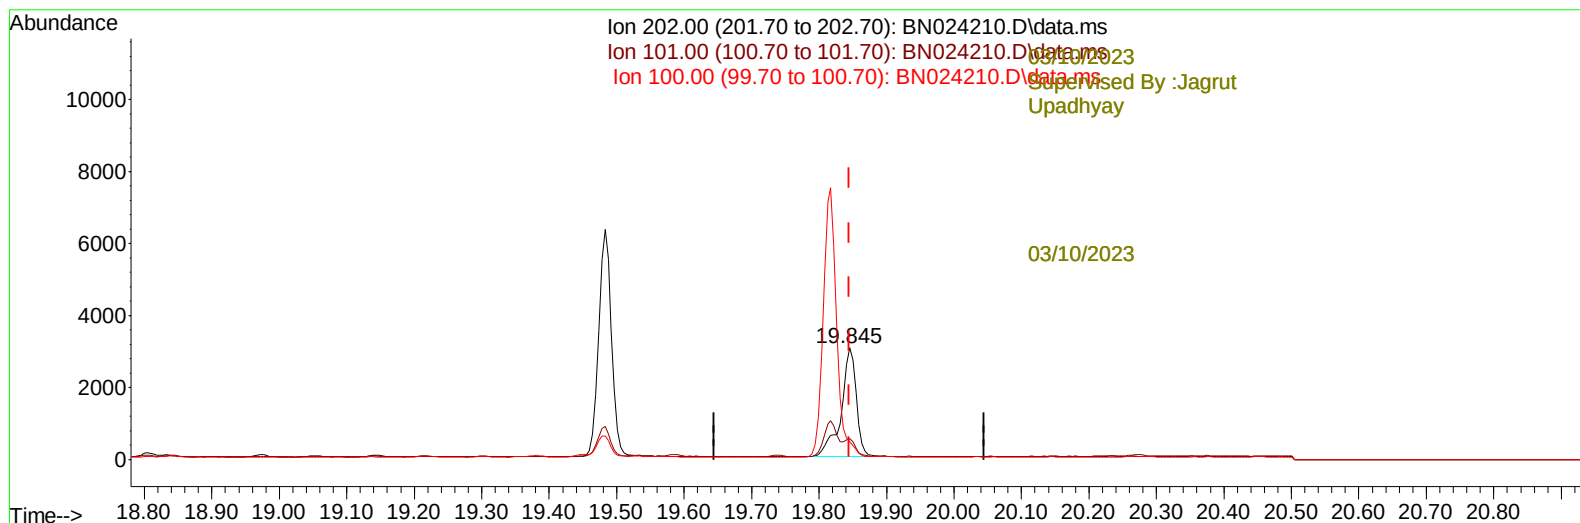

TIC: BN024210.D\data.ms

(20) Pyrene

19.845min (+ 0.000) 0.06 ng/u1

response 4742

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	18.41#
100.00	11.70	15.87#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024210.D
Acq On : 09 Mar 2023 21:32
Operator : CG/JU
Sample : 01746-11DL 5X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAE6DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:25:42 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian
Giraldo

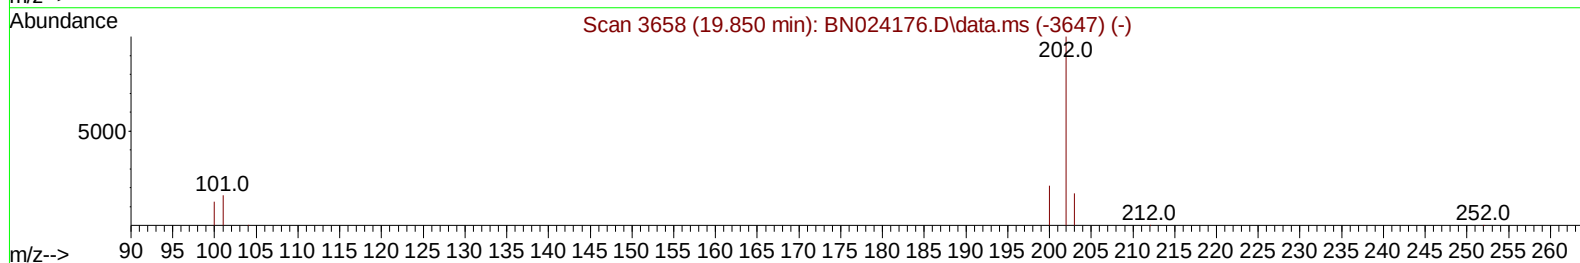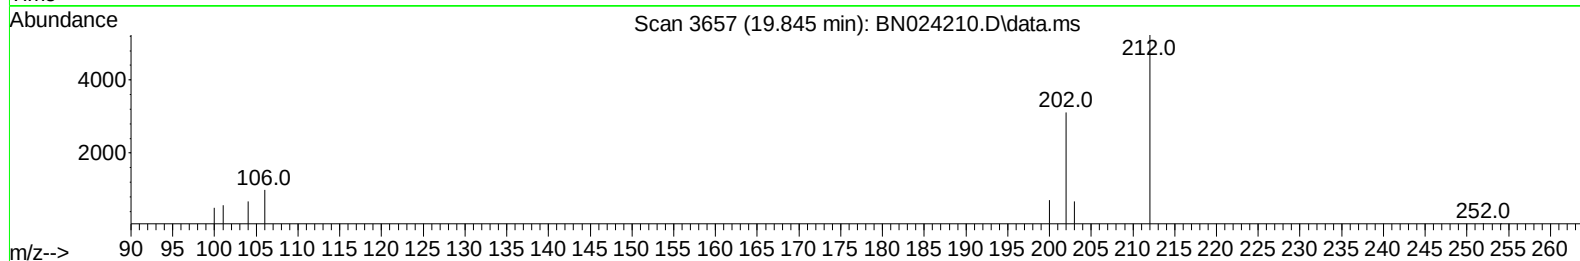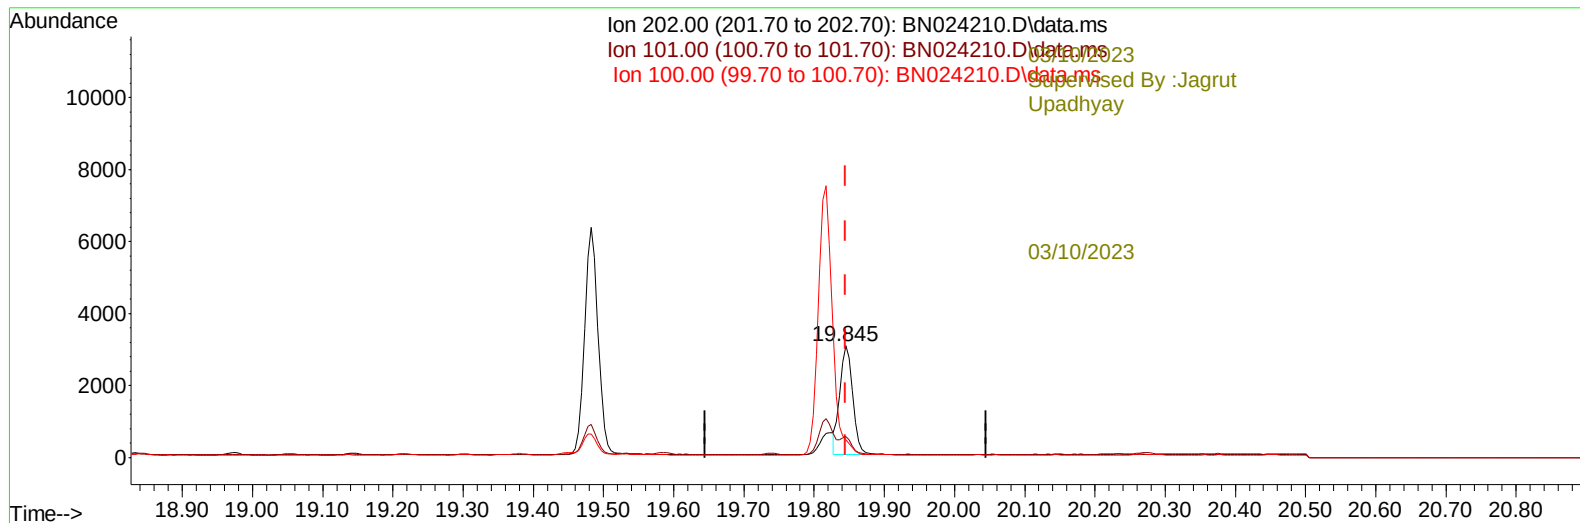

TIC: BN024210.D\data.ms

(20) Pyrene

19.845min (+ 0.000) 0.05 ng/ul m

response 3972

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	18.41#
100.00	11.70	15.87#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024210.D
 Acq On : 09 Mar 2023 21:32
 Operator : CG/JU
 Sample : 01746-11DL 5X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAE6DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:25:42 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 08:02:24 2023
 Response via : Initial Calibration

Reviewed By :Christian
 Giraldo

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----03/10/2023							
Supervised By :Jagrut							
Jadhay							
-----03/10/2023							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.055	152		9099	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136		27272	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164		14859	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188		30315	0.400	ng/ul	0.00
17) Chrysene-d12	21.615	240		20683	0.400	ng/ul	0.00
23) Perylene-d12	24.129	264		15392	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.405	96		4106	0.410	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152		2199	0.068	ng/ul	0.00
18) Fluoranthene-d10	19.455	212		4935	0.090	ng/ul	0.00
Target Compounds							
							Qvalue
5) Naphthalene	10.922	128		293459	4.311	ng/ul	99
7) 2-Methylnaphthalene	12.528	142		13171	0.319	ng/ul	100
8) 1-Methylnaphthalene	12.742	142		9571	0.221	ng/ul	100
10) Acenaphthylene	14.407	152		5158	0.083	ng/ul#	95
11) Acenaphthene	14.749	153		11768	0.246	ng/ul	99
12) Fluorene	15.734	166		8927	0.167	ng/ul#	98
14) Pentachlorophenol	17.076	266		24129	2.866	ng/ul#	73
15) Phenanthrene	17.472	178		16555	0.191	ng/ul	99
16) Anthracene	17.565	178		3859	0.051	ng/ul#	93
19) Fluoranthene	19.483	202		8468	0.103	ng/ul	98
20) Pyrene	19.845	202		3972m	0.048	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024210.D
Acq On : 09 Mar 2023 21:32
Operator : CG/JU
Sample : 01746-11DL 5X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAE6DL

Manual IntegrationsAPPROVED

Quant Time: Mar 10 02:25:42 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 08:02:24 2023
Response via : Initial Calibration

Reviewed By :Christian
Giraldo

