




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024225.D
Acq On : 10 Mar 2023 07:16
Operator : CG/JU
Sample : 01784-18
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAD4

Manual IntegrationsAPPROVED

Quant Time: Mar 10 07:46:11 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 03:43:59 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

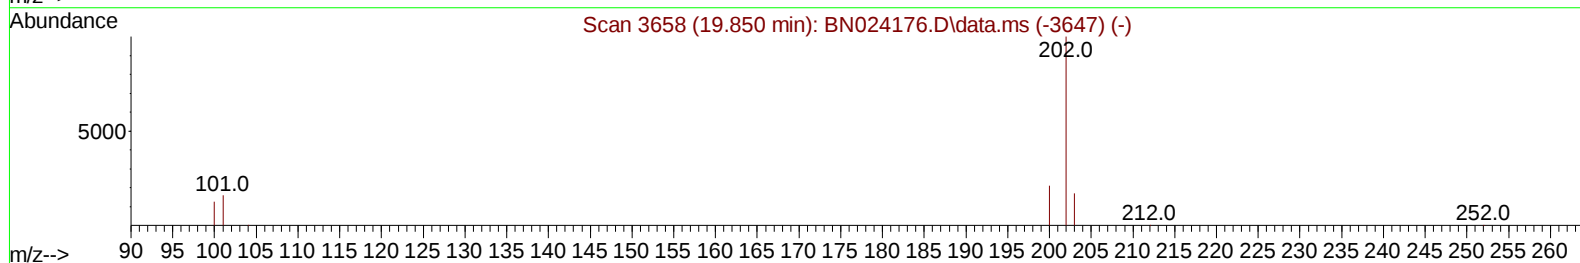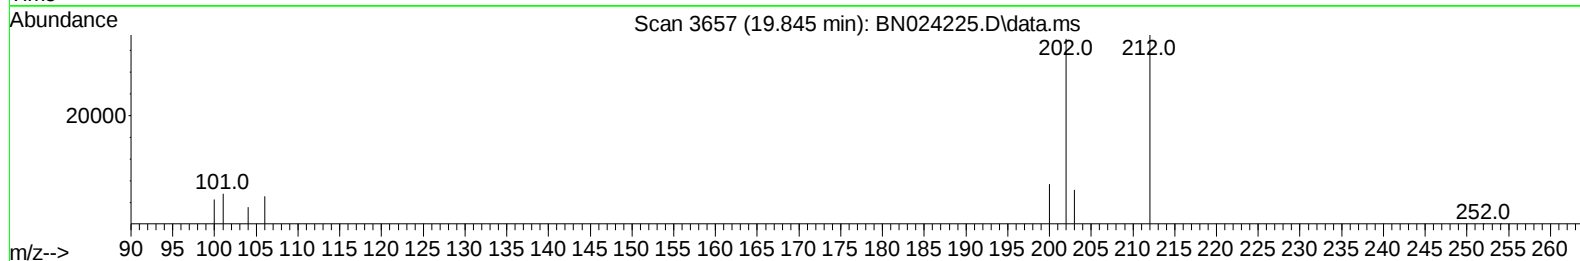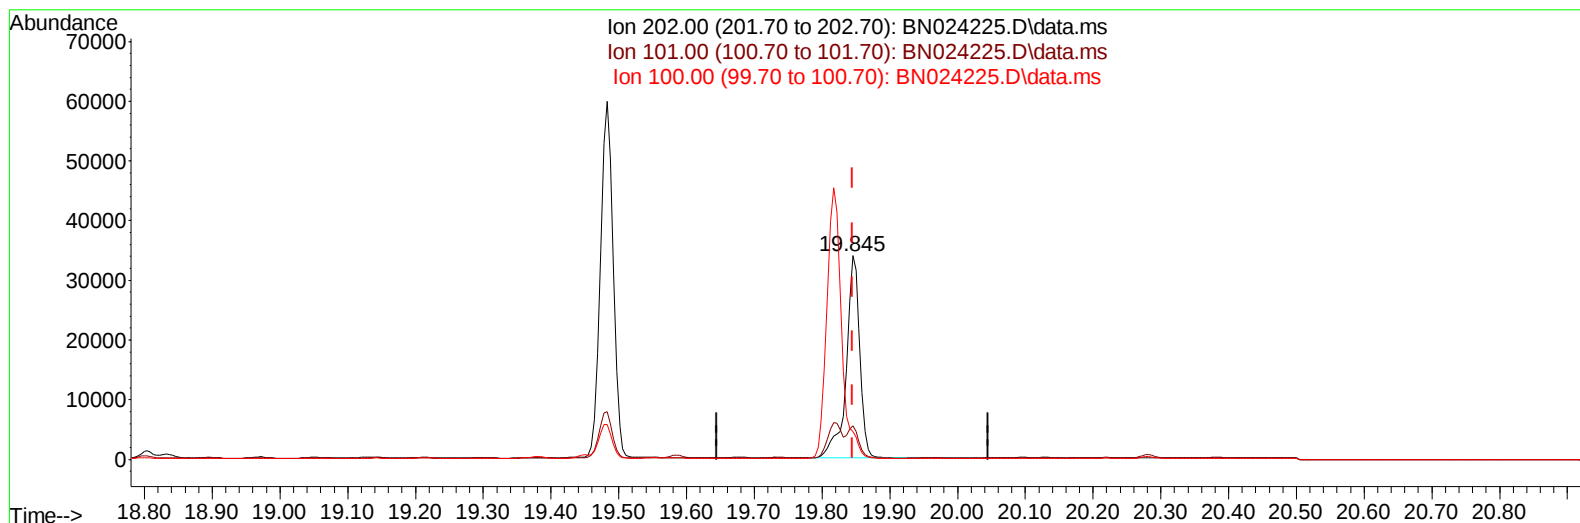

TIC: BN024225.D\data.ms

(20) Pyrene

19.845min (+ 0.000) 0.42 ng/u1

response 47698

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	16.40
100.00	11.70	13.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024225.D
Acq On : 10 Mar 2023 07:16
Operator : CG/JU
Sample : 01784-18
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAD4

Manual IntegrationsAPPROVED

Quant Time: Mar 10 07:46:11 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 03:43:59 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

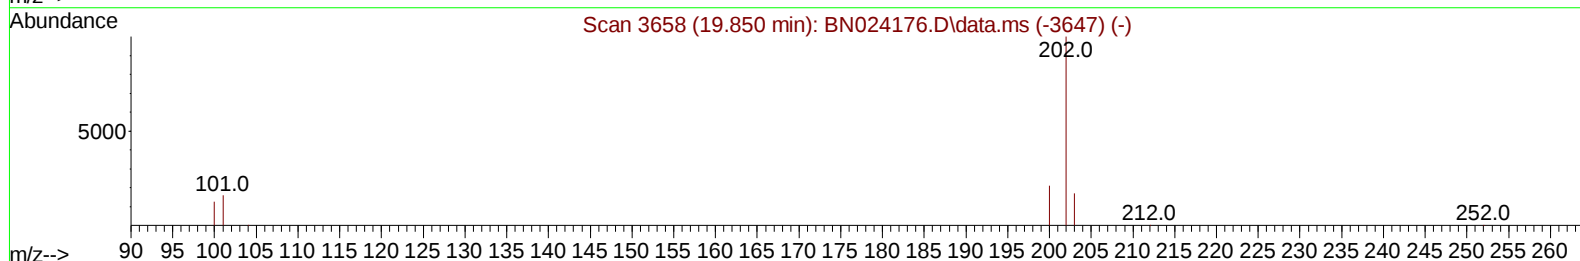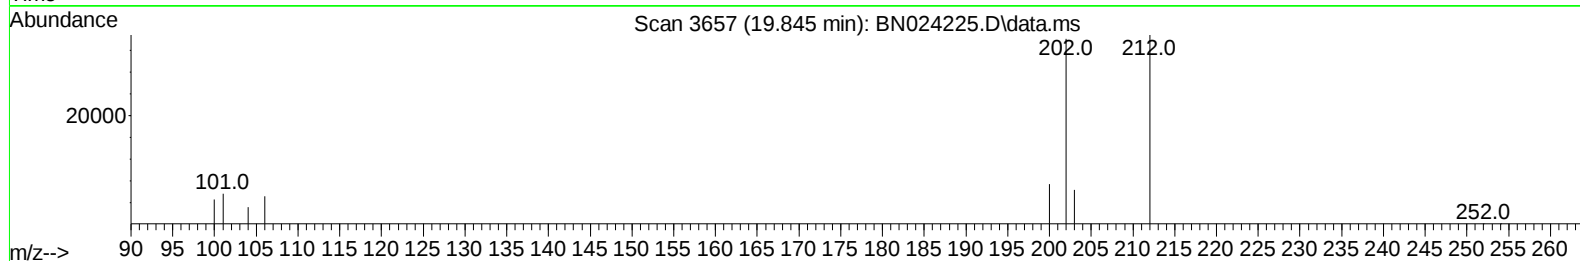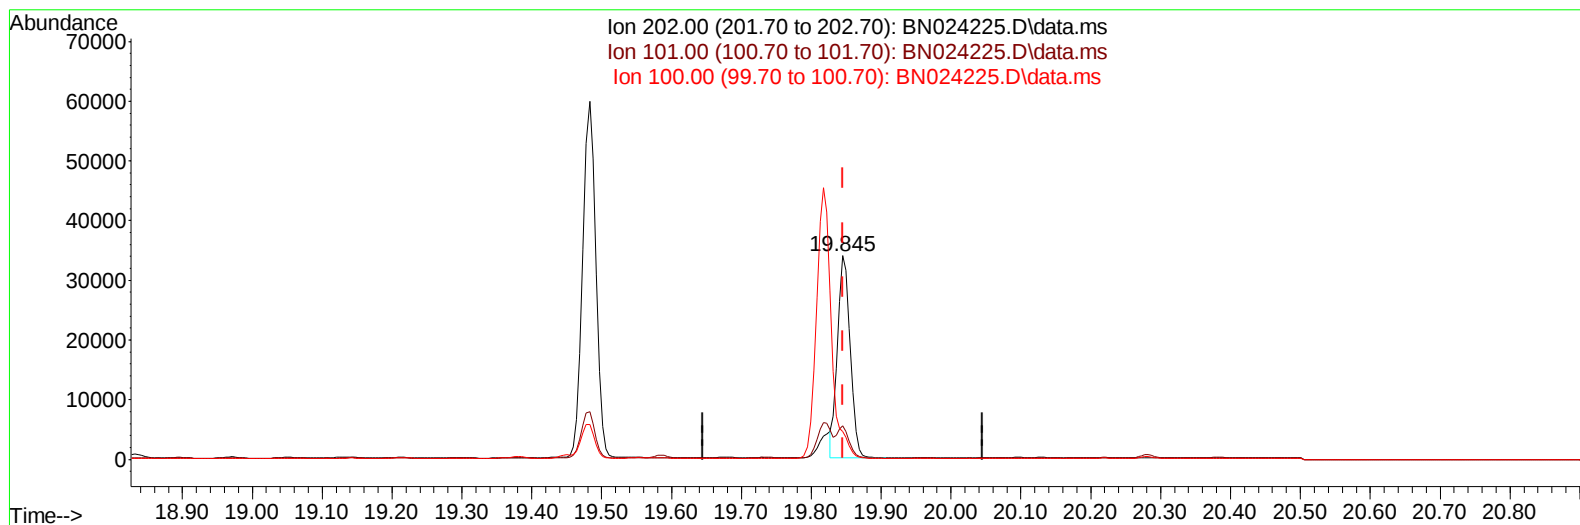

TIC: BN024225.D\data.ms

(20) Pyrene

19.845min (+ 0.000) 0.38 ng/ul m

response 42760

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	15.10	16.40
100.00	11.70	13.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024225.D
 Acq On : 10 Mar 2023 07:16
 Operator : CG/JU
 Sample : 01784-18
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAD4

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 07:46:11 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 03:43:59 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.051	152		9477	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136		29301	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.684	164		17751	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188		35787	0.400	ng/ul	0.00
17) Chrysene-d12	21.618	240		28045	0.400	ng/ul	0.00
23) Perylene-d12	24.120	264		28106	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.406	96		56097	5.379	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152		15391	0.442	ng/ul	0.00
18) Fluoranthene-d10	19.450	212		39859	0.534	ng/ul	0.00
Target Compounds				Qvalue			
5) Naphthalene	10.922	128		5194	0.071	ng/ul#	76
8) 1-Methylnaphthalene	12.742	142		2179	0.047	ng/ul	99
10) Acenaphthylene	14.407	152		13751	0.186	ng/ul#	94
11) Acenaphthene	14.749	153		47507	0.833	ng/ul	97
12) Fluorene	15.730	166		260565	4.089	ng/ul	99
14) Pentachlorophenol	17.076	266		59647	6.001	ng/ul#	73
15) Phenanthrene	17.472	178		27983	0.273	ng/ul	97
16) Anthracene	17.561	178		13116	0.146	ng/ul	93
19) Fluoranthene	19.483	202		76974	0.690	ng/ul	99
20) Pyrene	19.845	202		42760m	0.378	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024225.D
Acq On : 10 Mar 2023 07:16
Operator : CG/JU
Sample : 01784-18
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAD4

Manual IntegrationsAPPROVED

Quant Time: Mar 10 07:46:11 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 03:43:59 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

