

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024175.D
 Acq On : 08 Mar 2023 19:17
 Operator : CG/JU
 Sample : 01746-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC8

Quant Time: Mar 09 03:36:44 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 01:03:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.059	152	7507	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	22592	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.693	164	12627	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	25753	0.400	ng/ul	0.00
17) Chrysene-d12	21.624	240	18356	0.400	ng/ul	0.00
23) Perylene-d12	24.146	264	15222	0.400	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	35611	4.311	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.456	152	9180	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.459	212	20948	0.429	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.927	128	1441	0.026	ng/ul#	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024175.D
Acq On : 08 Mar 2023 19:17
Operator : CG/JU
Sample : 01746-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAC8


Quant Time: Mar 09 03:36:44 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 01:03:32 2023
Response via : Initial Calibration

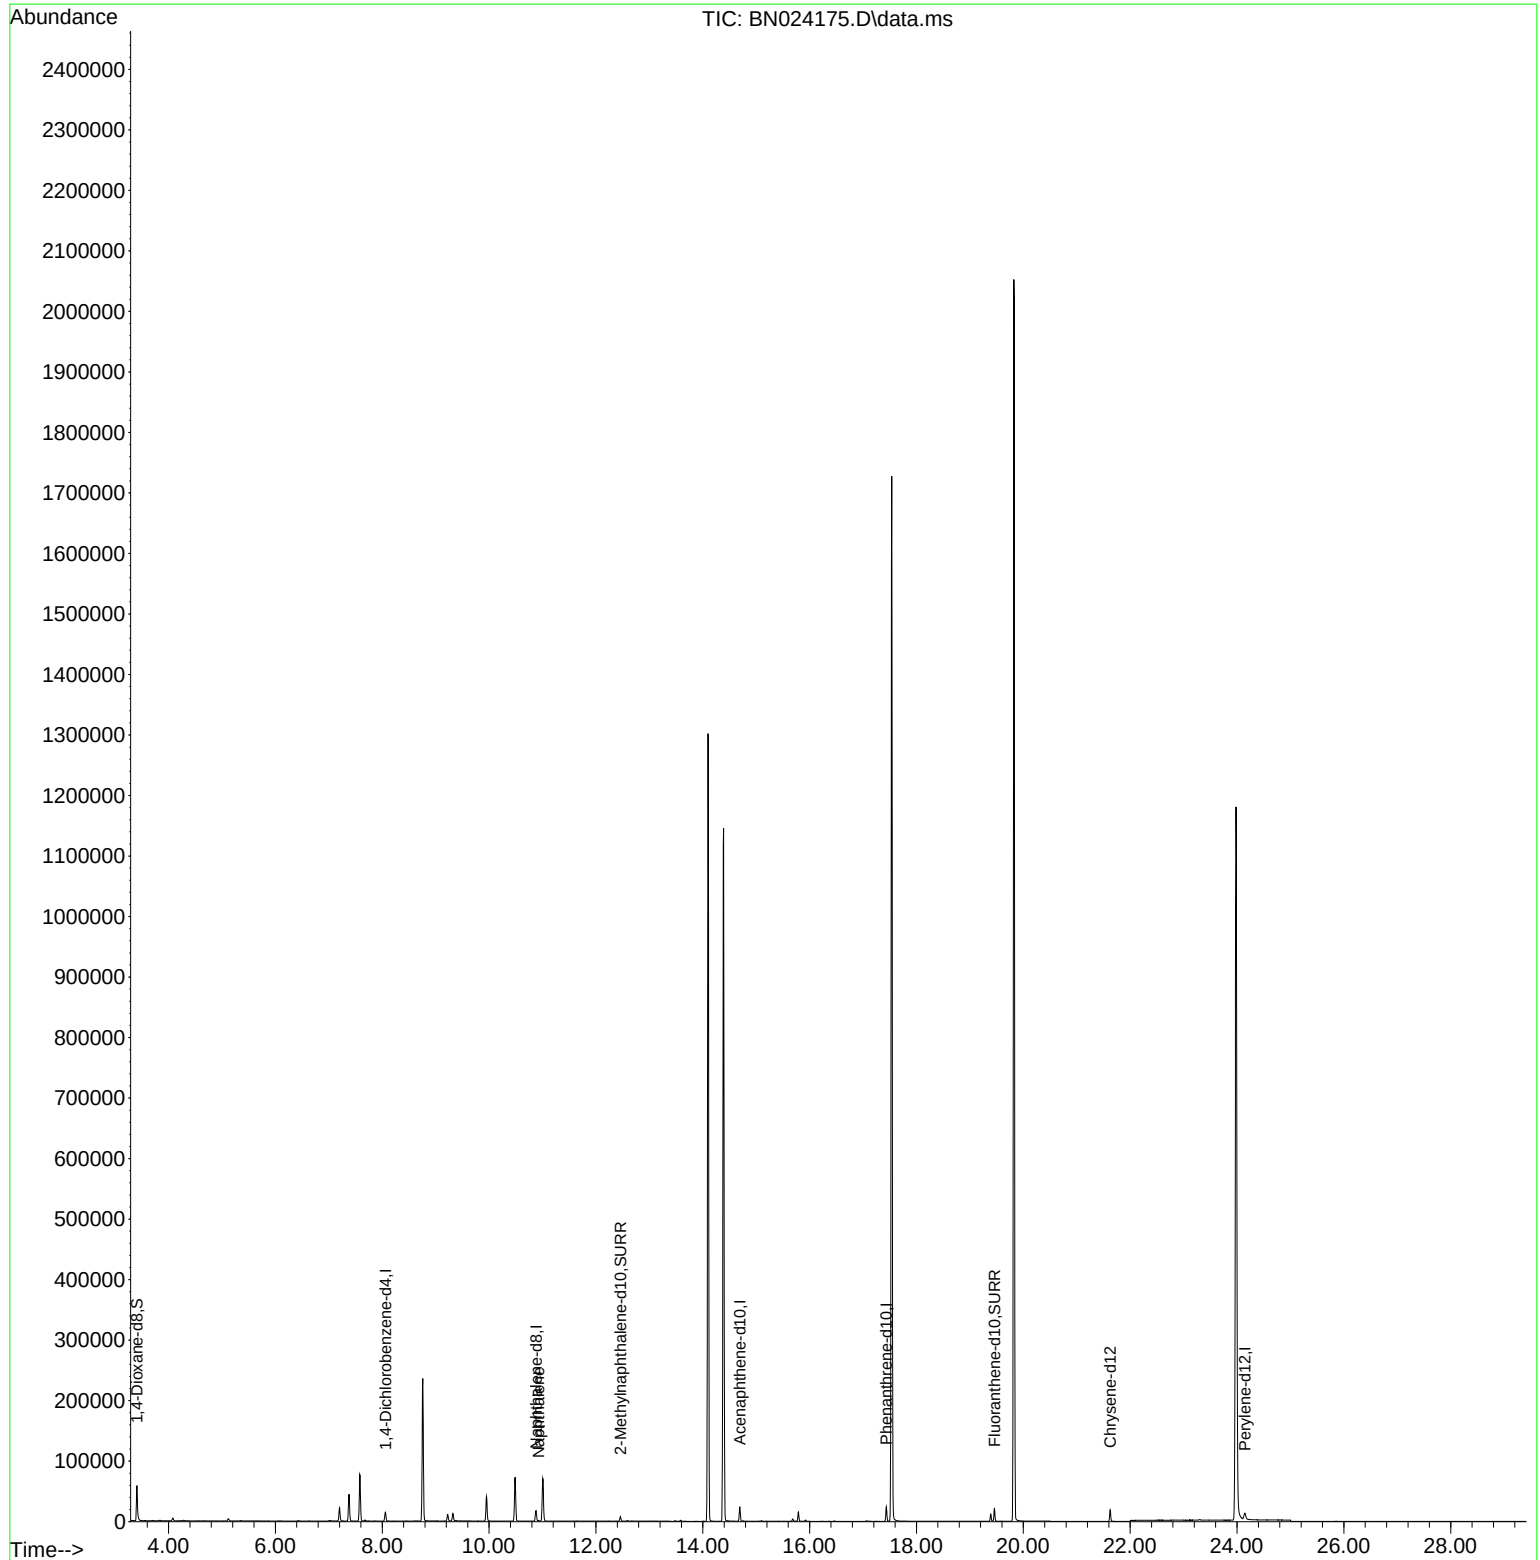

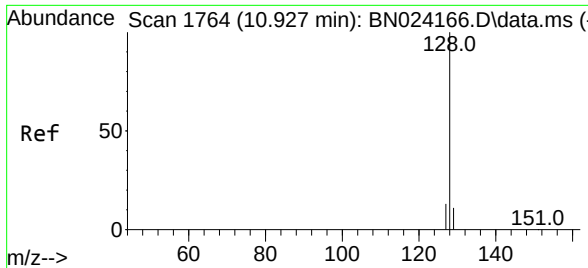

#5
Naphthalene
Concen: 0.026 ng/ul
RT: 10.927 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN024175.D
Acq: 08 Mar 2023 19:17

Instrument :
BNA_N
ClientSampleId :
DCAC8

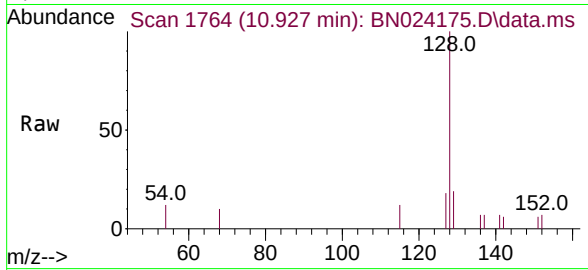

Tgt Ion:	128	Resp:	1441
Ion	Ratio	Lower	Upper
128	100		
129	18.5	9.0	13.6#
127	17.8	10.5	15.7#

