

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024187.D
 Acq On : 09 Mar 2023 03:15
 Operator : CG/JU
 Sample : 01746-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAE7

Quant Time: Mar 09 04:26:05 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 03:48:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.054	152	9407	0.400	ng/u1	0.00
4) Naphthalene-d8	10.871	136	28982	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.687	164	16655	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.433	188	33796	0.400	ng/u1	0.00
17) Chrysene-d12	21.622	240	24093	0.400	ng/u1	0.00
23) Perylene-d12	24.124	264	22695	0.400	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.409	96	50002	4.830	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.454	152	12353	0.359	ng/u1	0.00
18) Fluoranthene-d10	19.458	212	30643	0.478	ng/u1	0.00
Target Compounds						
11) Acenaphthene	14.752	153	3344	0.062	ng/u1	Qvalue 99
14) Pentachlorophenol	17.078	266	359	0.038	ng/u1#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024187.D
Acq On : 09 Mar 2023 03:15
Operator : CG/JU
Sample : 01746-12
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAE7

Quant Time: Mar 09 04:26:05 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 03:48:21 2023
Response via : Initial Calibration

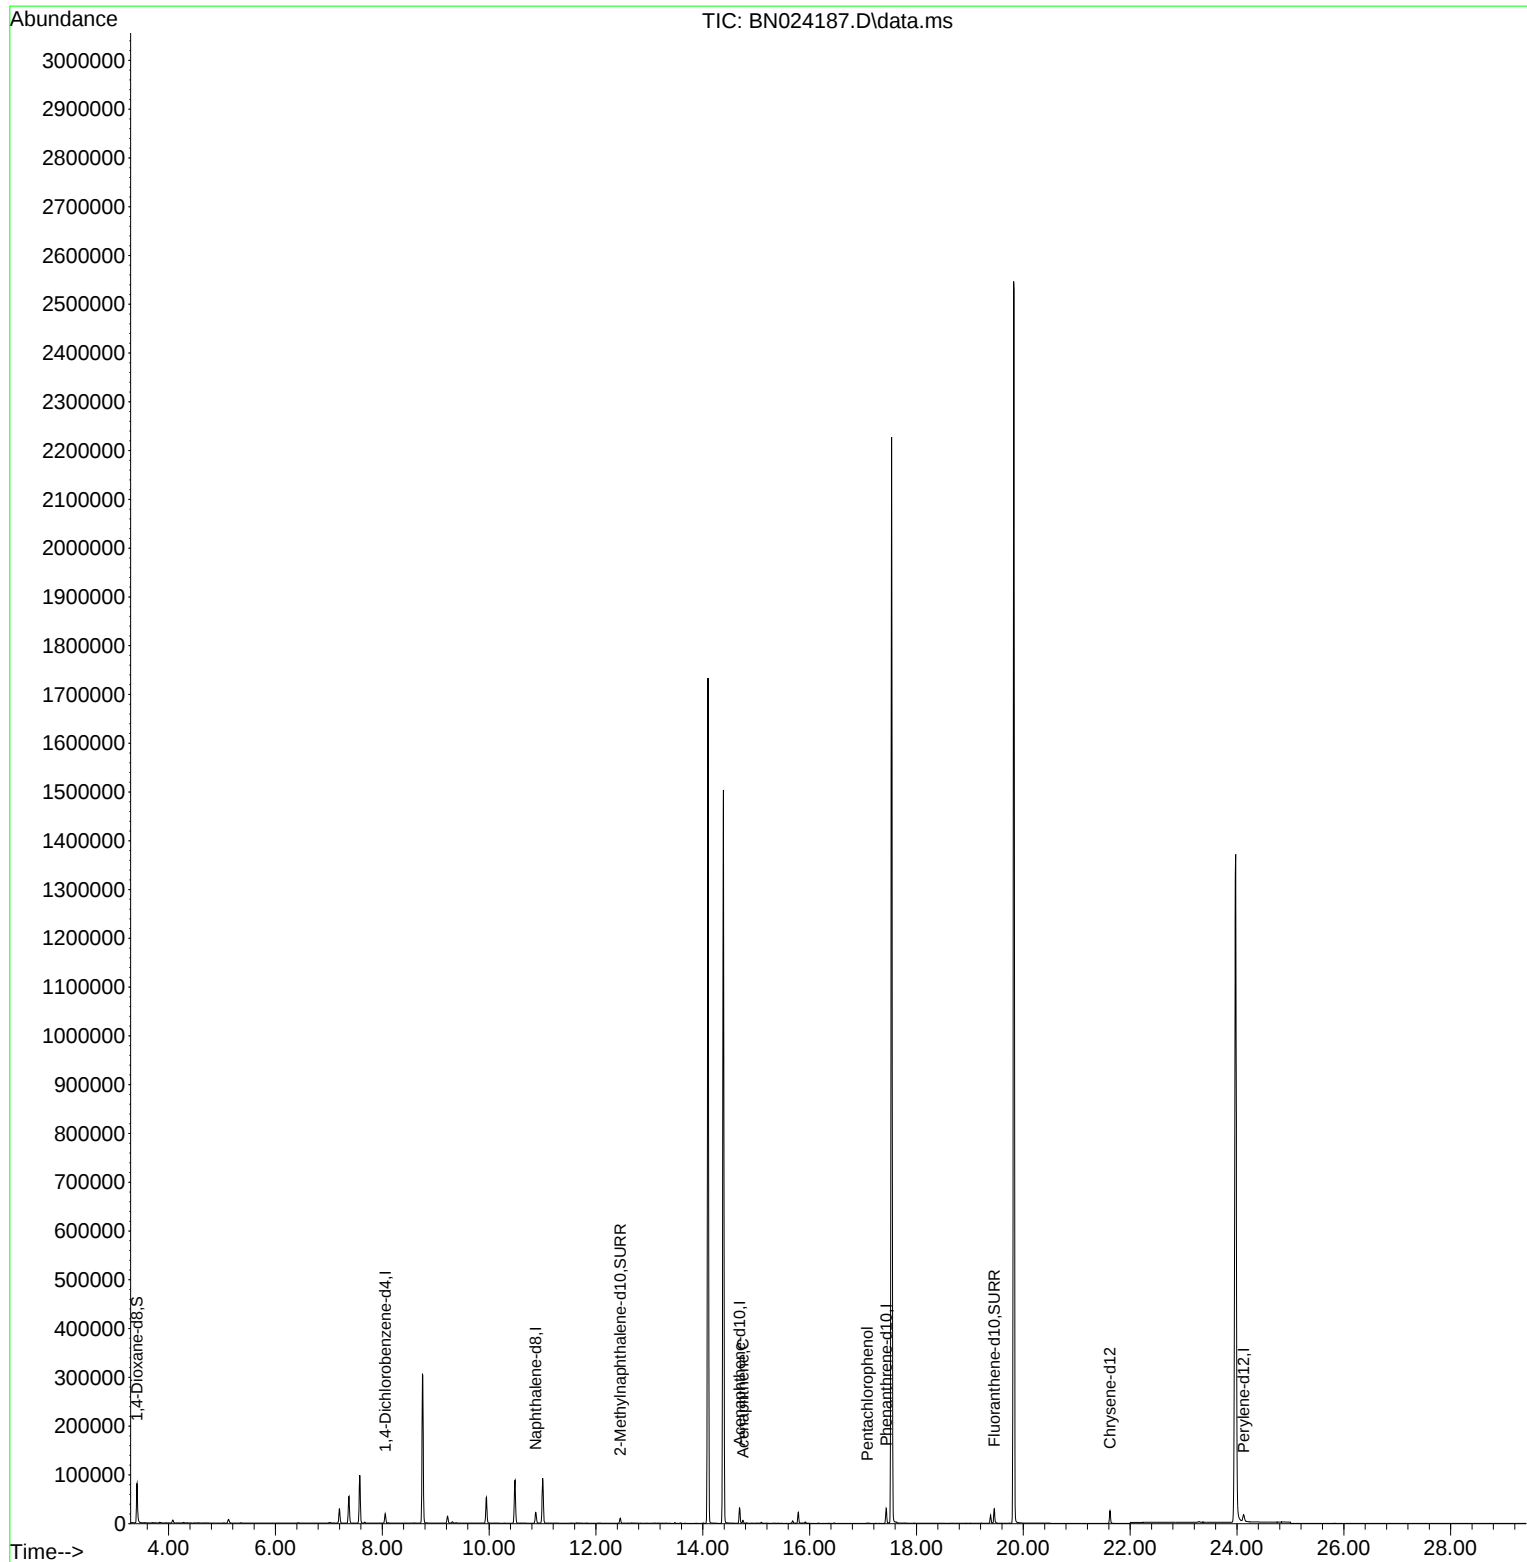

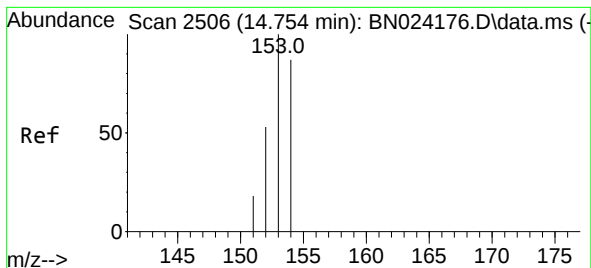

#11

Acenaphthene

Concen: 0.062 ng/ul

RT: 14.752 min Scan# 2506

Delta R.T. -0.002 min

Lab File: BN024187.D

Acq: 09 Mar 2023 03:15

Instrument :

BNA_N

ClientSampleId :

DCAE7





Tgt Ion:153 Resp: 3344

Ion Ratio Lower Upper

153 100

152 52.4 42.6 64.0

154 88.5 70.6 105.8

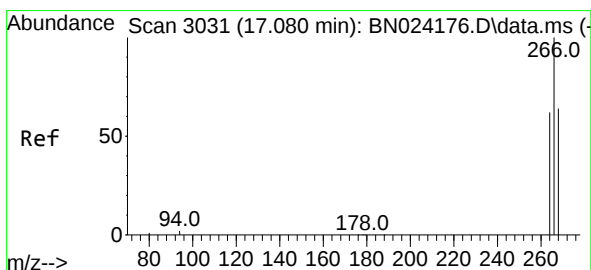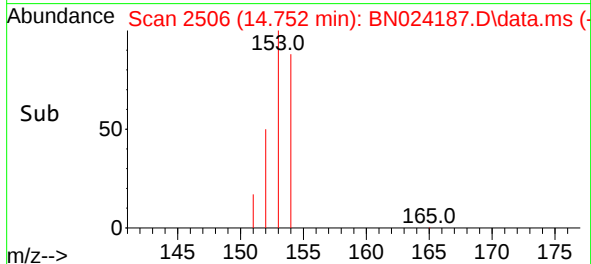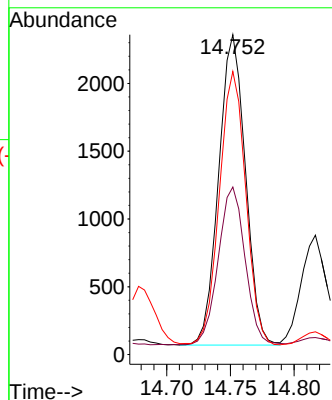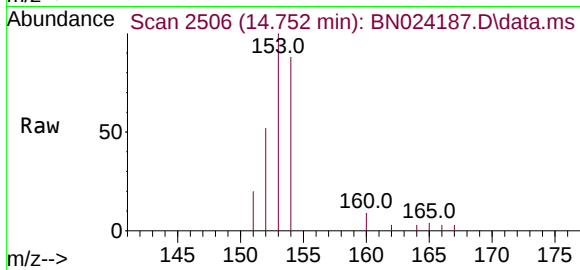

#14

Pentachlorophenol

Concen: 0.038 ng/ul

RT: 17.078 min Scan# 3031

Delta R.T. -0.002 min

Lab File: BN024187.D

Acq: 09 Mar 2023 03:15

Tgt Ion:266 Resp: 359

Ion Ratio Lower Upper

266 100

264 60.2 0.0 0.0#

268 63.2 0.1 0.1#

