

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024188.D
 Acq On : 09 Mar 2023 03:51
 Operator : CG/JU
 Sample : 01746-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAE8

Quant Time: Mar 09 04:26:42 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 03:48:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	8565	0.400	ng/u1	0.00
4) Naphthalene-d8	10.872	136	26128	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.689	164	15043	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.434	188	30892	0.400	ng/u1	0.00
17) Chrysene-d12	21.621	240	24147	0.400	ng/u1	0.00
23) Perylene-d12	24.117	264	22577	0.400	ng/u1	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	38946	4.132	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.456	152	10411	0.335	ng/u1	0.00
18) Fluoranthene-d10	19.455	212	27642	0.430	ng/u1	0.00
Target Compounds						
					Qvalue	
11) Acenaphthene	14.749	153	2674	0.055	ng/u1	98
14) Pentachlorophenol	17.075	266	7210	0.840	ng/u1#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024188.D
Acq On : 09 Mar 2023 03:51
Operator : CG/JU
Sample : 01746-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAE8

Quant Time: Mar 09 04:26:42 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 03:48:21 2023
Response via : Initial Calibration




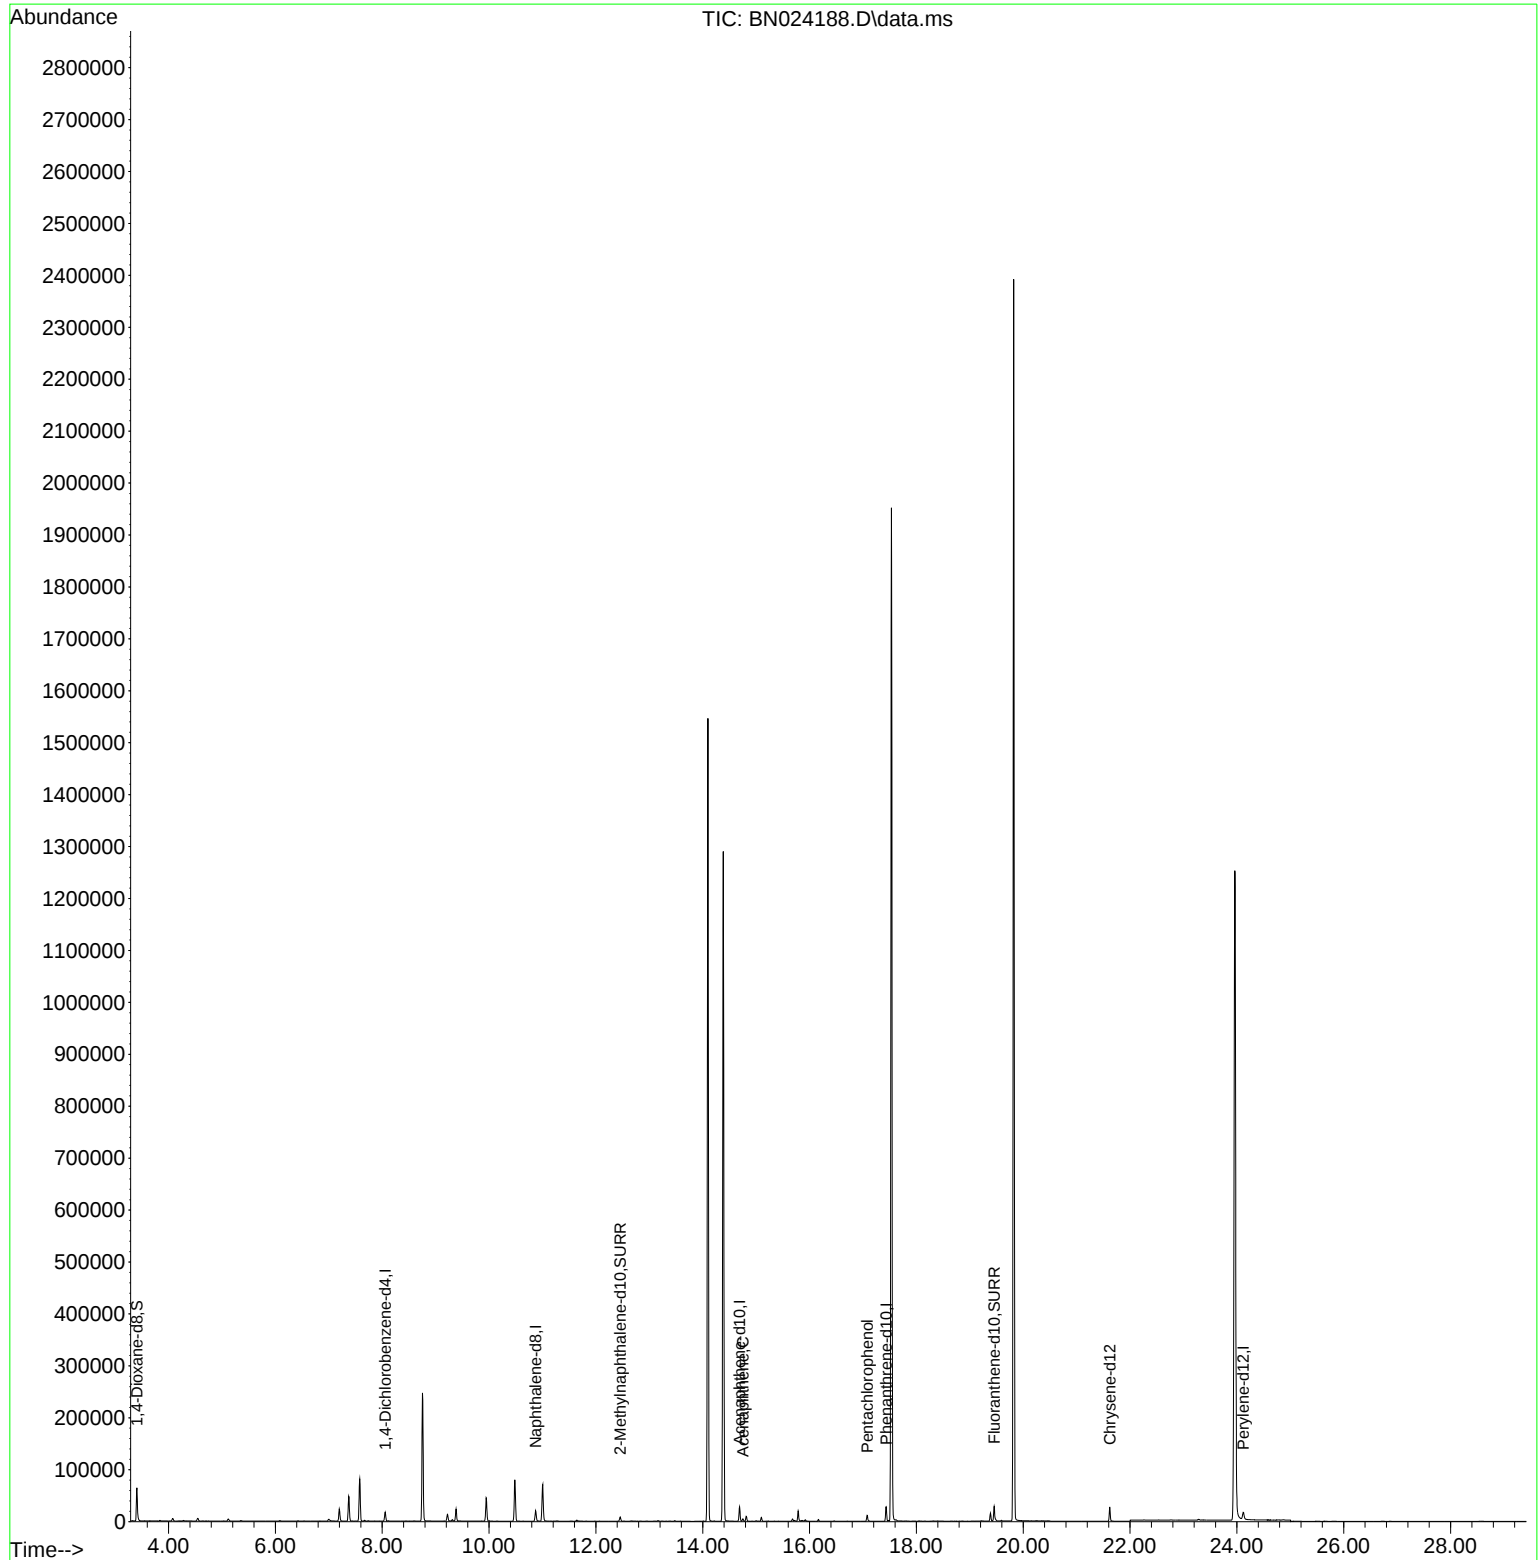


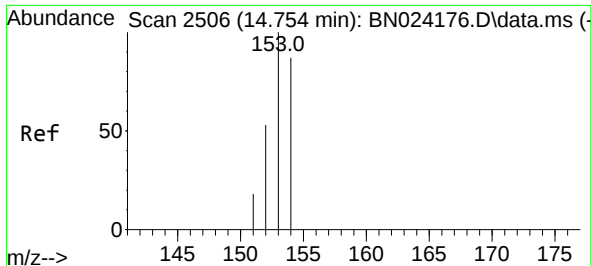

#11
Acenaphthene
Concen: 0.055 ng/ul
RT: 14.749 min Scan# 21
Delta R.T. -0.005 min
Lab File: BN024188.D
Acq: 09 Mar 2023 03:51

Instrument :
BNA_N
ClientSampleId :
DCAE8

Tgt Ion:153 Resp: 2674
Ion Ratio Lower Upper
153 100
152 51.5 42.6 64.0
154 87.1 70.6 105.8

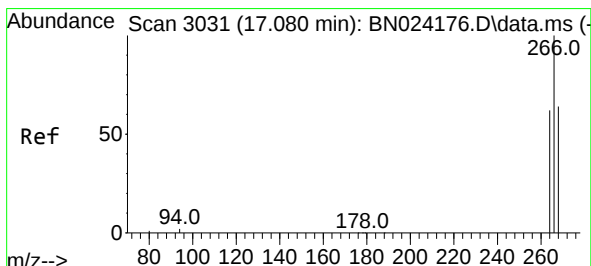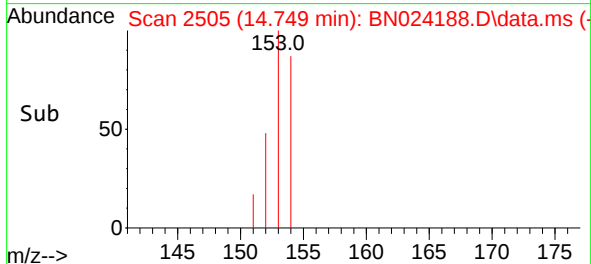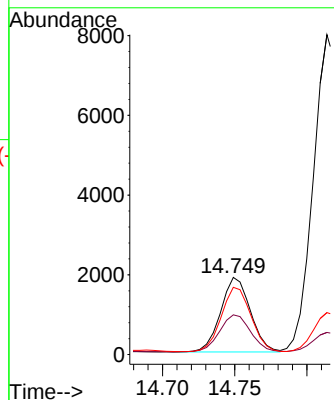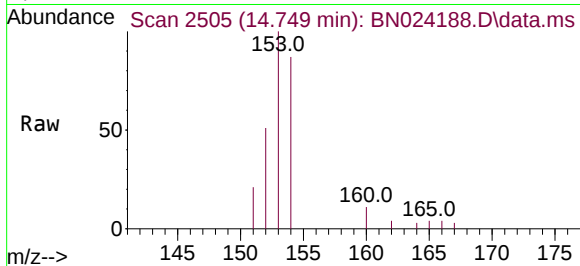

#14
Pentachlorophenol
Concen: 0.840 ng/ul
RT: 17.075 min Scan# 3030
Delta R.T. -0.004 min
Lab File: BN024188.D
Acq: 09 Mar 2023 03:51

Tgt Ion:266 Resp: 7210
Ion Ratio Lower Upper
266 100
264 63.2 0.0 0.0#
268 64.2 0.1 0.1#

