

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024189.D
 Acq On : 09 Mar 2023 04:27
 Operator : CG/JU
 Sample : 01746-14
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAF0

Quant Time: Mar 09 05:32:39 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 03:48:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	10154	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	31032	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.689	164	17710	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	35947	0.400	ng/ul	0.00
17) Chrysene-d12	21.624	240	25794	0.400	ng/ul	0.00
23) Perylene-d12	24.140	264	21906	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	47959	4.292	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.450	152	13900	0.377	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	32350	0.471	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.922	128	5506	0.071	ng/ul	96
11) Acenaphthene	14.749	153	1710	0.030	ng/ul	99
14) Pentachlorophenol	17.080	266	343	0.034	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024189.D
Acq On : 09 Mar 2023 04:27
Operator : CG/JU
Sample : 01746-14
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAF0

Quant Time: Mar 09 05:32:39 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 03:48:21 2023
Response via : Initial Calibration




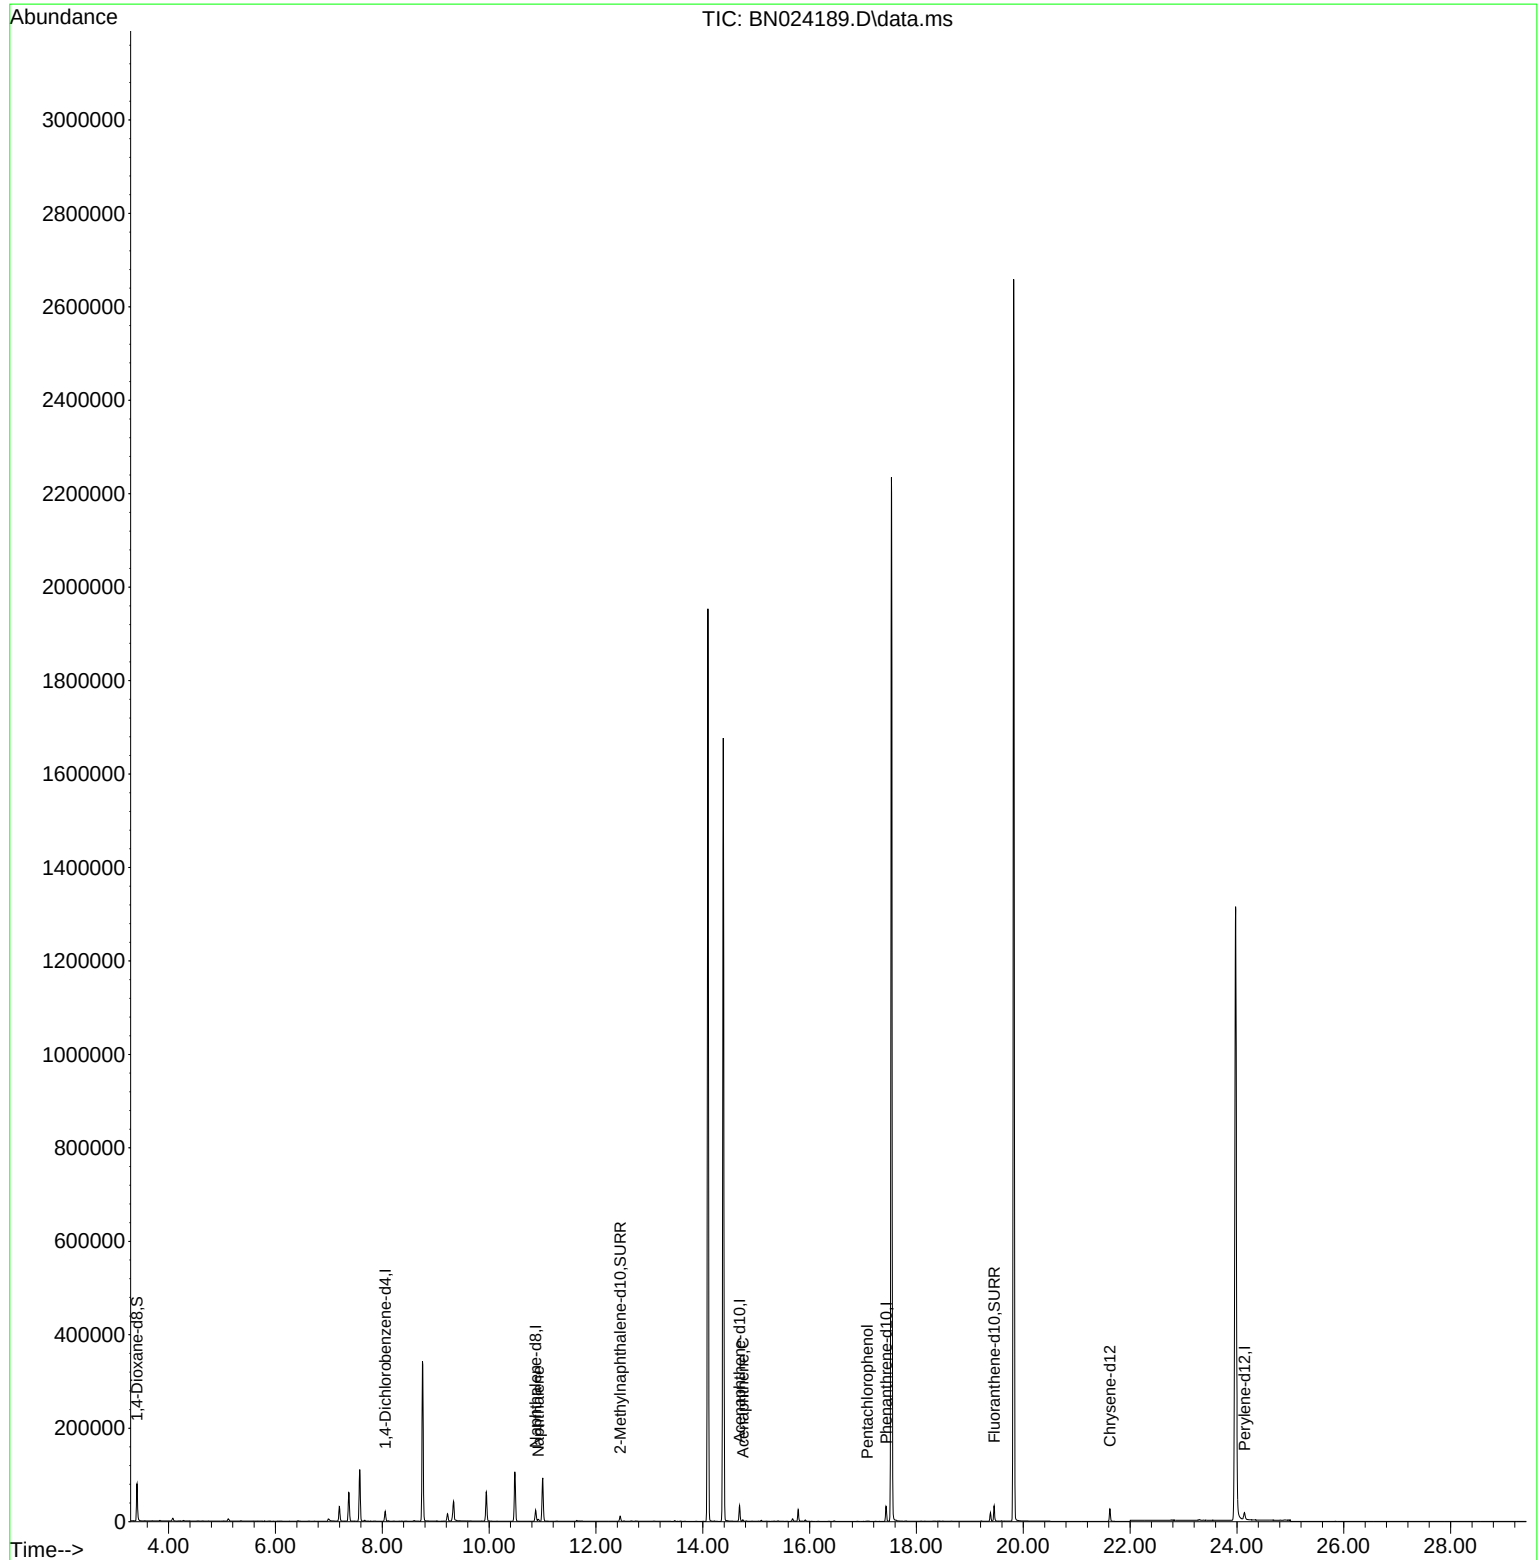


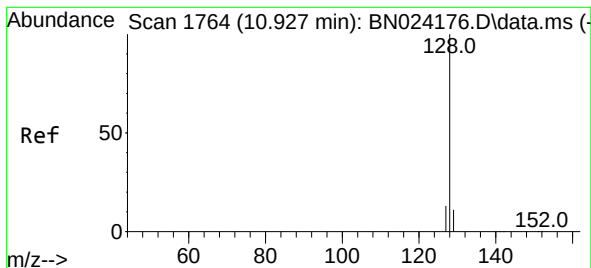

#5
Naphthalene
Concen: 0.071 ng/ul
RT: 10.922 min Scan# 11
Delta R.T. -0.006 min
Lab File: BN024189.D
Acq: 09 Mar 2023 04:27




Instrument :
BNA_N
ClientSampleId :
DCAF0


Tgt Ion:128 Resp: 5506
Ion Ratio Lower Upper
128 100
129 13.3 9.0 13.6
127 14.4 10.5 15.7

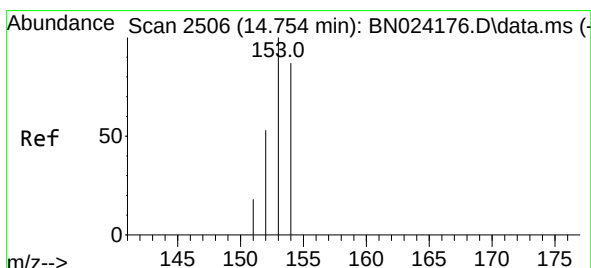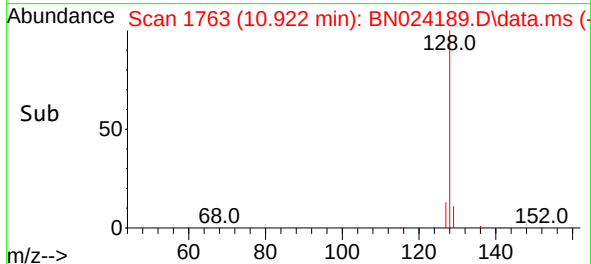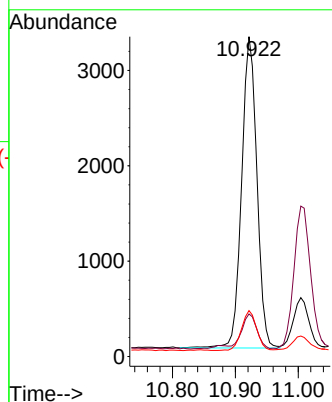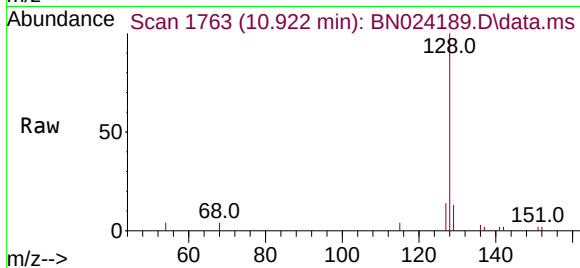

#11
Acenaphthene
Concen: 0.030 ng/ul
RT: 14.749 min Scan# 2505
Delta R.T. -0.005 min
Lab File: BN024189.D
Acq: 09 Mar 2023 04:27


Tgt Ion:153 Resp: 1710
Ion Ratio Lower Upper
153 100
152 54.3 42.6 64.0
154 88.0 70.6 105.8

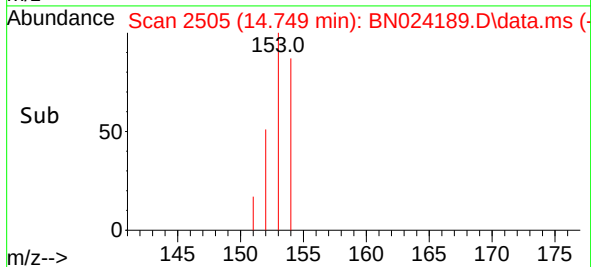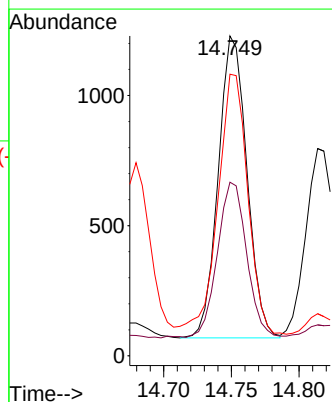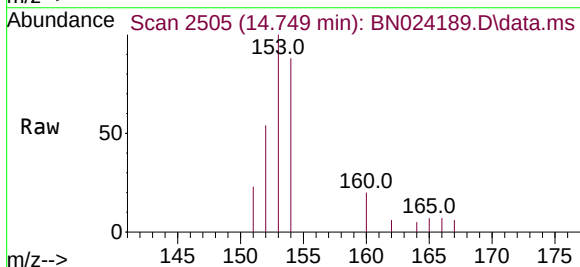

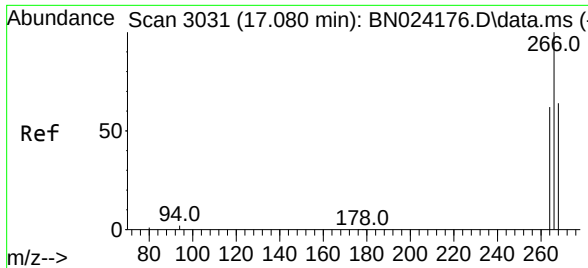

#14
 Pentachlorophenol
 Concen: 0.034 ng/ul
 RT: 17.080 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BN024189.D
 Acq: 09 Mar 2023 04:27

Instrument :
 BNA_N
 ClientSampleId :
 DCAF0

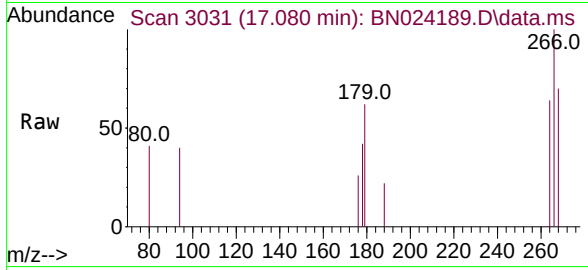

Tgt Ion:266 Resp: 343
 Ion Ratio Lower Upper
 266 100
 264 62.4 0.0 0.0#
 268 65.0 0.1 0.1#

