

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
 Data File : BN024224.D
 Acq On : 10 Mar 2023 06:40
 Operator : CG/JU
 Sample : 01784-14
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCAC4

Quant Time: Mar 10 07:10:13 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 03:43:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	7191	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	22180	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.684	164	12671	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188	25856	0.400	ng/ul	0.00
17) Chrysene-d12	21.618	240	19601	0.400	ng/ul	0.00
23) Perylene-d12	24.129	264	20706	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.401	96	33827	4.275	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	9982	0.379	ng/ul	0.00
18) Fluoranthene-d10	19.450	212	22877	0.439	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.916	128	2877	0.052	ng/ul#	91
16) Anthracene	17.561	178	4498	0.069	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030923\
Data File : BN024224.D
Acq On : 10 Mar 2023 06:40
Operator : CG/JU
Sample : 01784-14
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCAC4

Quant Time: Mar 10 07:10:13 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 03:43:59 2023
Response via : Initial Calibration




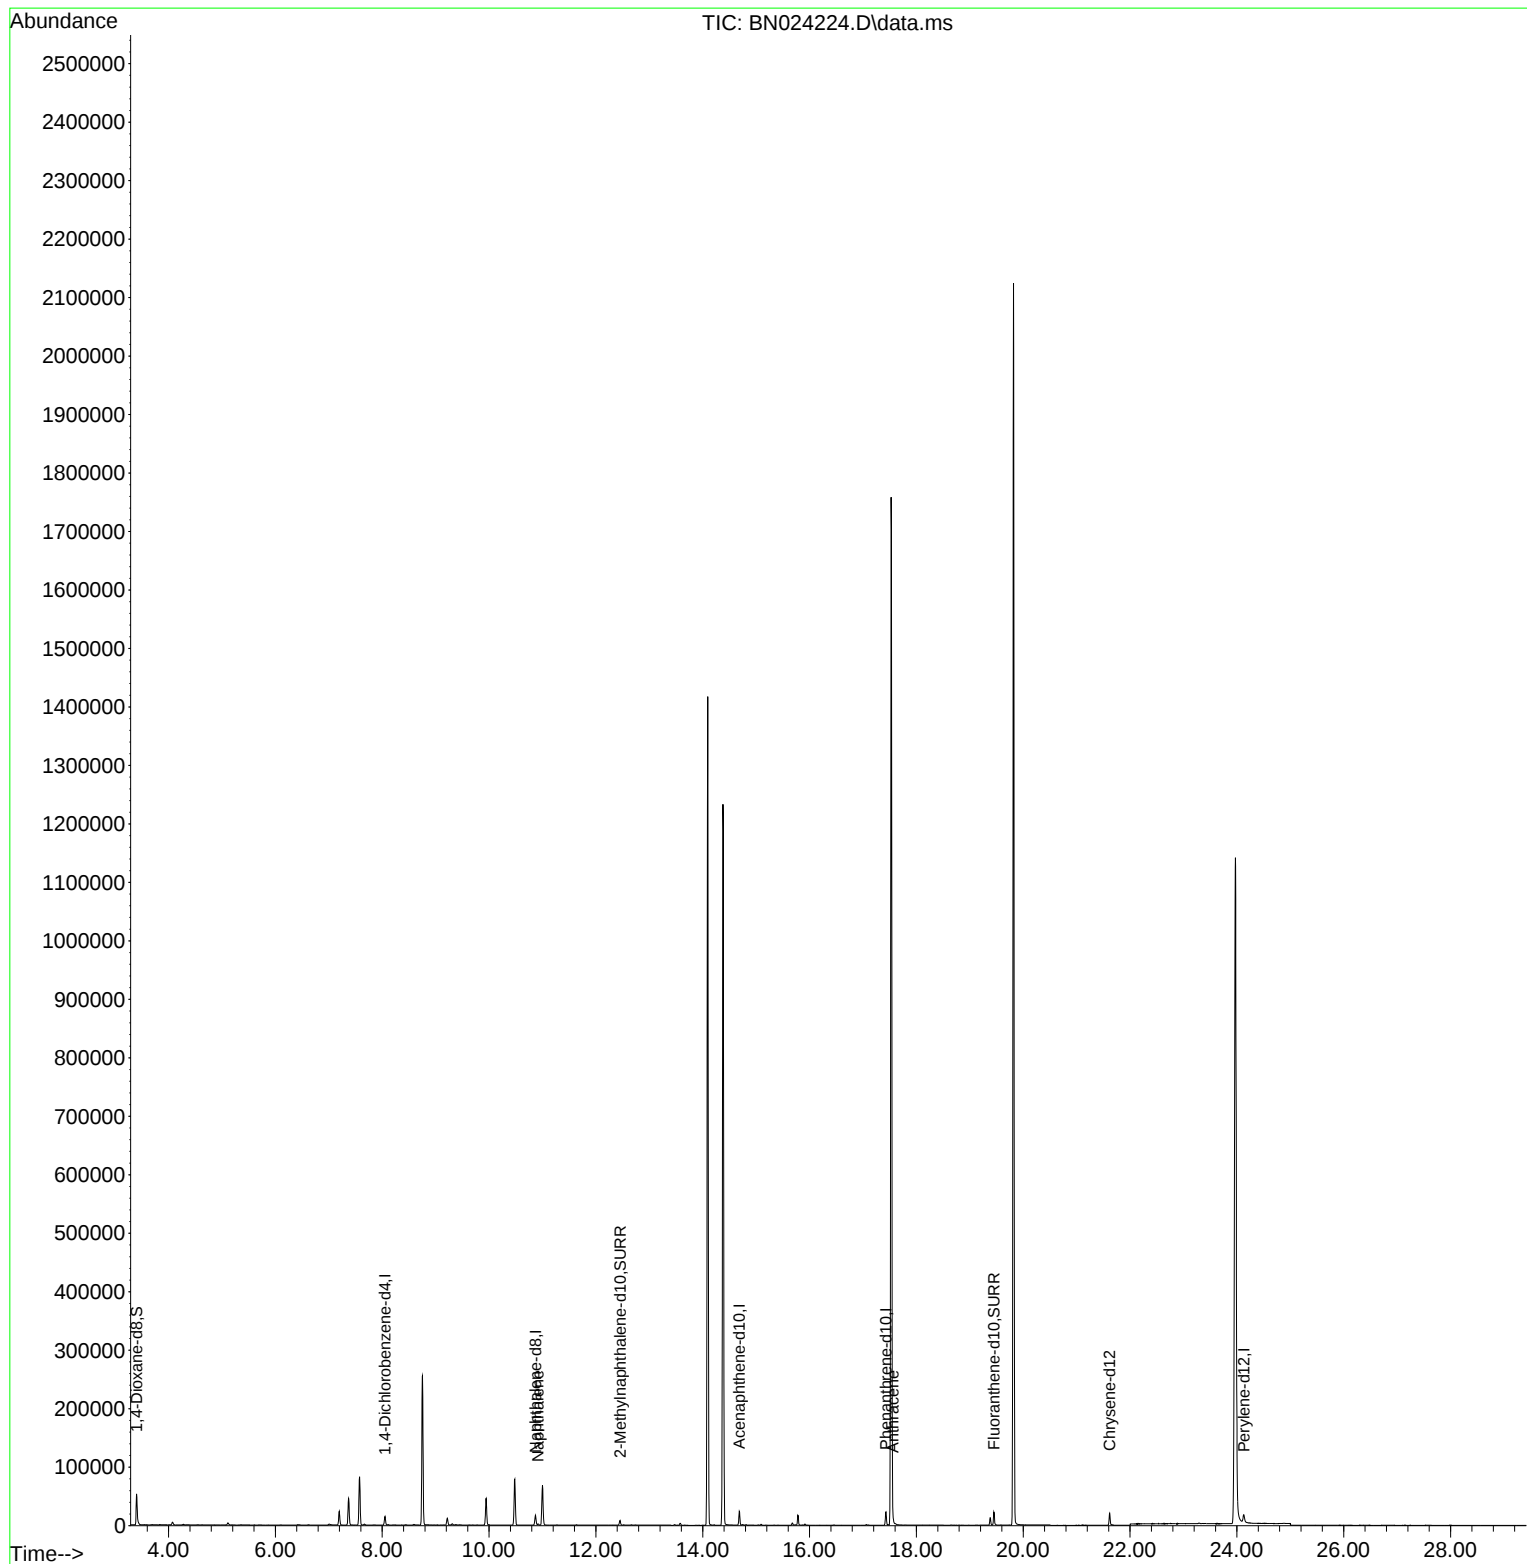


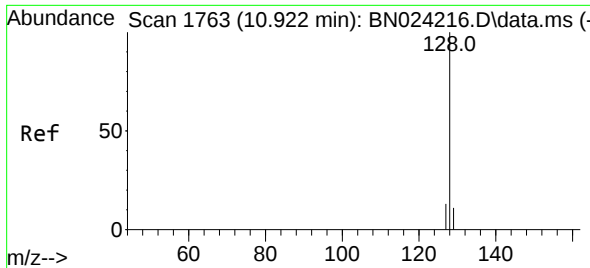

#5
Naphthalene
Concen: 0.052 ng/ul
RT: 10.916 min Scan# 1762
Delta R.T. -0.005 min
Lab File: BN024224.D
Acq: 10 Mar 2023 06:40

Instrument :
BNA_N
ClientSampleId :
DCAC4

Tgt Ion:128 Resp: 2877
Ion Ratio Lower Upper
128 100
129 15.5 9.0 13.6#
127 16.2 10.5 15.7#

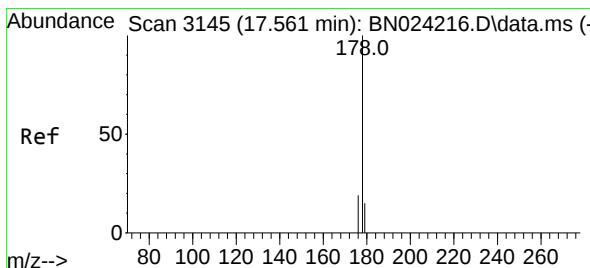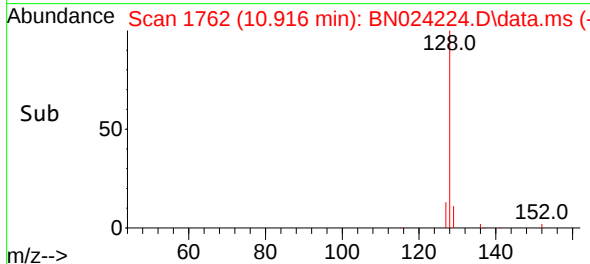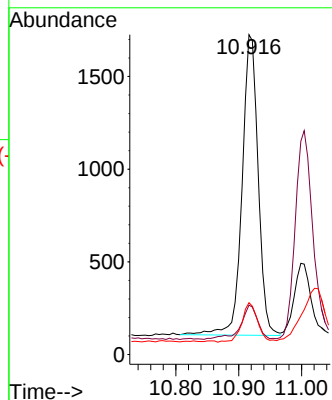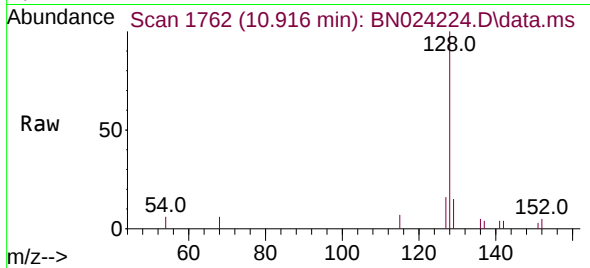

#16
Anthracene
Concen: 0.069 ng/ul
RT: 17.561 min Scan# 3145
Delta R.T. 0.000 min
Lab File: BN024224.D
Acq: 10 Mar 2023 06:40

Tgt Ion:178 Resp: 4498
Ion Ratio Lower Upper
178 100
179 18.9 12.3 18.5#
176 21.1 15.3 22.9

