


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN031419\
Data File : BN004757.D
Acq On : 14 Mar 2019 17:26
Operator : JU/SJ
Sample : DFTPP19
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP19

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN030719MA.M
Title : SVOA CALIBRATION
Last Update : Fri Mar 15 04:13:52 2019

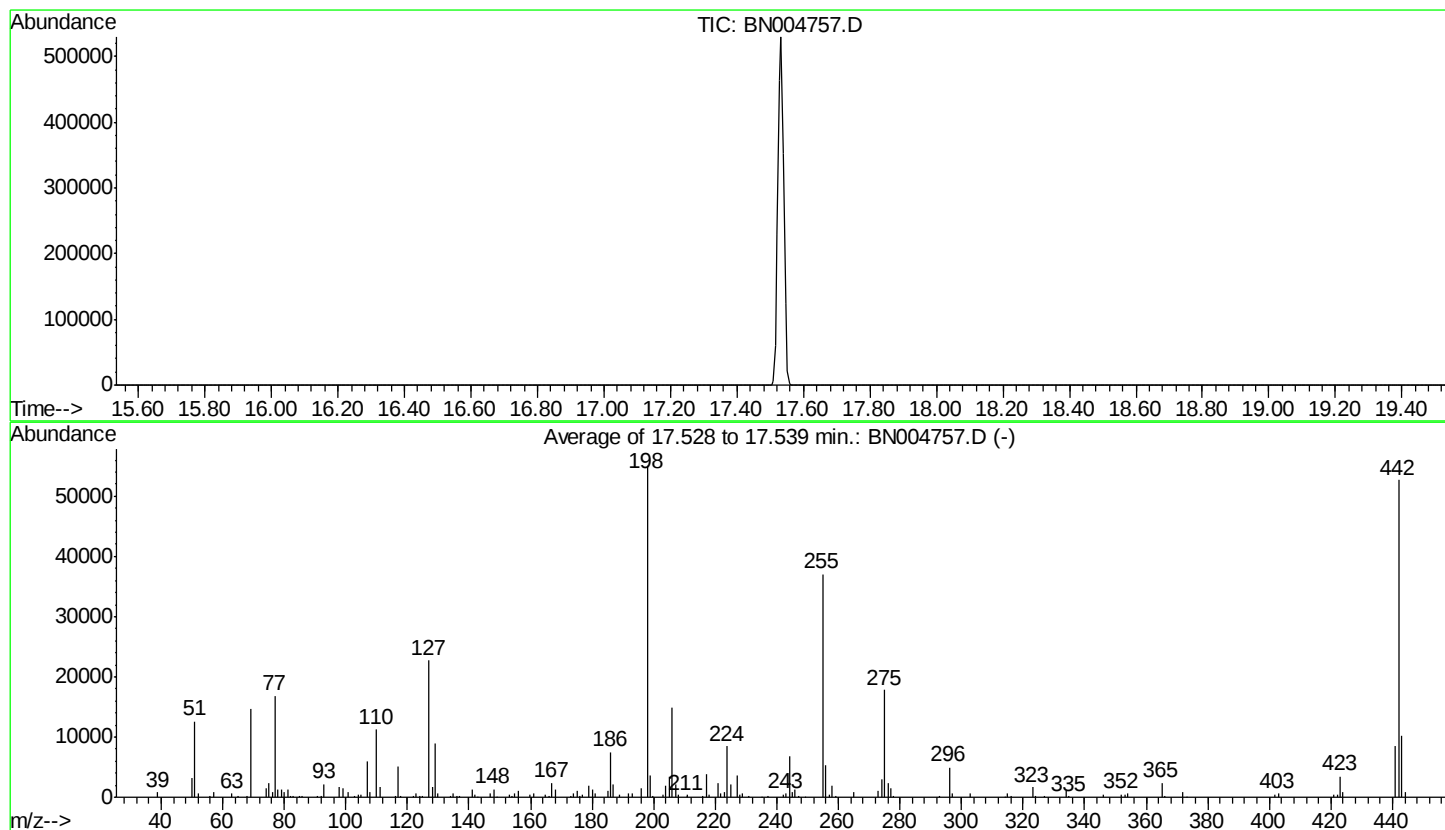

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.9	12585	PASS
68	69	0.00	2	1.5	224	PASS
69	198	0.00	100	26.7	14685	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.2	22675	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55072	PASS
199	198	5	9	6.6	3645	PASS
275	198	10	60	32.3	17806	PASS
365	198	1	100	4.4	2413	PASS
441	198	0.01	100	15.4	8467	PASS
442	198	50	100	95.7	52717	PASS
443	442	15	24	19.5	10266	PASS

m/z	Abundance
39.00	985.0
50.00	3740.0
51.00	15108.0
52.00	811.0
55.90	492.0
57.00	1095.0
63.00	702.0
65.00	348.0
68.10	335.0
69.00	17272.0
74.00	1900.0
75.00	2766.0
76.00	912.0
77.00	19496.0
78.00	1384.0
79.00	1469.0
80.00	1079.0
81.00	1519.0
81.90	360.0
82.90	357.0
84.90	370.0
85.90	446.0
90.90	361.0
92.00	377.0
93.00	2491.0
98.00	2031.0
99.00	1736.0
100.90	877.0
103.00	325.0
104.00	597.0
105.00	513.0
107.00	6804.0
108.00	1113.0
110.00	12693.0
111.00	2006.0
116.00	423.0
117.00	5559.0
117.90	408.0
122.00	415.0
122.90	781.0
124.00	332.0
125.00	317.0
127.00	25560.0
128.00	1950.0
129.00	10041.0
130.00	834.0
134.00	323.0
135.00	798.0
136.00	346.0
137.00	455.0
141.00	1422.0
141.90	403.0
142.90	302.0
147.00	679.0
148.00	1431.0
153.00	419.0
154.00	342.0
155.00	829.0
156.00	1112.0
160.00	408.0
161.00	633.0
164.90	499.0
166.00	409.0
167.00	2552.0
168.00	1587.0
173.00	304.0
174.00	563.0
175.00	1016.0
176.00	316.0
177.00	519.0
179.00	2076.0
180.00	1435.0
181.00	693.0
185.00	1097.0
186.00	7885.0
187.00	2314.0
188.90	516.0
192.00	662.0
193.00	733.0
196.00	1531.0
198.00	57928.0
199.00	4121.0
199.90	311.0
203.00	417.0
204.00	2124.0
205.00	3511.0
206.00	15321.0
207.00	2158.0
208.00	528.0
210.90	645.0
216.00	307.0

Instrument :
BNA_N
ClientSampleId :
DFTPP19

217.00	4062.0
218.00	515.0
221.00	2386.0
221.80	614.0
223.00	925.0
224.00	8867.0
225.00	2322.0
227.00	3697.0
228.00	502.0
229.00	742.0
231.00	332.0
237.00	430.0
242.00	445.0
243.00	509.0
244.00	7019.0
245.00	1004.0
246.00	1383.0
246.90	314.0
255.00	36904.0
256.00	5295.0
257.00	478.0
258.00	1944.0
258.90	380.0
265.00	820.0
273.00	1169.0
274.00	2936.0
275.00	17328.0
276.00	2298.0
277.00	1443.0
277.90	320.0
296.00	4694.0
297.00	707.0
303.00	531.0
315.00	544.0
316.00	312.0
323.00	1508.0
324.00	328.0
326.90	311.0
334.00	1011.0
345.90	328.0
351.90	511.0
353.00	329.0
354.00	548.0
365.00	2173.0
365.90	324.0
372.00	860.0
401.90	334.0
403.00	496.0
421.00	404.0
422.00	338.0
423.00	2937.0
424.00	841.0
441.00	7052.0
442.00	42864.0
443.00	8765.0
444.00	790.0

Instrument :
BNA_N
ClientSampleId :
DFTPP19

m/z	Abundance
39.00	971.0
50.00	3688.0
51.00	14424.0
52.00	681.0
55.90	433.0
57.00	1044.0
63.00	642.0
68.10	337.0
69.00	16880.0
74.00	1731.0
75.00	2775.0
76.10	992.0
77.00	19584.0
78.00	1394.0
79.00	1411.0
79.90	1050.0
81.00	1444.0
82.00	371.0
83.00	363.0
84.90	338.0
86.00	479.0
90.90	326.0
92.00	432.0
93.00	2549.0
98.00	1999.0
99.00	1637.0
100.90	917.0
102.90	308.0
103.90	572.0
104.90	577.0
107.00	6873.0
108.00	1053.0
110.00	13097.0
111.00	1940.0
116.00	424.0
117.00	5893.0
118.00	457.0
121.90	506.0
123.00	744.0
123.90	344.0
124.90	309.0
127.00	26272.0
128.00	2038.0
129.00	10262.0
130.00	903.0
134.00	308.0
135.00	843.0
137.00	478.0
141.00	1470.0
141.90	428.0
147.00	737.0
148.00	1611.0
149.00	317.0
152.90	443.0
153.90	373.0
155.00	840.0
156.00	1178.0
160.00	436.0
161.00	667.0
165.00	564.0
166.00	434.0
167.00	2874.0
168.00	1452.0
172.90	383.0
174.00	634.0
175.00	1162.0
176.00	304.0
177.00	601.0
179.00	2341.0
180.00	1672.0
181.00	782.0
185.00	1186.0
186.00	8793.0
187.00	2601.0
189.00	545.0
192.00	725.0
193.00	784.0
196.00	2012.0
198.00	64720.0
199.00	4206.0
199.90	308.0
202.90	428.0
204.00	2337.0
205.00	3933.0
206.00	17576.0
207.00	2338.0
208.00	592.0
211.10	623.0
216.00	371.0
217.00	4540.0
218.00	579.0

Instrument :
BNA_N
ClientSampleId :
DFTPP19

221.00	2774.0
221.80	673.0
223.00	1106.0
224.00	10004.0
225.00	2436.0
227.00	4247.0
228.00	611.0
229.00	857.0
231.00	415.0
235.00	304.0
237.00	374.0
242.00	559.0
243.00	631.0
244.00	8067.0
245.00	1082.0
246.00	1601.0
246.90	325.0
249.00	318.0
255.00	44232.0
256.00	6416.0
257.00	486.0
258.00	2450.0
259.00	410.0
265.00	962.0
273.00	1301.0
274.00	3607.0
275.00	21360.0
276.00	2789.0
277.00	1800.0
277.90	330.0
293.00	399.0
296.00	5863.0
297.00	761.0
303.00	751.0
313.90	305.0
315.00	694.0
316.00	401.0
323.00	2062.0
324.00	395.0
326.90	381.0
334.00	1301.0
335.00	380.0
345.90	463.0
352.00	605.0
353.00	433.0
354.00	653.0
365.00	2767.0
366.00	408.0
372.00	1097.0
373.00	309.0
401.90	534.0
403.00	637.0
421.00	581.0
422.00	582.0
423.00	4151.0
424.00	1011.0
441.10	10032.0
442.00	62280.0
443.00	11979.0
444.00	1021.0

Instrument :
BNA_N
ClientSampleId :
DFTPP19

m/z	Abundance
39.00	580.0
50.00	2100.0
51.00	8224.0
52.00	415.0
57.00	593.0
63.00	357.0
69.00	9905.0
74.00	1094.0
75.00	1663.0
76.00	603.0
77.00	11610.0
78.00	822.0
79.00	855.0
80.00	634.0
81.00	915.0
93.00	1540.0
98.00	1187.0
99.00	980.0
100.90	513.0
103.90	307.0
104.90	344.0
107.00	4271.0
108.00	668.0
110.00	7917.0
111.00	1166.0
117.00	3624.0
123.00	451.0
127.00	16193.0
128.00	1203.0
129.00	6331.0
129.90	512.0
135.00	561.0
141.00	915.0
142.00	310.0
147.00	429.0
148.00	1079.0
153.00	316.0
155.00	516.0
156.00	789.0
159.90	347.0
160.90	448.0
164.90	359.0
167.00	1768.0
168.00	875.0
173.90	476.0
175.00	757.0
176.90	371.0
179.00	1487.0
180.00	985.0
181.00	453.0
185.00	721.0
186.00	5940.0
187.00	1781.0
188.90	379.0
192.00	492.0
193.00	570.0
196.00	1198.0
198.00	42568.0
198.90	2610.0
203.00	339.0
204.00	1540.0
205.00	2744.0
206.00	11675.0
207.00	1591.0
208.00	400.0
210.90	488.0
217.00	3091.0
218.00	389.0
221.00	1948.0
221.80	450.0
223.00	743.0
224.00	6639.0
225.00	1716.0
227.00	2798.0
228.00	393.0
228.90	587.0
242.00	353.0
243.00	483.0
244.00	5483.0
245.00	721.0
246.00	1078.0
255.00	29840.0
256.00	4244.0
257.00	365.0
258.00	1642.0
265.00	731.0
273.00	1008.0
274.00	2502.0
275.00	14731.0
276.00	1962.0
277.00	1226.0

Instrument :
BNA_N
ClientSampleId :
DFTPP19

296.00	4139.0
296.90	565.0
303.00	536.0
314.90	502.0
323.00	1500.0
334.00	1049.0
345.90	325.0
352.00	429.0
353.00	325.0
354.00	587.0
365.00	2301.0
372.00	858.0
401.90	368.0
402.90	562.0
421.00	447.0
421.90	457.0
423.00	3336.0
424.00	681.0
441.00	8317.0
442.00	53008.0
443.00	10055.0
444.00	889.0

Instrument :
BNA_N
ClientSampleId :
DFTPP19

m/z Abundance

Instrument :
BNA_N
ClientSampleId :
DFTPP19