

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024416.D
 Acq On : 20 Mar 2023 17:49
 Operator : CG/JU
 Sample : 01884-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB923

Quant Time: Mar 21 02:15:50 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:12:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.038	152	11519	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136	35751	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.670	164	20544	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188	42349	0.400	ng/ul	0.00
17) Chrysene-d12	21.606	240	33188	0.400	ng/ul	0.00
23) Perylene-d12	24.094	264	29944	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.397	96	51180	4.037	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	14493	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	32598	0.369	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.803	202	5027	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.936	252	8701	0.088	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024416.D
Acq On : 20 Mar 2023 17:49
Operator : CG/JU
Sample : 01884-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB923

Quant Time: Mar 21 02:15:50 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:12:19 2023
Response via : Initial Calibration




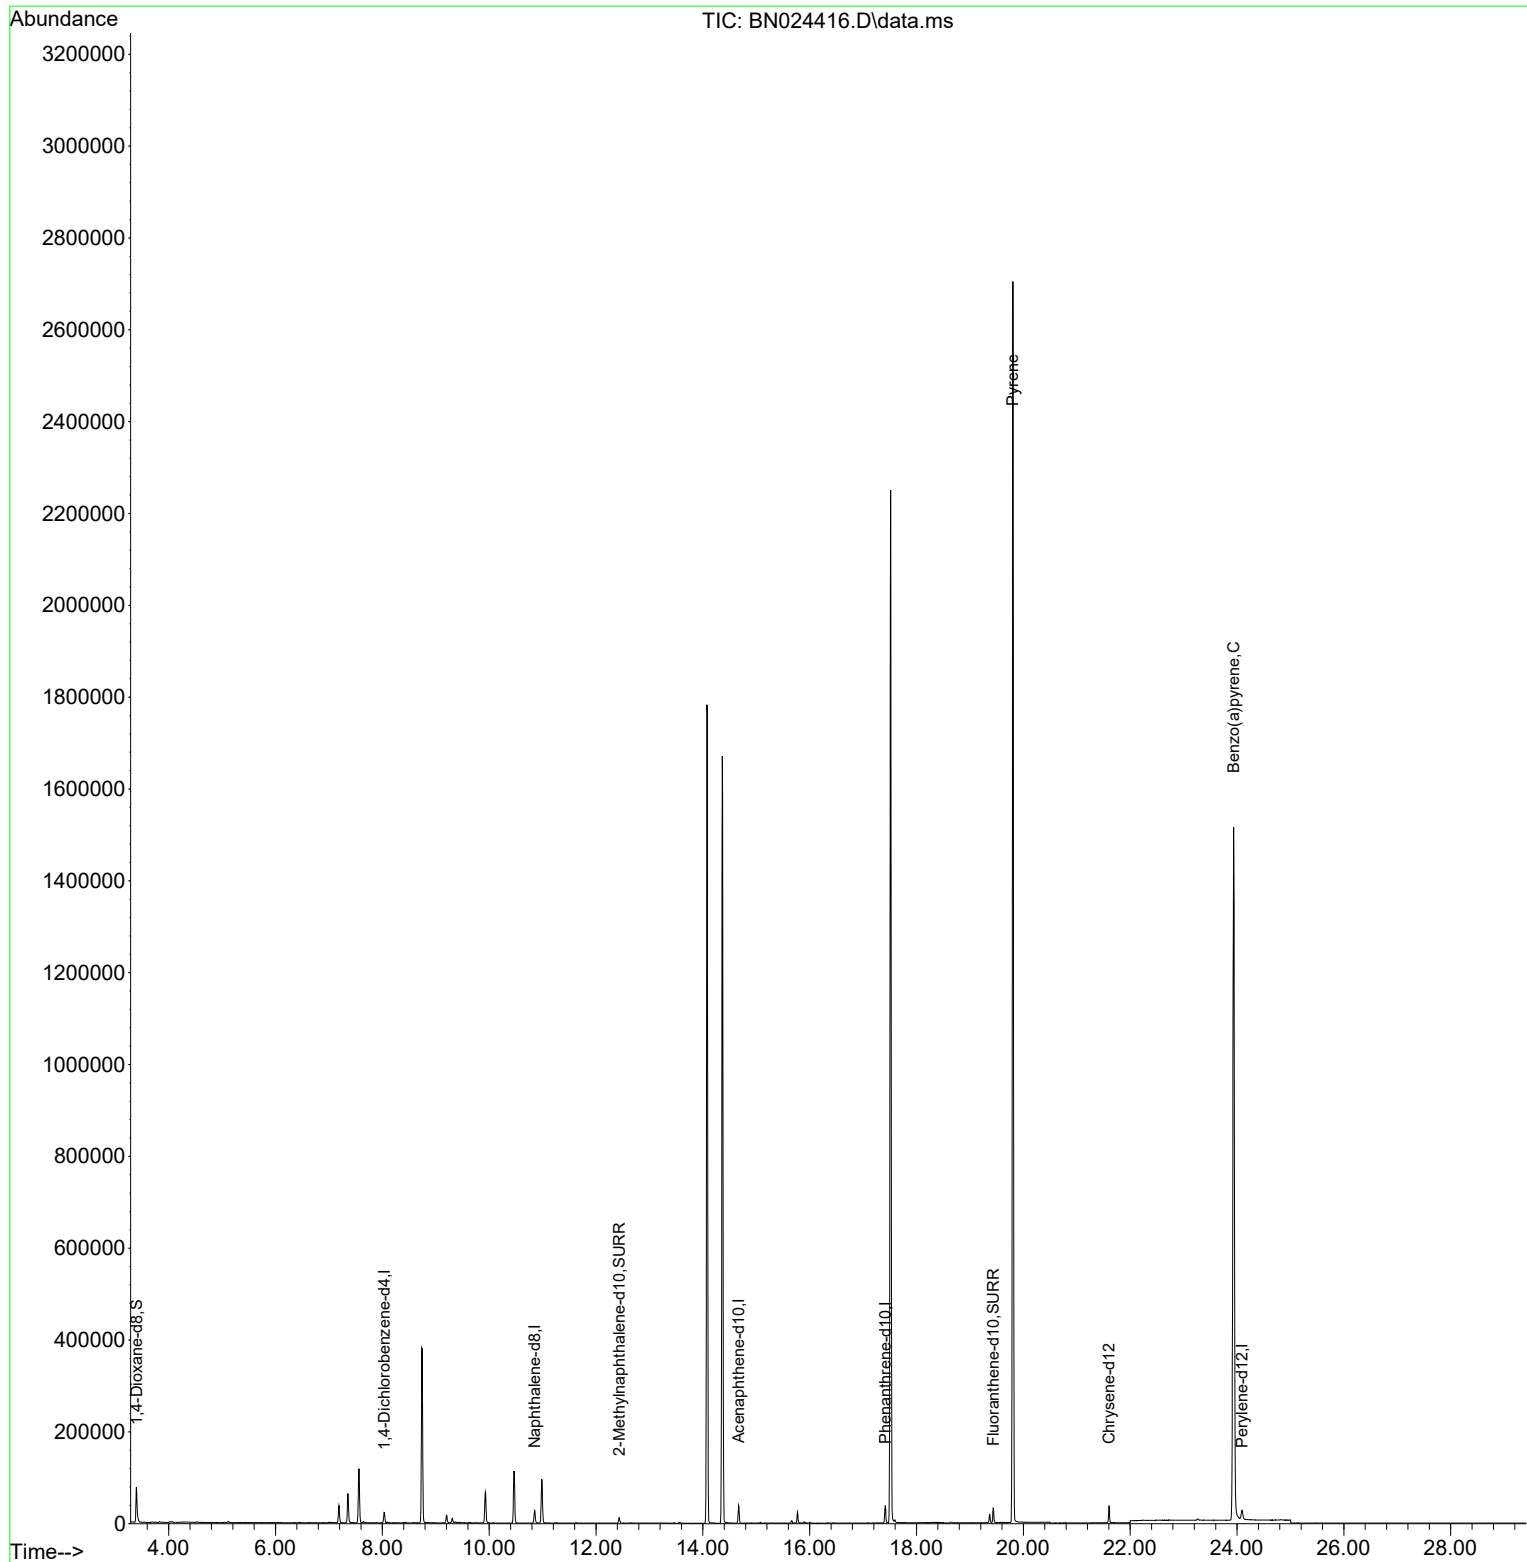


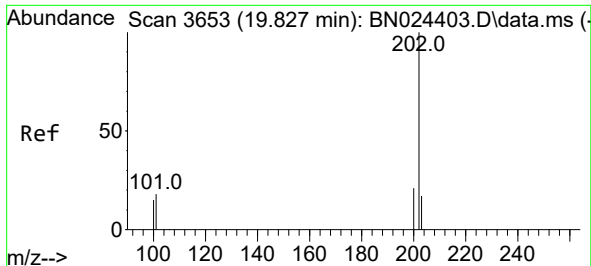

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.803 min Scan# 3648
Delta R.T. -0.024 min
Lab File: BN024416.D
Acq: 20 Mar 2023 17:49

Instrument :
BNA_N
ClientSampleId :
CB923

Tgt Ion:202 Resp: 5027
Ion Ratio Lower Upper
202 100
101 158.1 12.1 18.1#
100 1183.2 9.4 14.0#

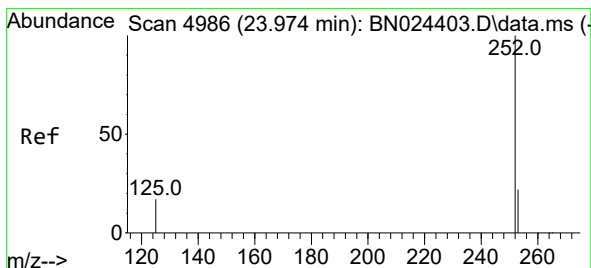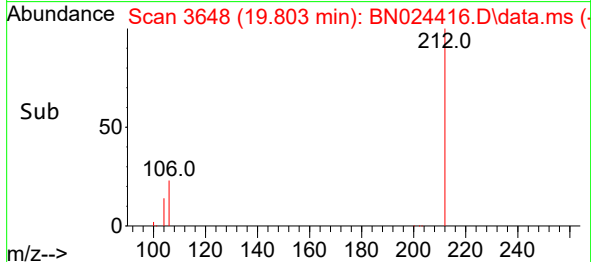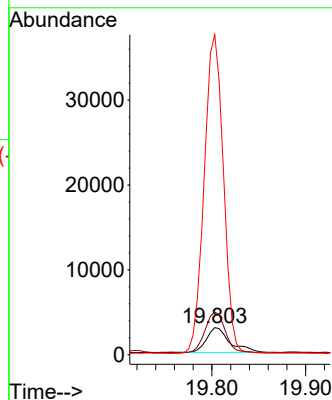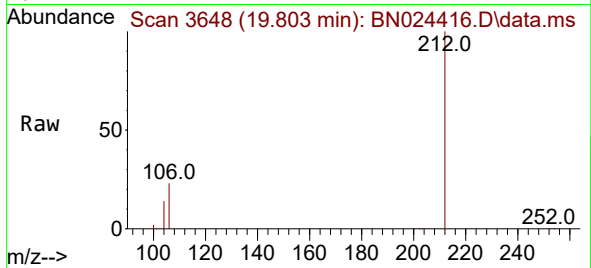

#26
Benzo(a)pyrene
Concen: 0.088 ng/ul
RT: 23.936 min Scan# 4973
Delta R.T. -0.038 min
Lab File: BN024416.D
Acq: 20 Mar 2023 17:49

Tgt Ion:252 Resp: 8701
Ion Ratio Lower Upper
252 100
253 45.9 19.2 28.8#
125 46.3 15.8 23.6#

