

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024421.D
 Acq On : 20 Mar 2023 21:29
 Operator : CG/JU
 Sample : PB151455BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK455

Quant Time: Mar 21 02:44:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:42:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	8571	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136	26767	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.670	164	15209	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	30339	0.400	ng/ul	0.00
17) Chrysene-d12	21.597	240	21595	0.400	ng/ul	0.00
23) Perylene-d12	24.088	264	20825	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.397	96	75124	7.965	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	14915	0.469	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	28273	0.492	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.665	166	4676	0.086	ng/ul#	13
20) Pyrene	19.803	202	4165	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.927	252	7798	0.114	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024421.D
Acq On : 20 Mar 2023 21:29
Operator : CG/JU
Sample : PB151455BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK455

Quant Time: Mar 21 02:44:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:42:36 2023
Response via : Initial Calibration




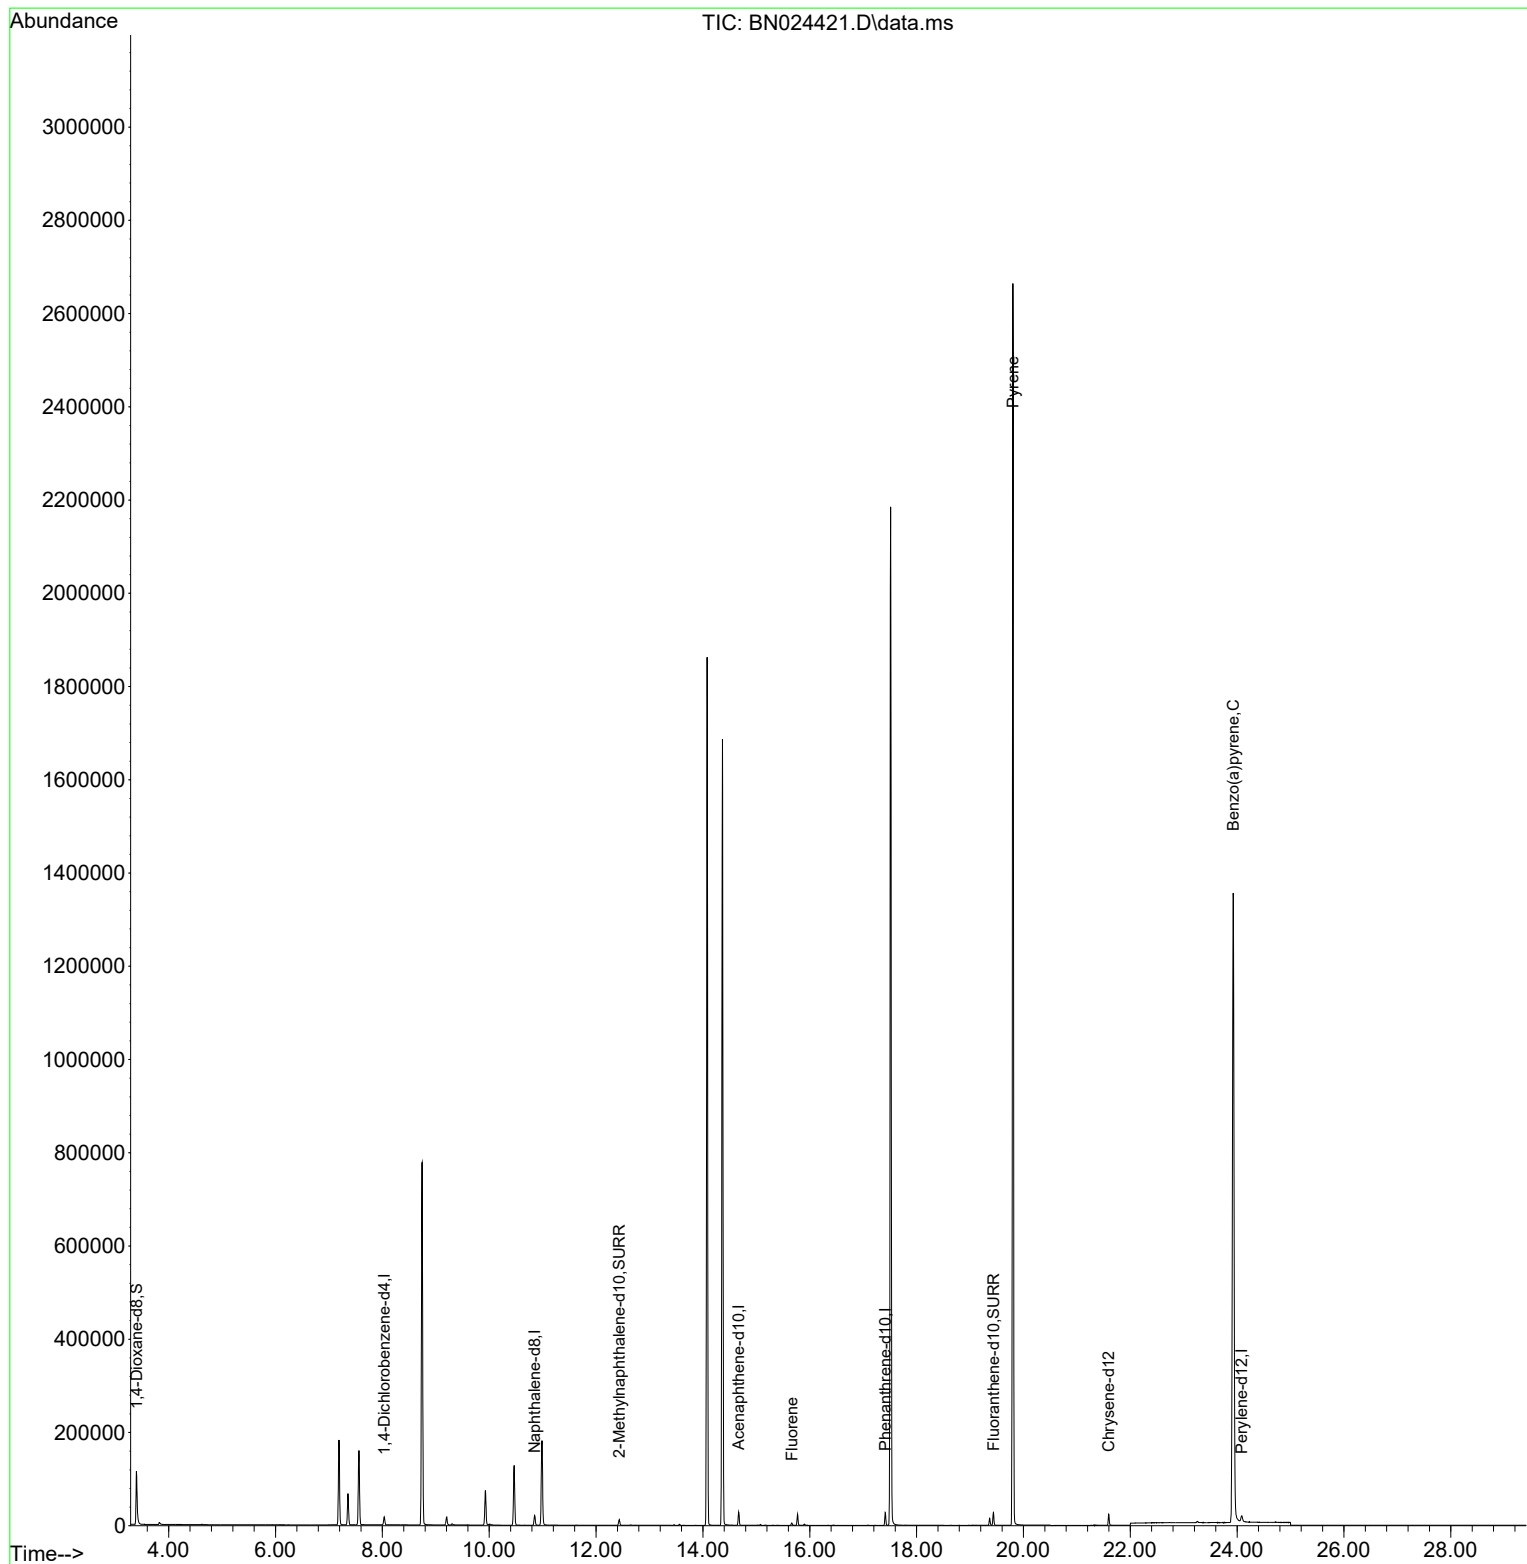


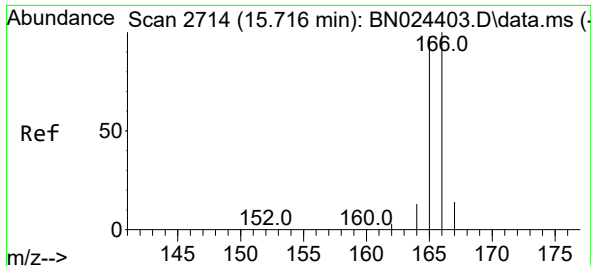

#12
Fluorene
Concen: 0.086 ng/ul
RT: 15.665 min Scan# 21
Delta R.T. -0.051 min
Lab File: BN024421.D
Acq: 20 Mar 2023 21:29




Instrument :
BNA_N
ClientSampleId :
SBLK455


Tgt Ion:166 Resp: 4676
Ion Ratio Lower Upper
166 100
165 7.3 77.4 116.0#
167 36.0 10.9 16.3#

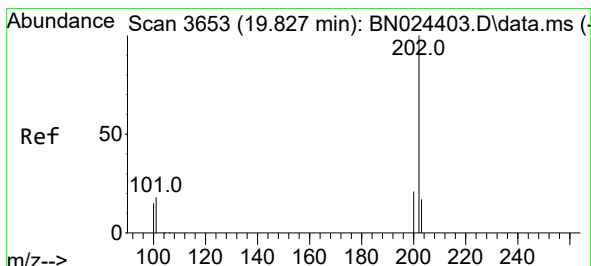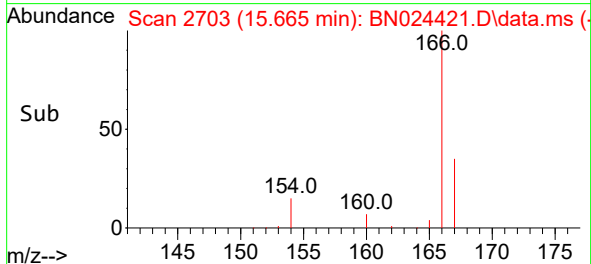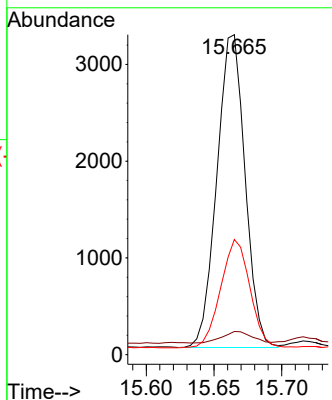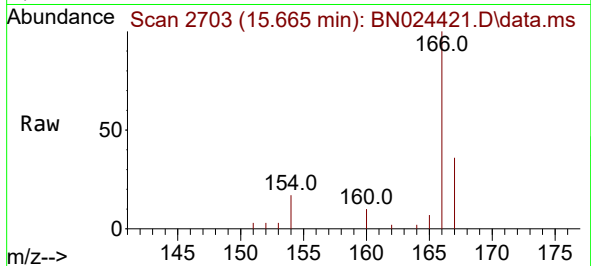

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.803 min Scan# 3648
Delta R.T. -0.028 min
Lab File: BN024421.D
Acq: 20 Mar 2023 21:29


Tgt Ion:202 Resp: 4165
Ion Ratio Lower Upper
202 100
101 167.3 12.1 18.1#
100 1250.2 9.4 14.0#

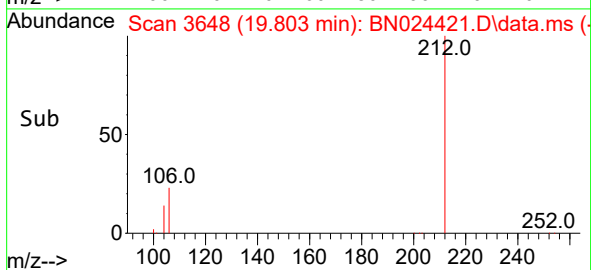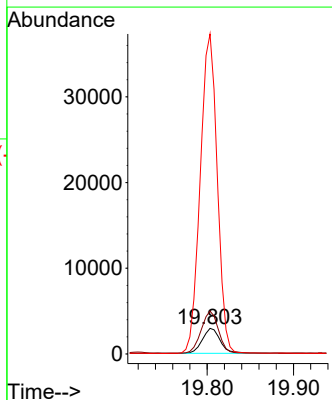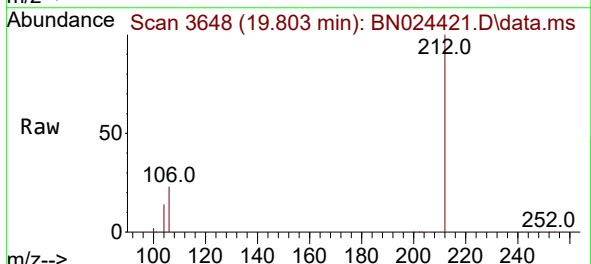

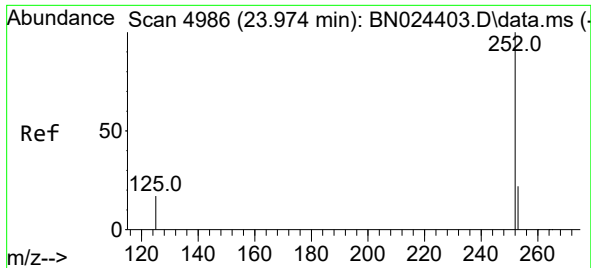

#26
Benzo(a)pyrene
Concen: 0.114 ng/ul
RT: 23.927 min Scan# 49
Delta R.T. -0.062 min
Lab File: BN024421.D
Acq: 20 Mar 2023 21:29

Instrument :
BNA_N
ClientSampleId :
SBLK455

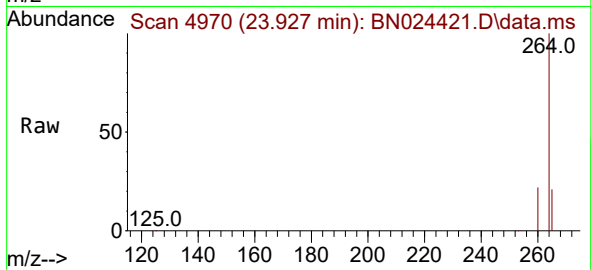

Tgt Ion:252 Resp: 7798
Ion Ratio Lower Upper
252 100
253 46.0 19.2 28.8#
125 43.9 15.8 23.6#

