

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024422.D
 Acq On : 20 Mar 2023 22:05
 Operator : CG/JU
 Sample : 01884-03DL 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB908DL

Quant Time: Mar 21 02:44:44 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:42:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	12606	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136	40957	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.670	164	23784	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	50347	0.400	ng/ul	0.00
17) Chrysene-d12	21.603	240	34525	0.400	ng/ul	0.00
23) Perylene-d12	24.100	264	27597	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.401	96	3976	0.287	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	2530	0.052	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	5217	0.057	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.435	88	78714	5.216	ng/ul	88
11) Acenaphthene	14.731	153	39503	0.517	ng/ul	98
12) Fluorene	15.716	166	29067	0.340	ng/ul	98
15) Phenanthrene	17.456	178	4855	0.034	ng/ul#	87
16) Anthracene	17.544	178	3332	0.026	ng/ul#	78
19) Fluoranthene	19.469	202	3253	0.024	ng/ul#	82
20) Pyrene	19.831	202	3234	0.023	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024422.D
Acq On : 20 Mar 2023 22:05
Operator : CG/JU
Sample : 01884-03DL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB908DL

Quant Time: Mar 21 02:44:44 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:42:36 2023
Response via : Initial Calibration




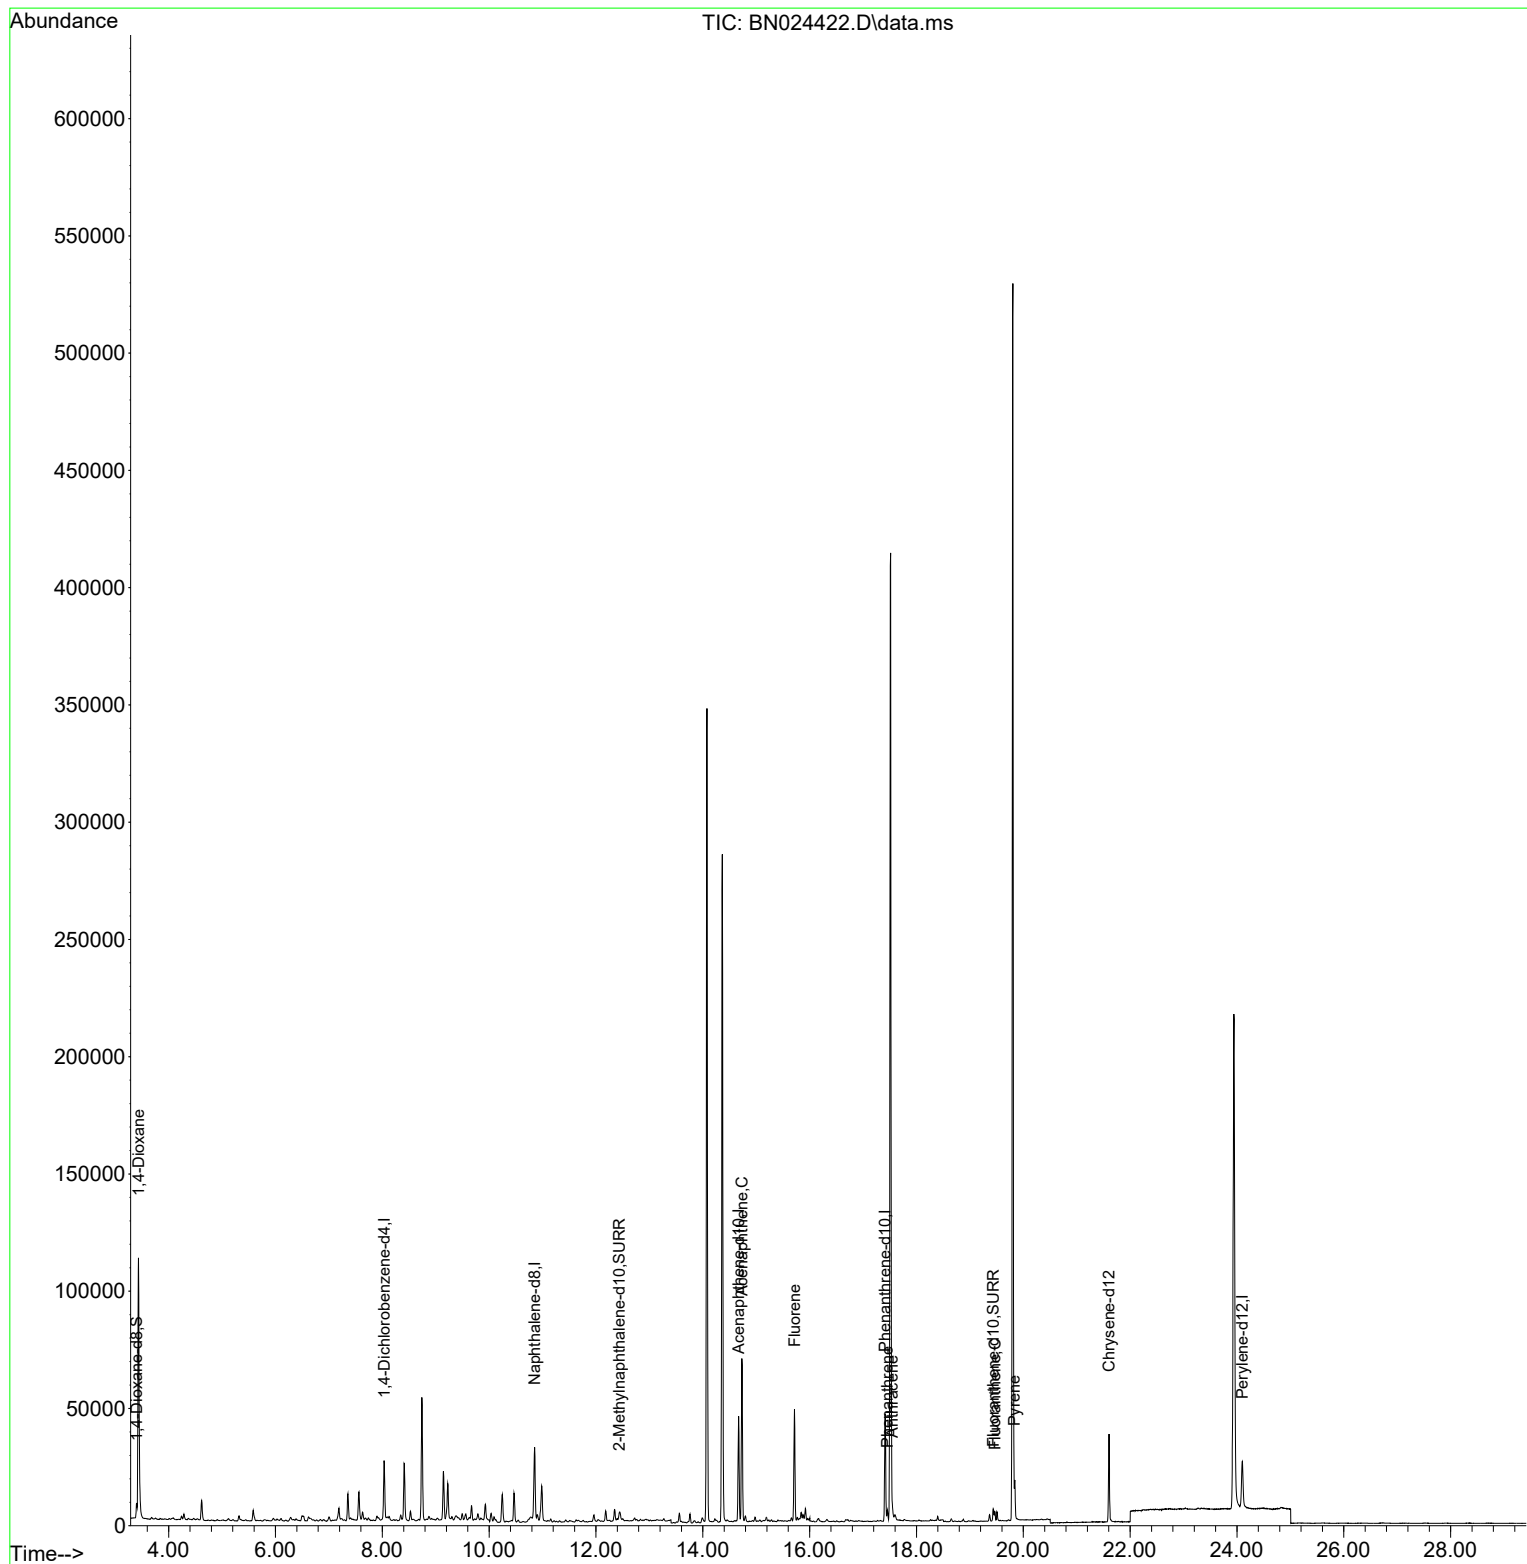


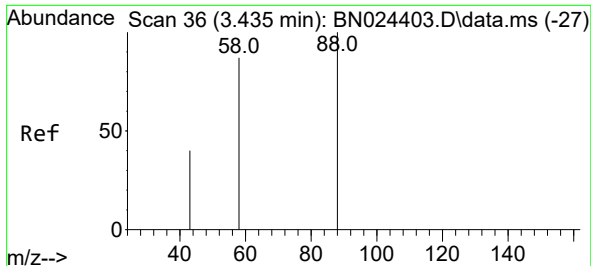

#2
 1,4-Dioxane
 Concen: 5.216 ng/ul
 RT: 3.435 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BN024422.D
 Acq: 20 Mar 2023 22:05




Instrument :
 BNA_N
 ClientSampleId :
 CB908DL


Tgt Ion: 88 Resp: 78714
 Ion Ratio Lower Upper
 88 100
 43 35.5 32.1 48.1
 58 81.0 55.1 82.7

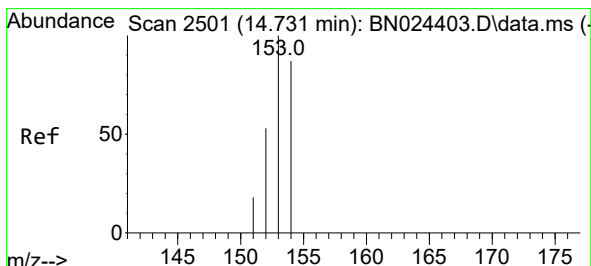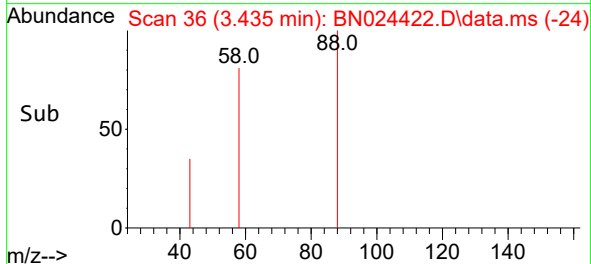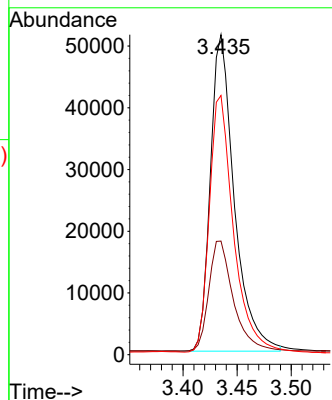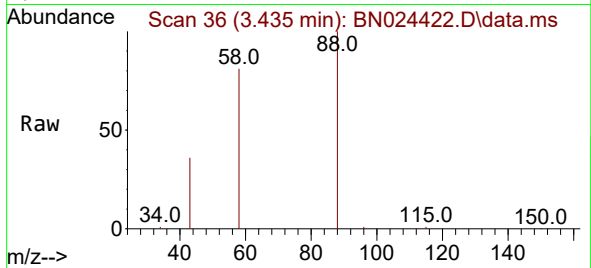

#11
 Acenaphthene
 Concen: 0.517 ng/ul
 RT: 14.731 min Scan# 2501
 Delta R.T. -0.000 min
 Lab File: BN024422.D
 Acq: 20 Mar 2023 22:05

Tgt Ion: 153 Resp: 39503
 Ion Ratio Lower Upper
 153 100
 152 50.1 42.6 64.0
 154 87.1 70.6 105.8


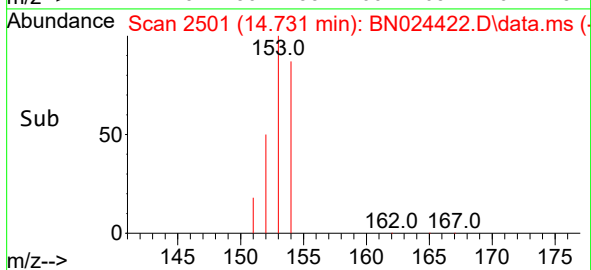
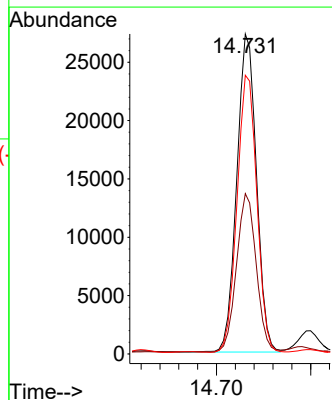
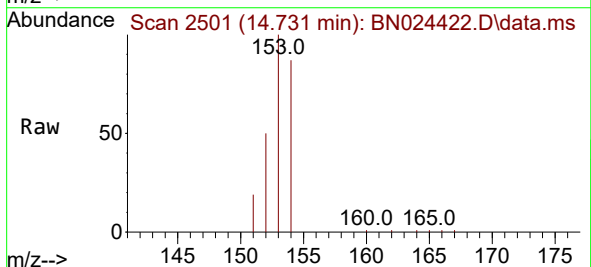


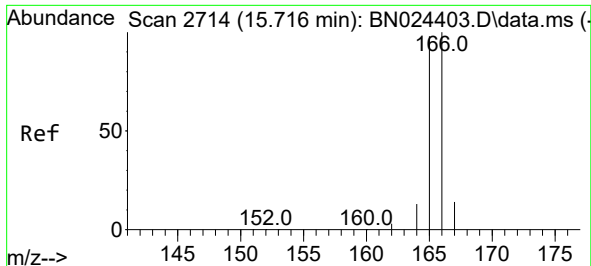

#12
Fluorene
Concen: 0.340 ng/ul
RT: 15.716 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN024422.D
Acq: 20 Mar 2023 22:05




Instrument :
BNA_N
ClientSampleId :
CB908DL


Tgt Ion:166 Resp: 29067
Ion Ratio Lower Upper
166 100
165 98.4 77.4 116.0
167 14.3 10.9 16.3

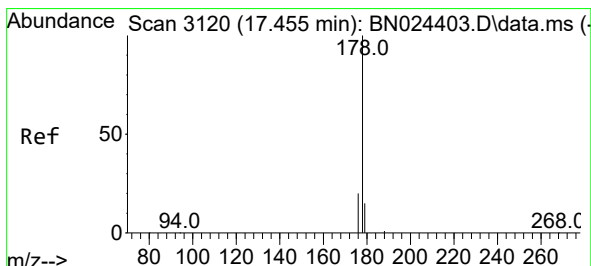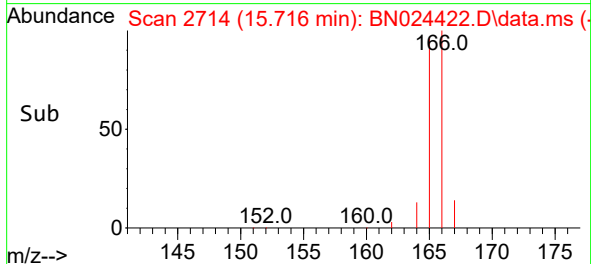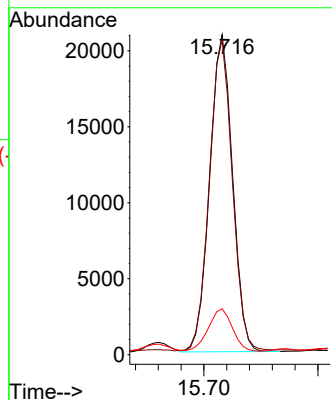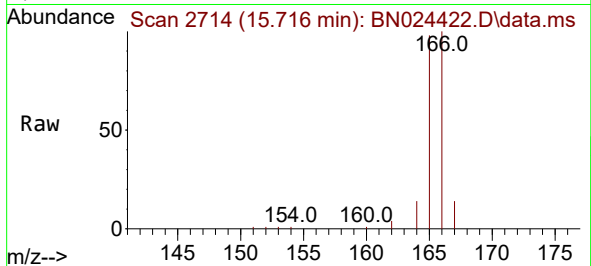

#15
Phenanthrene
Concen: 0.034 ng/ul
RT: 17.456 min Scan# 3120
Delta R.T. -0.000 min
Lab File: BN024422.D
Acq: 20 Mar 2023 22:05

Tgt Ion:178 Resp: 4855
Ion Ratio Lower Upper
178 100
179 22.2 12.2 18.2#
176 24.3 15.7 23.5#


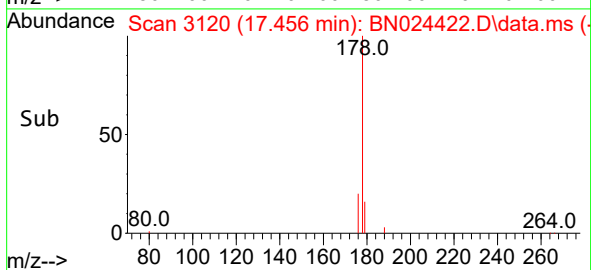
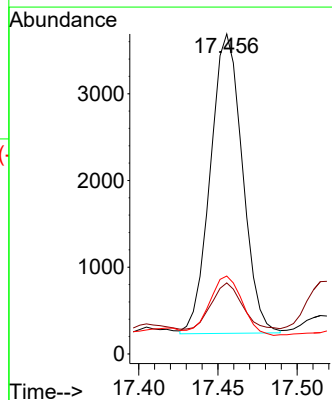
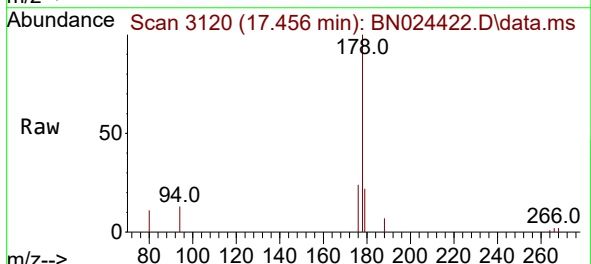


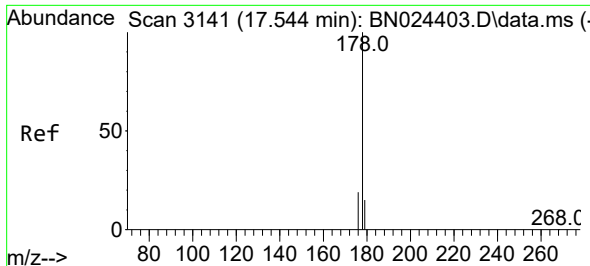

#16
 Anthracene
 Concen: 0.026 ng/ul
 RT: 17.544 min Scan# 3141
 Delta R.T. -0.004 min
 Lab File: BN024422.D
 Acq: 20 Mar 2023 22:05




Instrument :
 BNA_N
 ClientSampleId :
 CB908DL


Tgt Ion:178 Resp: 3332
 Ion Ratio Lower Upper
 178 100
 179 26.4 12.3 18.5#
 176 27.8 15.3 22.9#

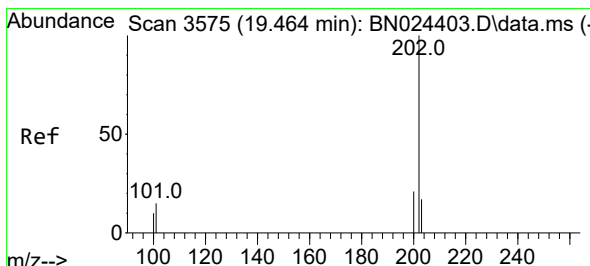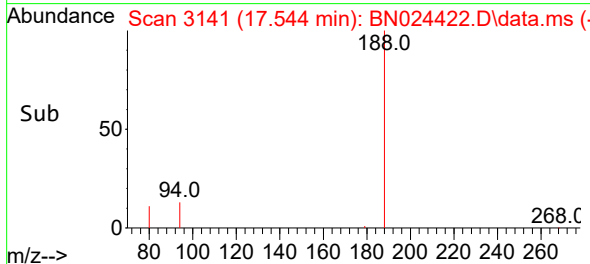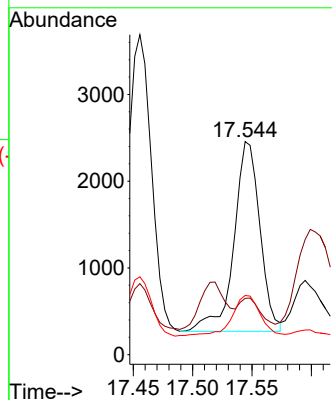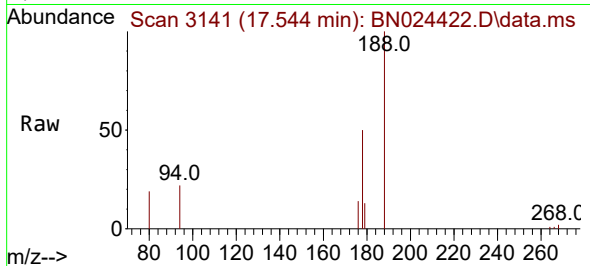

#19
 Fluoranthene
 Concen: 0.024 ng/ul
 RT: 19.469 min Scan# 3576
 Delta R.T. 0.000 min
 Lab File: BN024422.D
 Acq: 20 Mar 2023 22:05

Tgt Ion:202 Resp: 3253
 Ion Ratio Lower Upper
 202 100
 101 21.5 10.4 15.6#
 100 14.4 7.7 11.5#

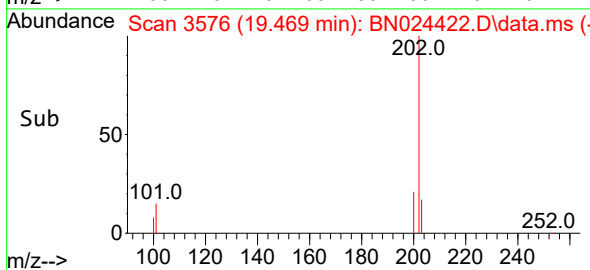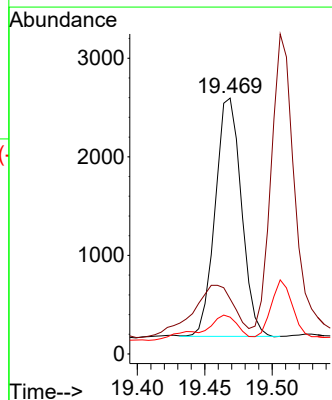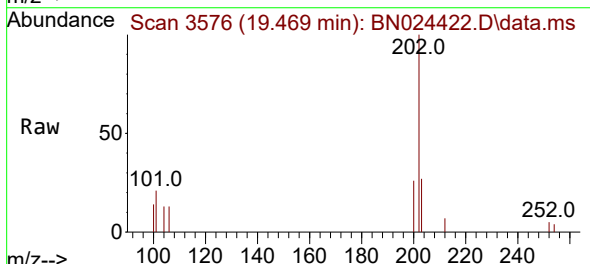

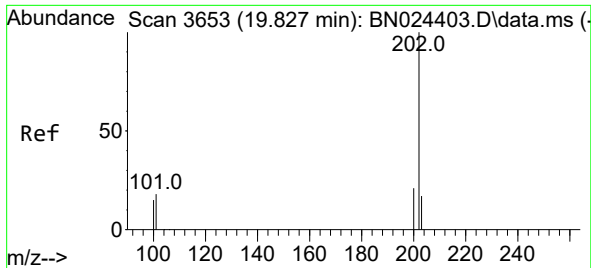

#20

Pyrene

Concen: 0.023 ng/ul

RT: 19.831 min Scan# 30

Delta R.T. 0.000 min

Lab File: BN024422.D


Acq: 20 Mar 2023 22:05

Instrument :

BNA_N

ClientSampleId :

CB908DL

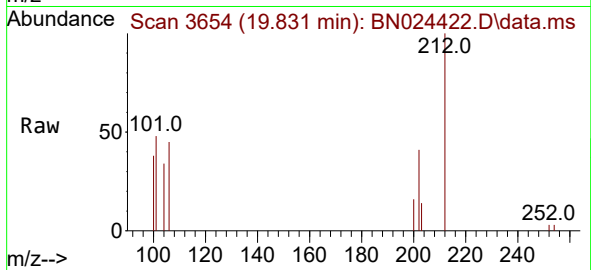

Tgt Ion:202 Resp: 3234

Ion Ratio Lower Upper

202 100

101 114.8 12.1 18.1#

100 91.9 9.4 14.0#

