

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024428.D
 Acq On : 21 Mar 2023 01:46
 Operator : CG/JU
 Sample : 01885-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB923

Quant Time: Mar 21 02:45:26 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:42:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	10821	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136	33827	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.671	164	19676	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	41026	0.400	ng/ul	0.00
17) Chrysene-d12	21.592	240	32543	0.400	ng/ul	0.00
23) Perylene-d12	24.094	264	30043	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.397	96	47822	4.016	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	14302	0.356	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	32945	0.380	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.803	202	5015	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.933	252	8918	0.090	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024428.D
Acq On : 21 Mar 2023 01:46
Operator : CG/JU
Sample : 01885-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB923

Quant Time: Mar 21 02:45:26 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:42:36 2023
Response via : Initial Calibration




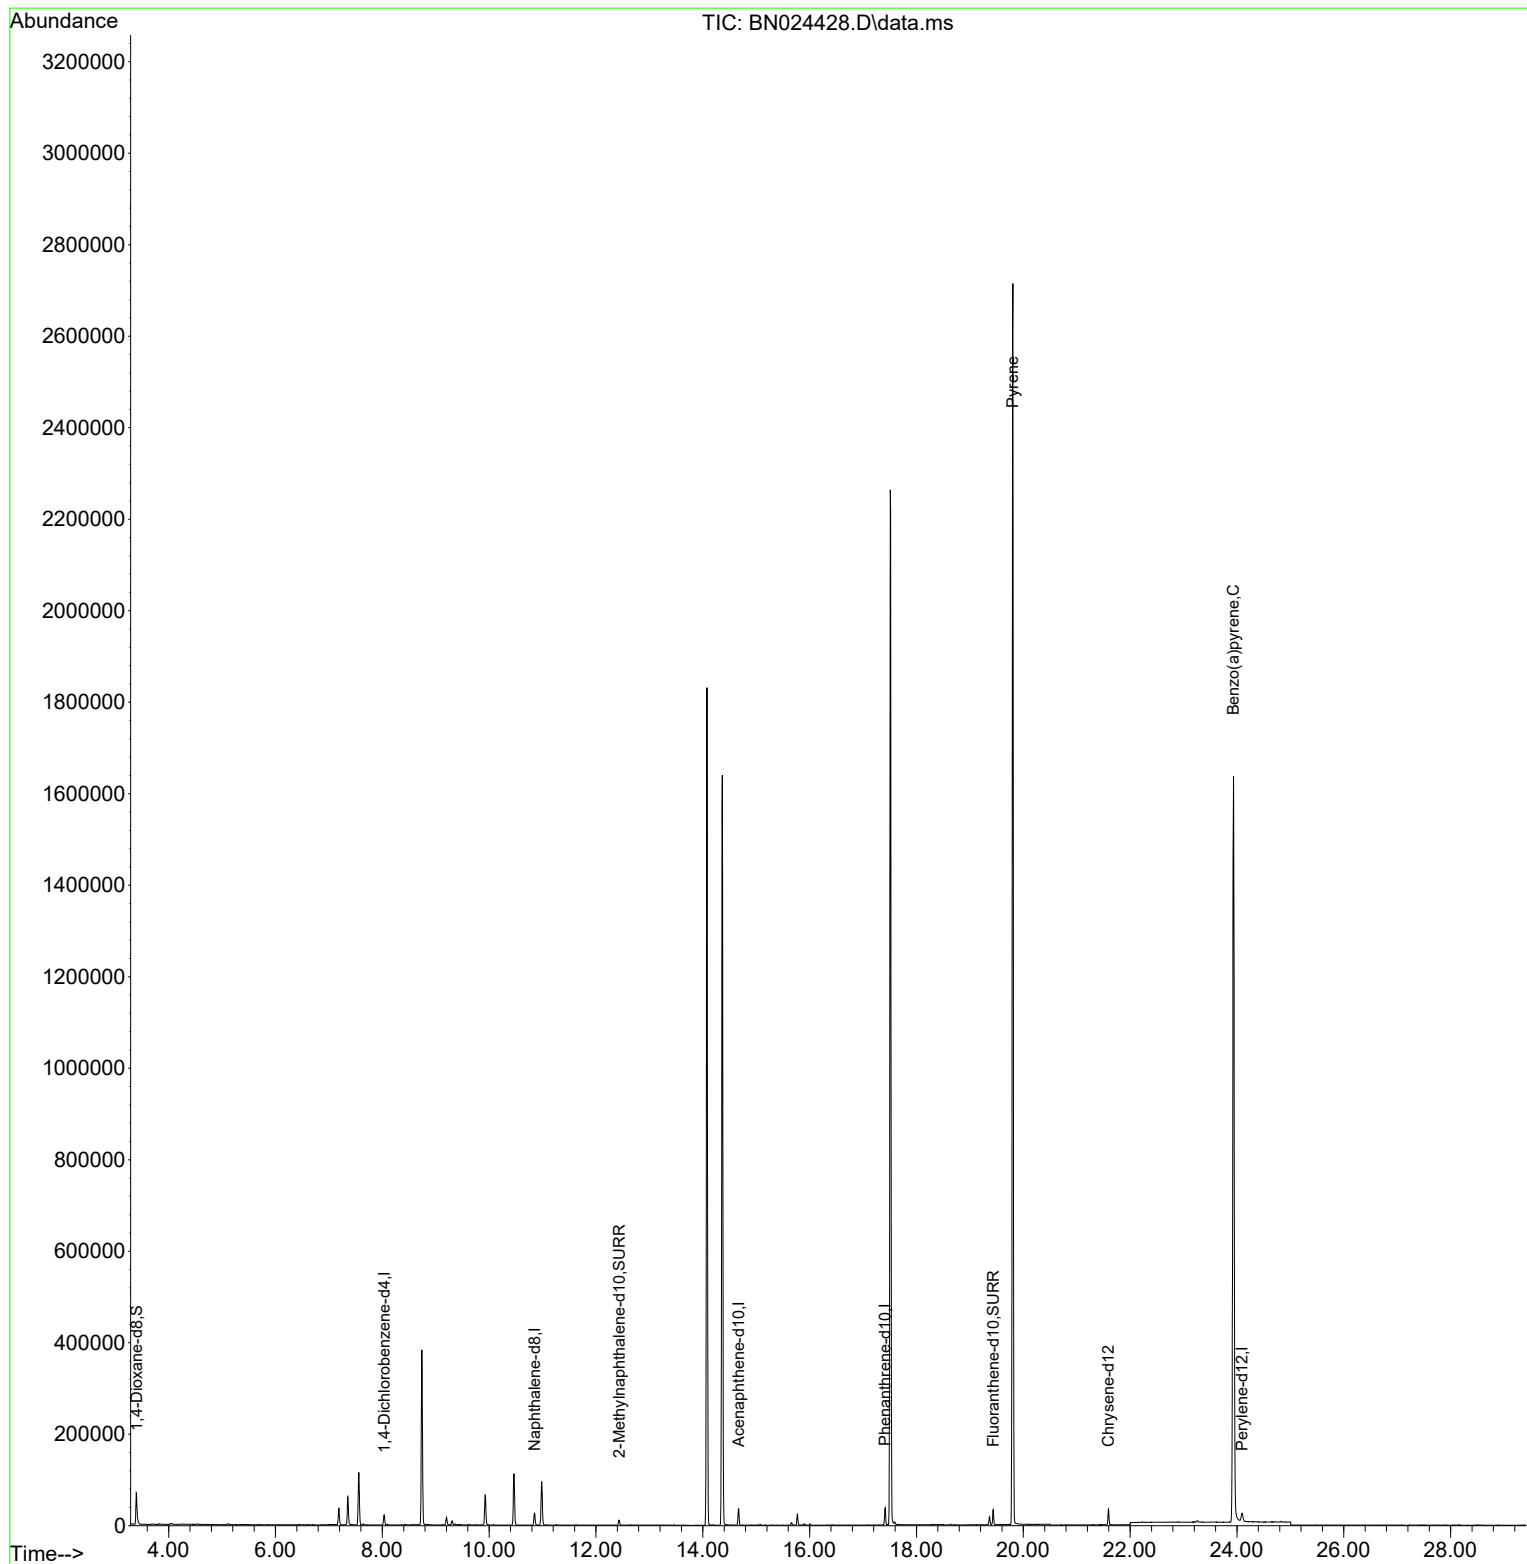


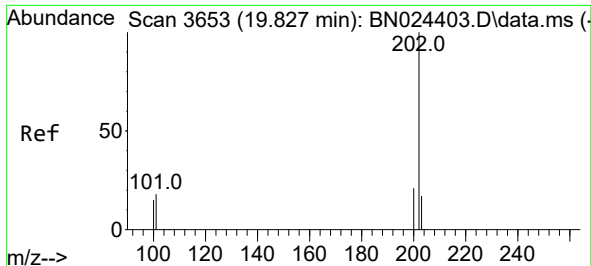

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.803 min Scan# 3648
Delta R.T. -0.028 min
Lab File: BN024428.D
Acq: 21 Mar 2023 01:46

Instrument :
BNA_N
ClientSampleId :
CB923

Tgt Ion:202 Resp: 5015
Ion Ratio Lower Upper
202 100
101 157.4 12.1 18.1#
100 1107.9 9.4 14.0#

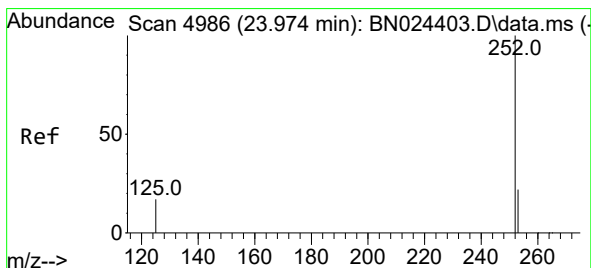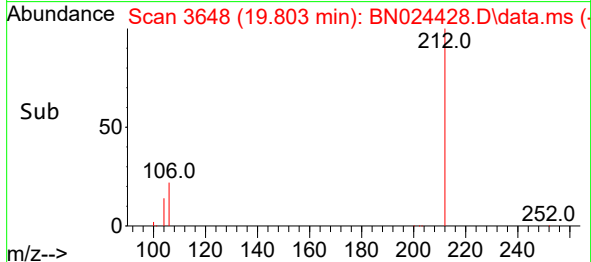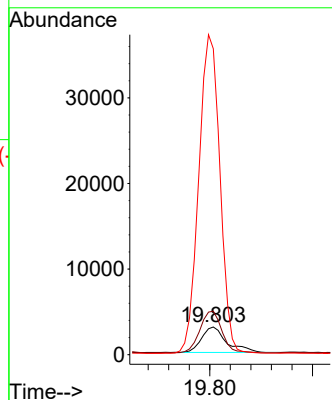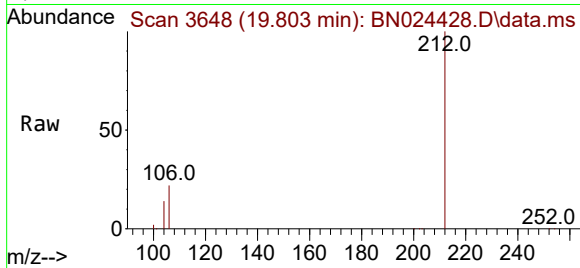

#26
Benzo(a)pyrene
Concen: 0.090 ng/ul
RT: 23.933 min Scan# 4972
Delta R.T. -0.055 min
Lab File: BN024428.D
Acq: 21 Mar 2023 01:46

Tgt Ion:252 Resp: 8918
Ion Ratio Lower Upper
252 100
253 45.5 19.2 28.8#
125 44.2 15.8 23.6#

