




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024405.D
 Acq On : 20 Mar 2023 11:08
 Operator : CG/JU
 Sample : PB151451BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS451

Manual IntegrationsAPPROVED

Quant Time: Mar 21 02:14:23 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:12:19 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/21/2023
 Supervised By :Jagrut Upadhyay 03/21/2023

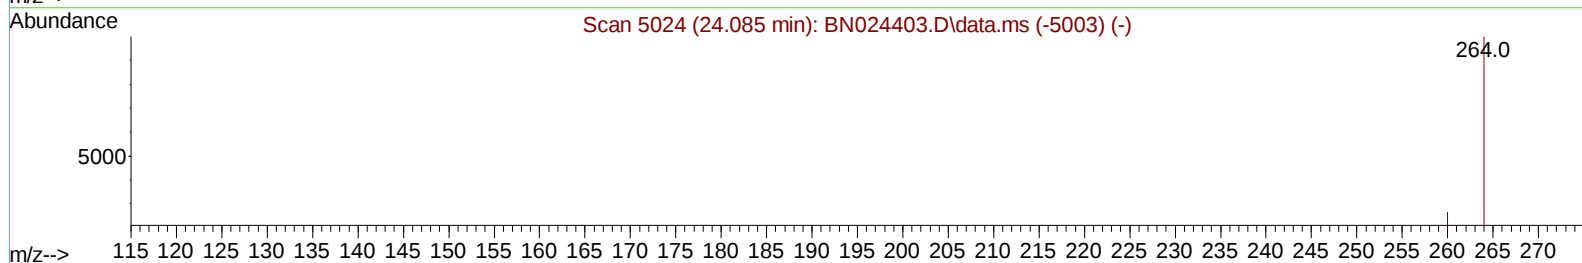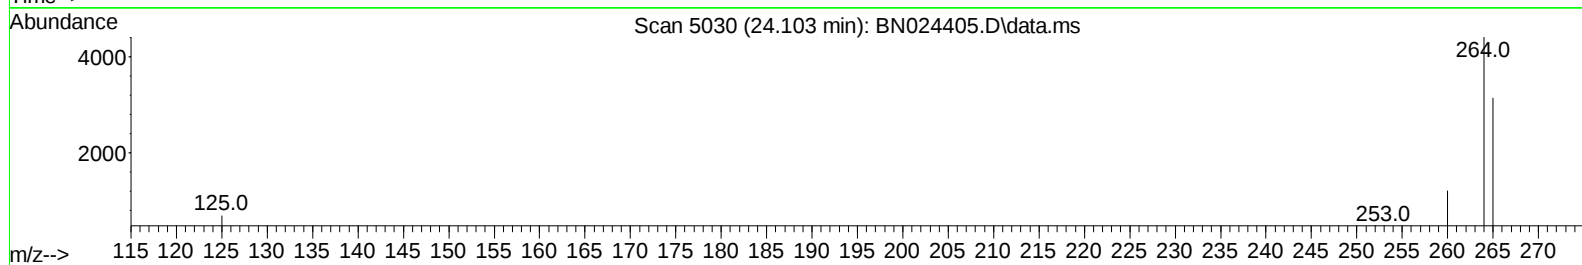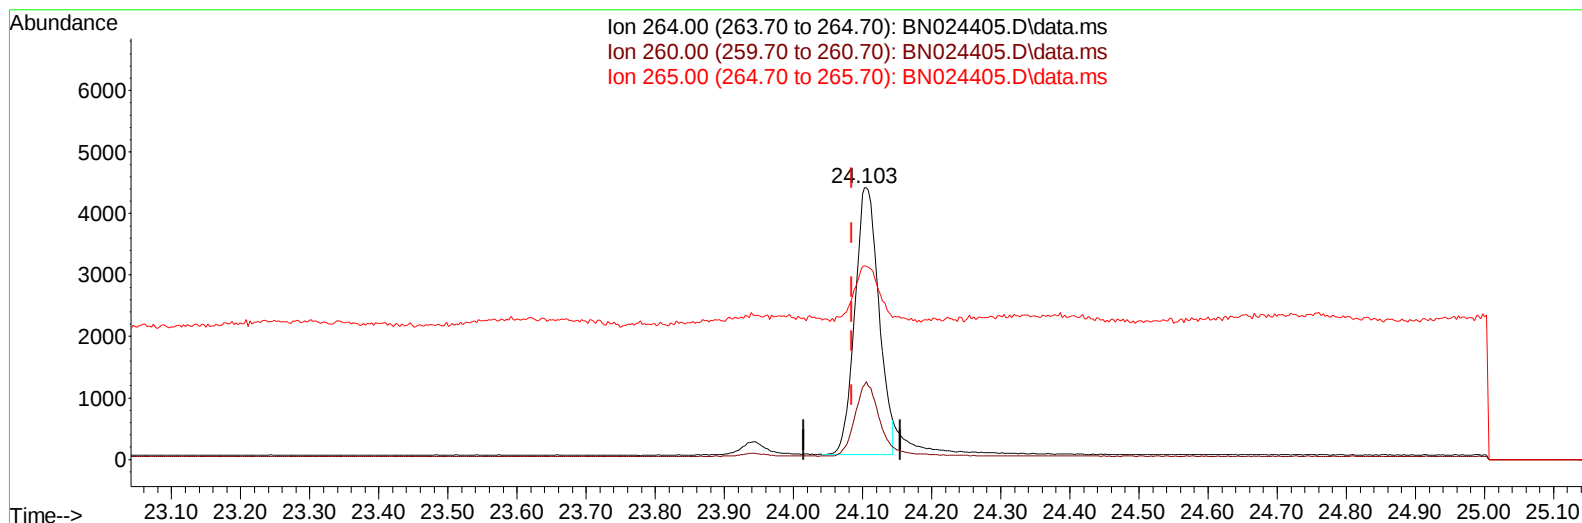

TIC: BN024405.D\data.ms

(23) Perylene-d12 (I)

24.103min (+ 0.018) 0.40 ng/ul

response 10476

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	27.48
265.00	38.30	71.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024405.D
Acq On : 20 Mar 2023 11:08
Operator : CG/JU
Sample : PB151451BS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLCS451

Manual IntegrationsAPPROVED

Quant Time: Mar 21 02:14:23 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:12:19 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/21/2023
Supervised By :Jagrut Upadhyay 03/21/2023

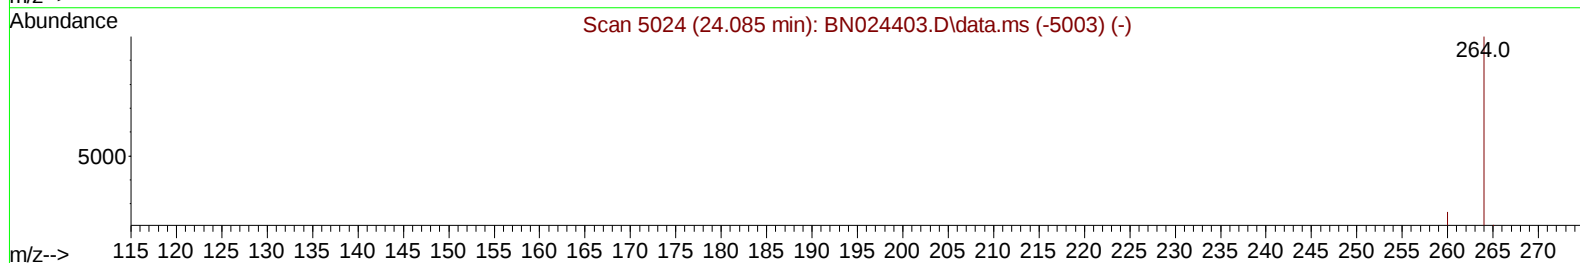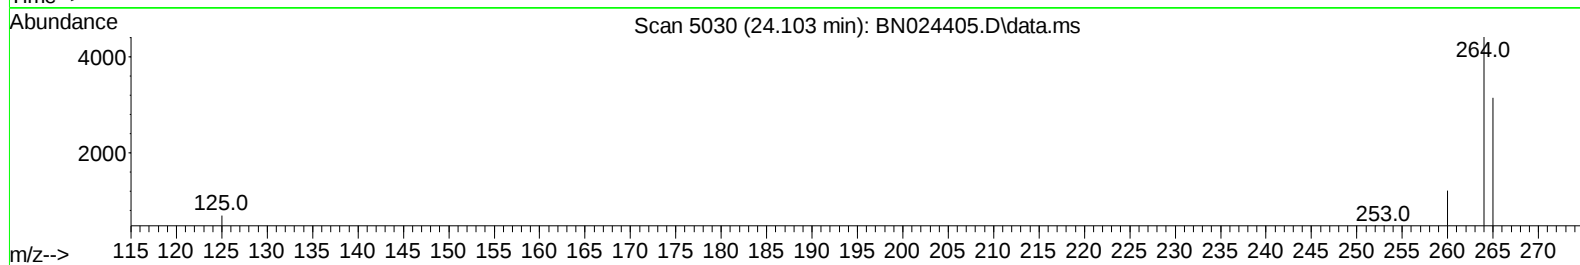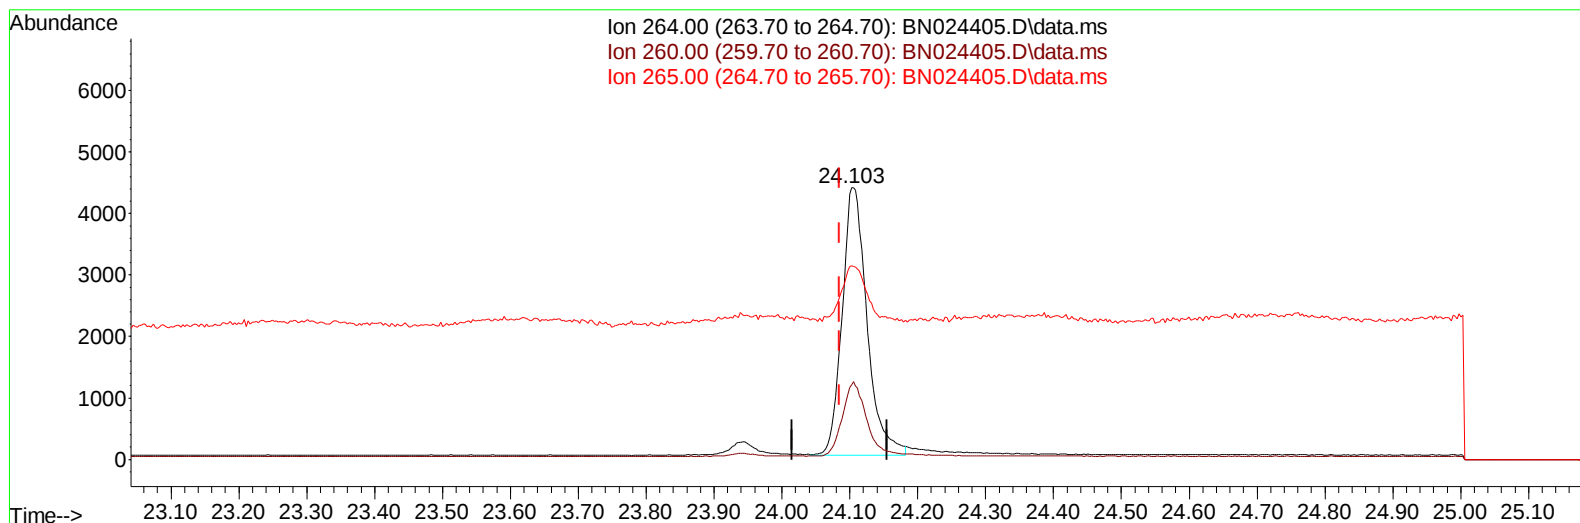

TIC: BN024405.D\data.ms

(23) Perylene-d12 (I)

24.103min (+ 0.018) 0.40 ng/ul m

response 11114

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	27.48
265.00	38.30	71.22#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024405.D
 Acq On : 20 Mar 2023 11:08
 Operator : CG/JU
 Sample : PB151451BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS451

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/21/2023
 Supervised By :Jagrut Upadhyay 03/21/2023

Quant Time: Mar 21 02:14:23 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:12:19 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.034	152		8679	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136		26909	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.670	164		12798	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188		25290	0.400	ng/ul	0.00
17) Chrysene-d12	21.600	240		15954	0.400	ng/ul	# 0.00
23) Perylene-d12	24.103	264		11114m	0.400	ng/ul	0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.397	96		5789	0.606	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152		9457	0.296	ng/ul	0.00
18) Fluoranthene-d10	19.436	212		15014	0.354	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.435	88		14957	1.440	ng/ul	90
5) Naphthalene	10.900	128		21257	0.316	ng/ul	100
7) 2-Methylnaphthalene	12.506	142		12249	0.301	ng/ul	98
8) 1-Methylnaphthalene	12.726	142		12780	0.298	ng/ul	99
10) Acenaphthylene	14.393	152		16487	0.309	ng/ul	99
11) Acenaphthene	14.731	153		12887	0.313	ng/ul	98
12) Fluorene	15.716	166		13907	0.303	ng/ul	97
14) Pentachlorophenol	17.059	266		3138	0.447	ng/ul#	73
15) Phenanthrene	17.456	178		22412	0.309	ng/ul	100
16) Anthracene	17.548	178		18487	0.291	ng/ul	99
19) Fluoranthene	19.469	202		22664	0.357	ng/ul	96
20) Pyrene	19.831	202		22320	0.346	ng/ul	95
21) Benzo(a)anthracene	21.586	228		15505	0.298	ng/ul	100
22) Chrysene	21.641	228		17674	0.321	ng/ul	100
24) Benzo(b)fluoranthene	23.334	252		14796	0.349	ng/ul	89
25) Benzo(k)fluoranthene	23.392	252		14913	0.339	ng/ul#	89
26) Benzo(a)pyrene	23.989	252		11601	0.318	ng/ul#	84
27) Indeno(1,2,3-cd)pyrene	26.723	276		12230	0.297	ng/ul#	100
28) Dibenzo(a,h)anthracene	26.750	278		8923	0.285	ng/ul	93
29) Benzo(g,h,i)perylene	27.532	276		11440	0.321	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024405.D
Acq On : 20 Mar 2023 11:08
Operator : CG/JU
Sample : PB151451BS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SLCS451

Manual IntegrationsAPPROVED

Quant Time: Mar 21 02:14:23 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:12:19 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/21/2023
Supervised By :Jagrut Upadhyay 03/21/2023

