

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024412.D
 Acq On : 20 Mar 2023 15:22
 Operator : CG/JU
 Sample : 01884-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB916

Quant Time: Mar 21 02:15:23 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:12:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	11400	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136	35988	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.670	164	21829	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.418	188	42897	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.595	240	32581	0.400	ng/ul	# 0.00
23) Perylene-d12	24.088	264	28839	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.397	96	50671	4.039	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	14280	0.334	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	29038	0.335	ng/ul	0.00
Target Compounds						
						Qvalue
10) Acenaphthylene	14.402	152	3037	0.033	ng/ul#	50
16) Anthracene	17.548	178	8619	0.080	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024412.D
Acq On : 20 Mar 2023 15:22
Operator : CG/JU
Sample : 01884-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB916


Quant Time: Mar 21 02:15:23 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:12:19 2023
Response via : Initial Calibration

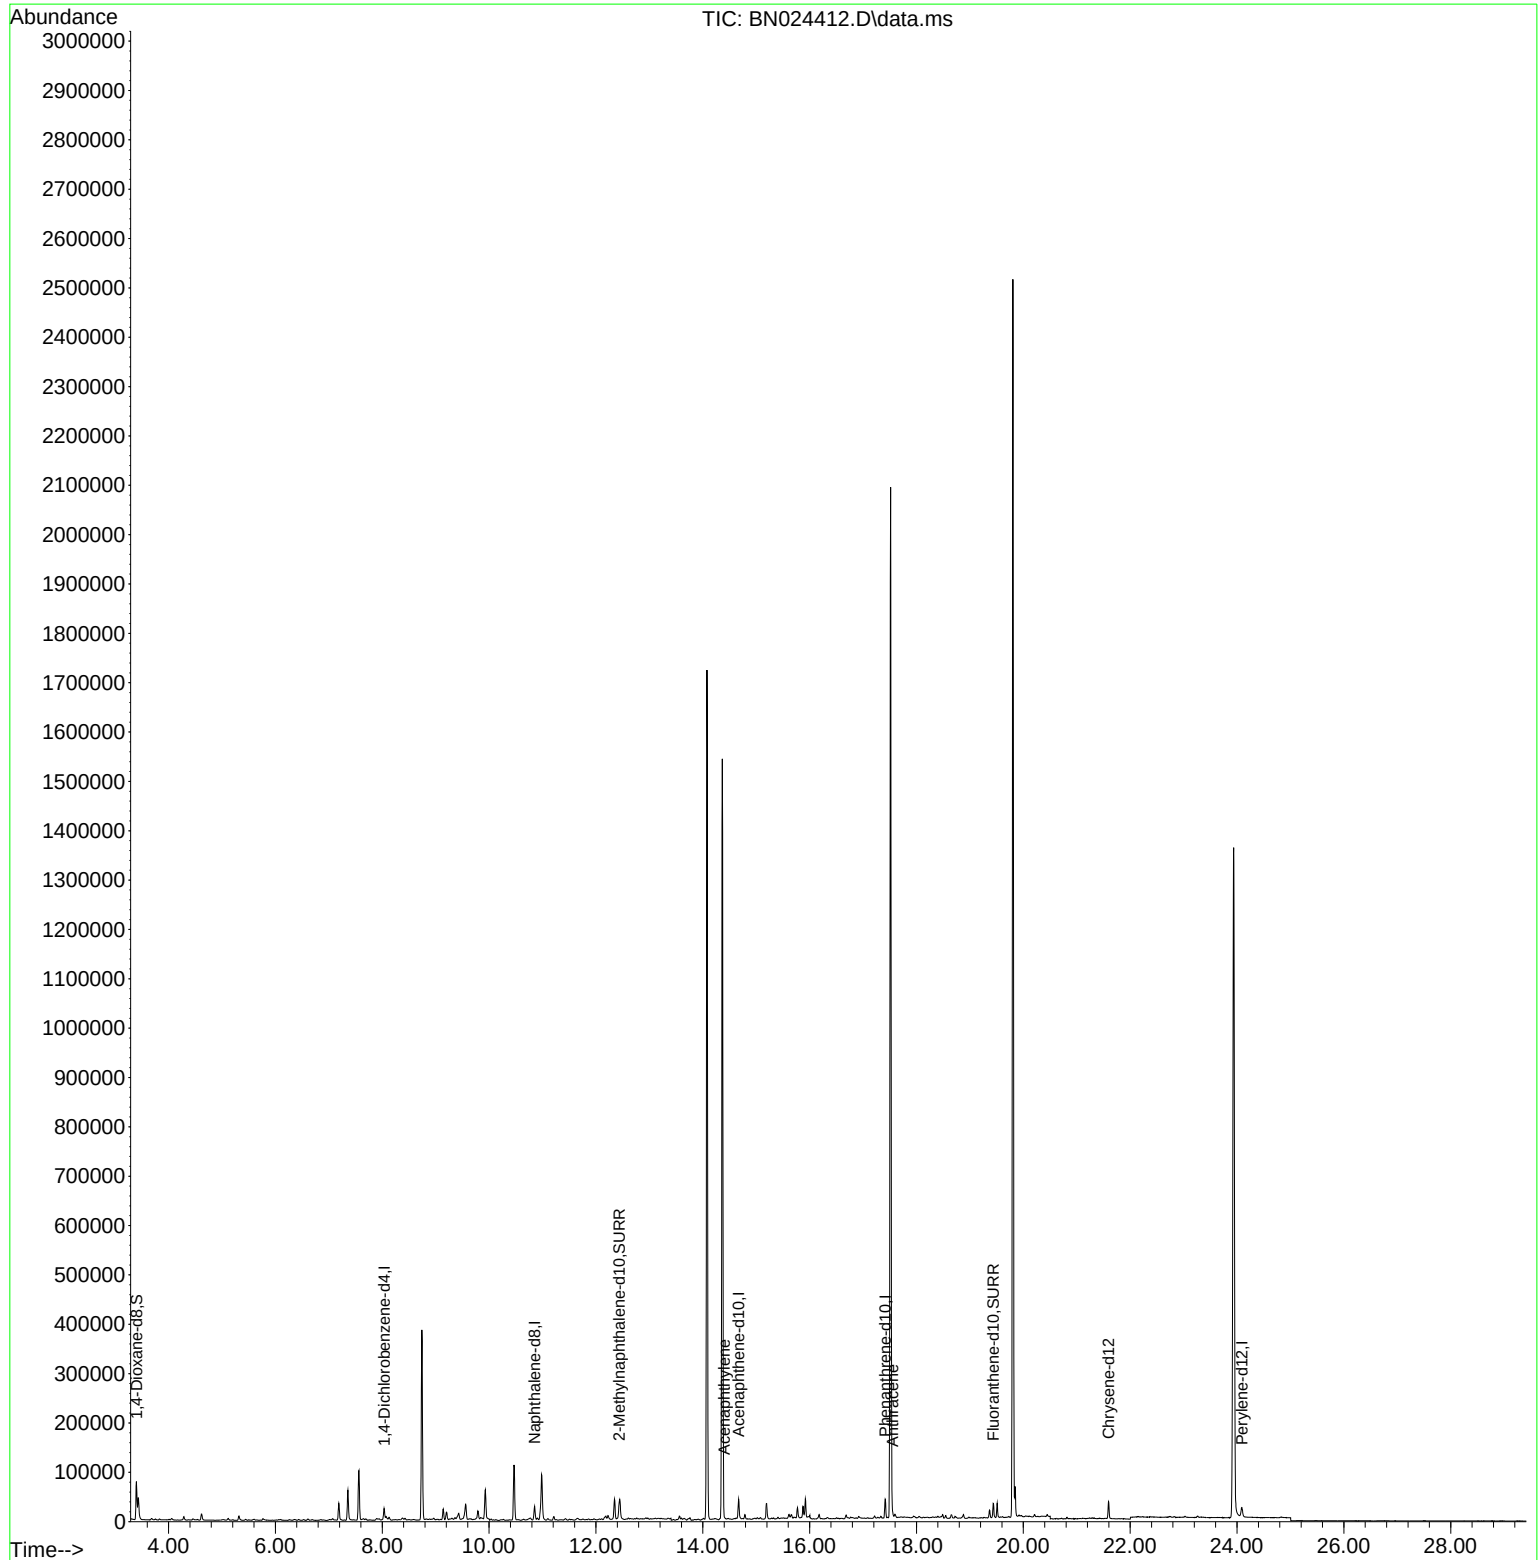



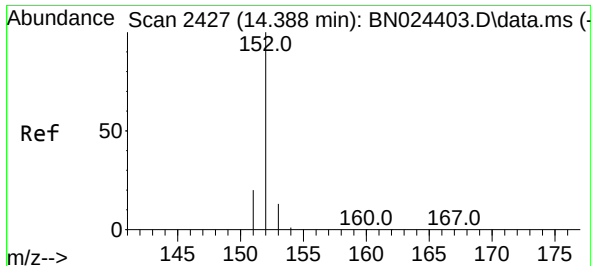


#10
Acenaphthylene
Concen: 0.033 ng/ul
RT: 14.402 min Scan# 2427
Delta R.T. 0.014 min
Lab File: BN024412.D
Acq: 20 Mar 2023 15:22

Instrument :
BNA_N
ClientSampleId :
CB916

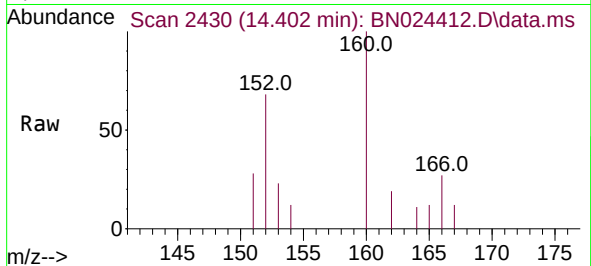

Tgt Ion:152 Resp: 3037
Ion Ratio Lower Upper
152 100
151 41.8 15.9 23.9#
153 34.5 10.6 16.0#

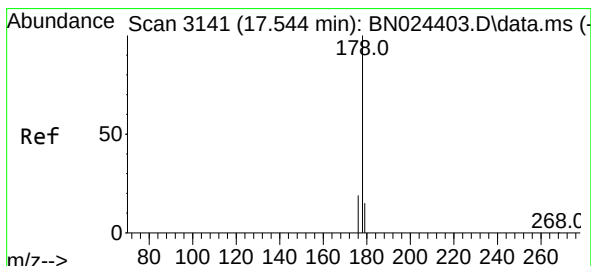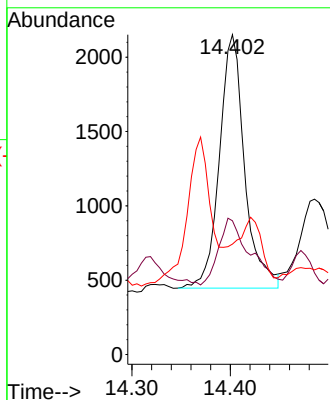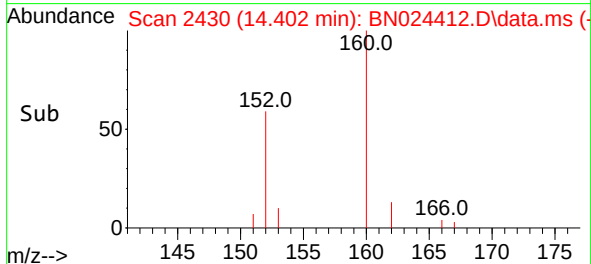

#16
Anthracene
Concen: 0.080 ng/ul
RT: 17.548 min Scan# 3142
Delta R.T. 0.004 min
Lab File: BN024412.D
Acq: 20 Mar 2023 15:22

Tgt Ion:178 Resp: 8619
Ion Ratio Lower Upper
178 100
179 33.0 12.3 18.5#
176 34.5 15.3 22.9#

