

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024414.D
 Acq On : 20 Mar 2023 16:35
 Operator : CG/JU
 Sample : 01884-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB919

Quant Time: Mar 21 02:15:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:12:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	13242	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136	41981	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.670	164	26539	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188	50450	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.600	240	38630	0.400	ng/ul	# 0.00
23) Perylene-d12	24.085	264	34524	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.397	96	51700	3.548	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	18450	0.370	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	38959	0.379	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.460	178	4410	0.031	ng/ul#	52
16) Anthracene	17.548	178	6286	0.050	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024414.D
Acq On : 20 Mar 2023 16:35
Operator : CG/JU
Sample : 01884-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB919

Quant Time: Mar 21 02:15:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:12:19 2023
Response via : Initial Calibration

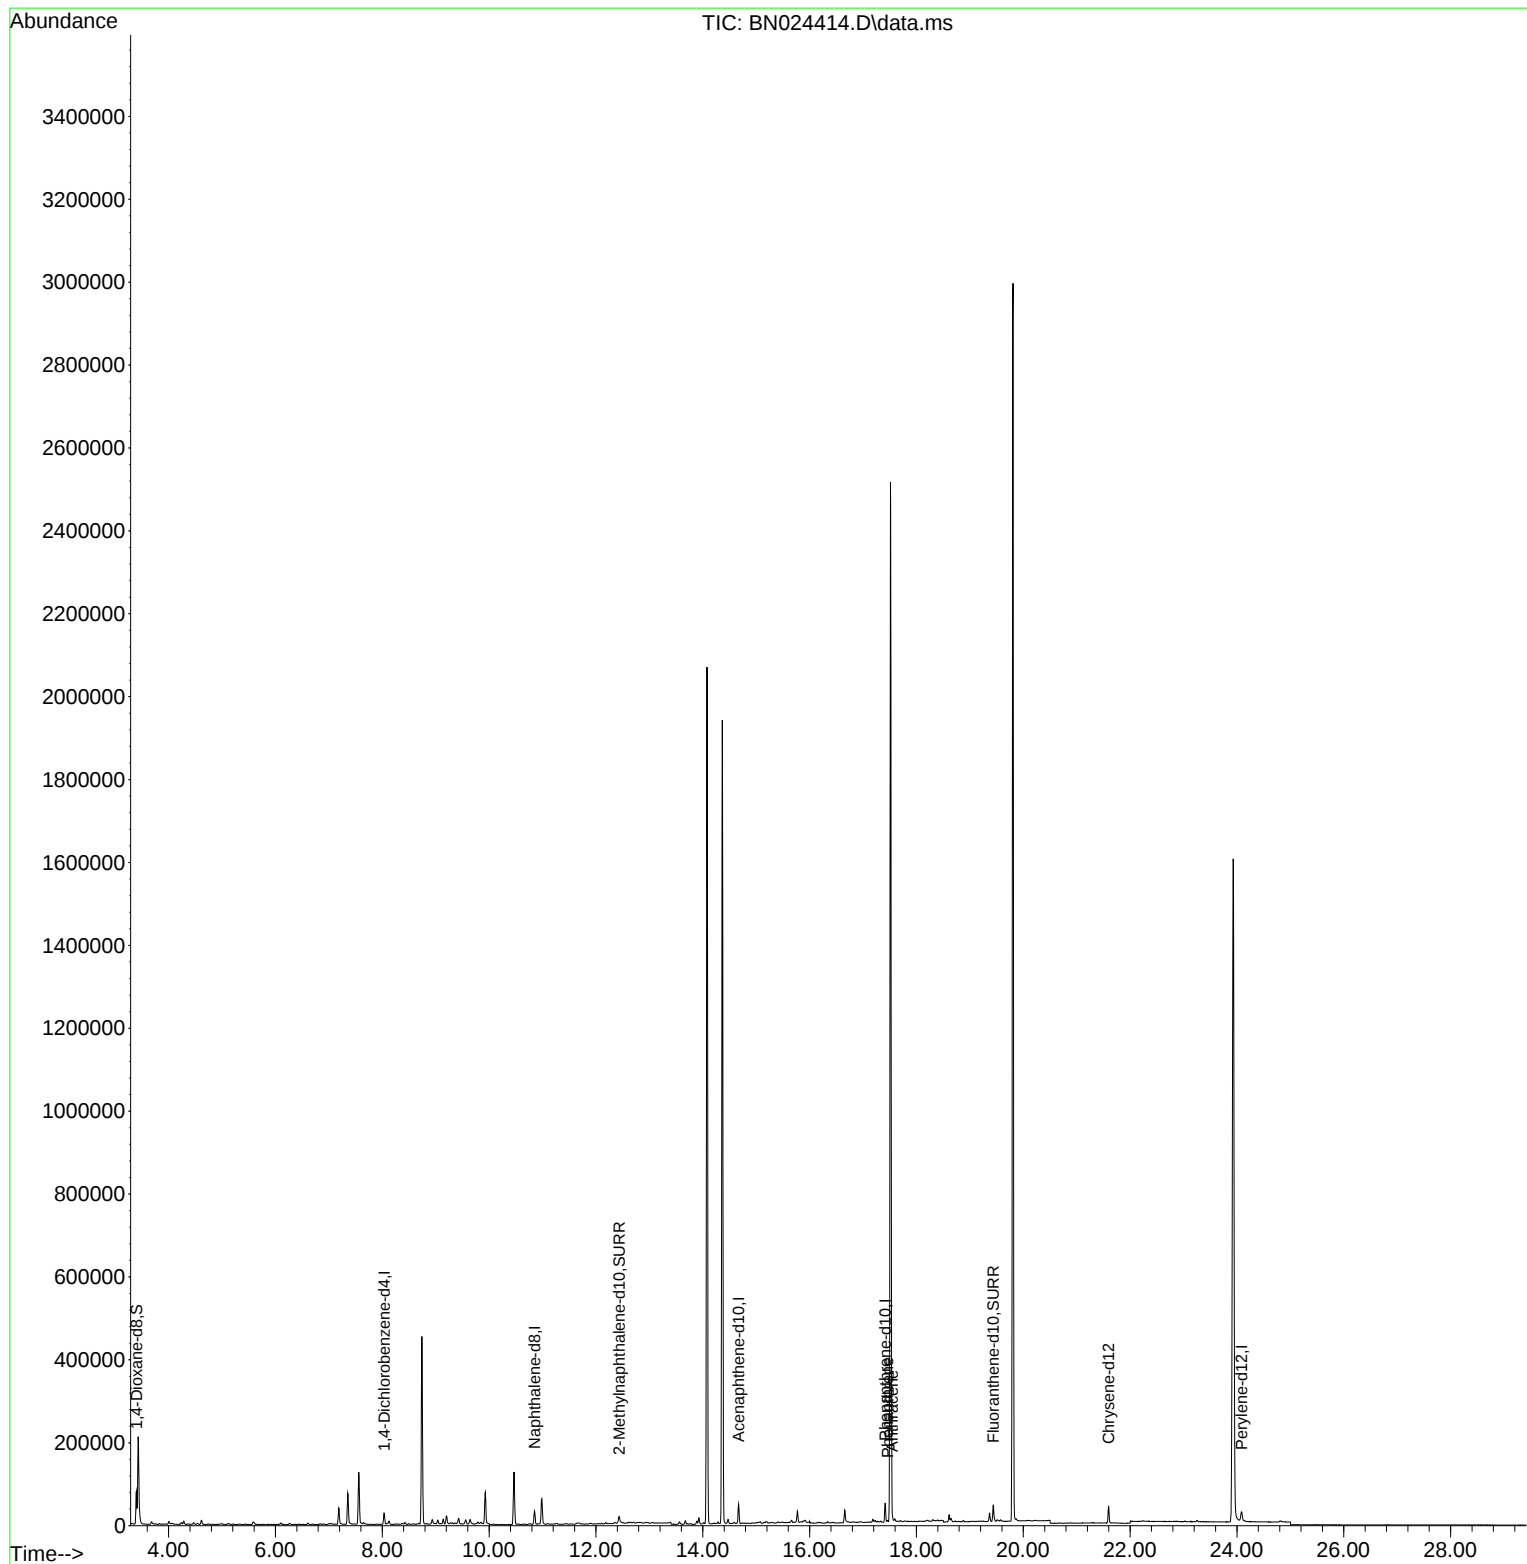

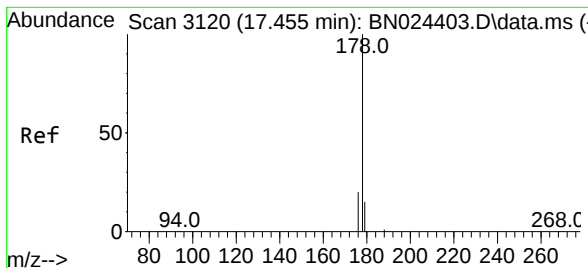

#15

Phenanthrene

Concen: 0.031 ng/ul

RT: 17.460 min Scan# 3121

Delta R.T. 0.004 min

Lab File: BN024414.D

Acq: 20 Mar 2023 16:35

Instrument :

BNA_N

ClientSampleId :

CB919





Tgt Ion:178 Resp: 4410

Ion Ratio Lower Upper

178 100

179 41.9 12.2 18.2#

176 35.8 15.7 23.5#

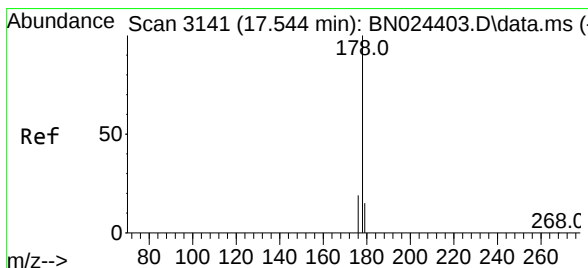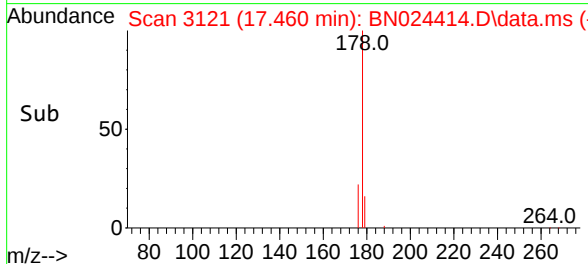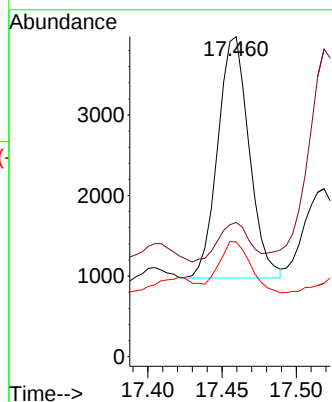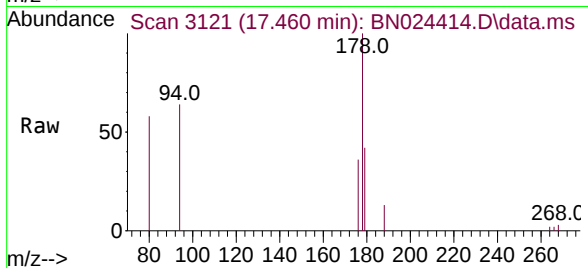

#16

Anthracene

Concen: 0.050 ng/ul

RT: 17.548 min Scan# 3142

Delta R.T. 0.004 min

Lab File: BN024414.D

Acq: 20 Mar 2023 16:35

Tgt Ion:178 Resp: 6286

Ion Ratio Lower Upper

178 100

179 38.0 12.3 18.5#

176 30.3 15.3 22.9#

