

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024415.D
 Acq On : 20 Mar 2023 17:12
 Operator : CG/JU
 Sample : 01884-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB921

Quant Time: Mar 21 02:15:44 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:12:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	9278	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136	29072	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.671	164	17055	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	35720	0.400	ng/ul	0.00
17) Chrysene-d12	21.600	240	29295	0.400	ng/ul	0.00
23) Perylene-d12	24.085	264	27647	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.397	96	43724	4.282	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	14084	0.408	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	31631	0.406	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.456	178	3043	0.030	ng/ul#	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024415.D
Acq On : 20 Mar 2023 17:12
Operator : CG/JU
Sample : 01884-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB921


Quant Time: Mar 21 02:15:44 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:12:19 2023
Response via : Initial Calibration

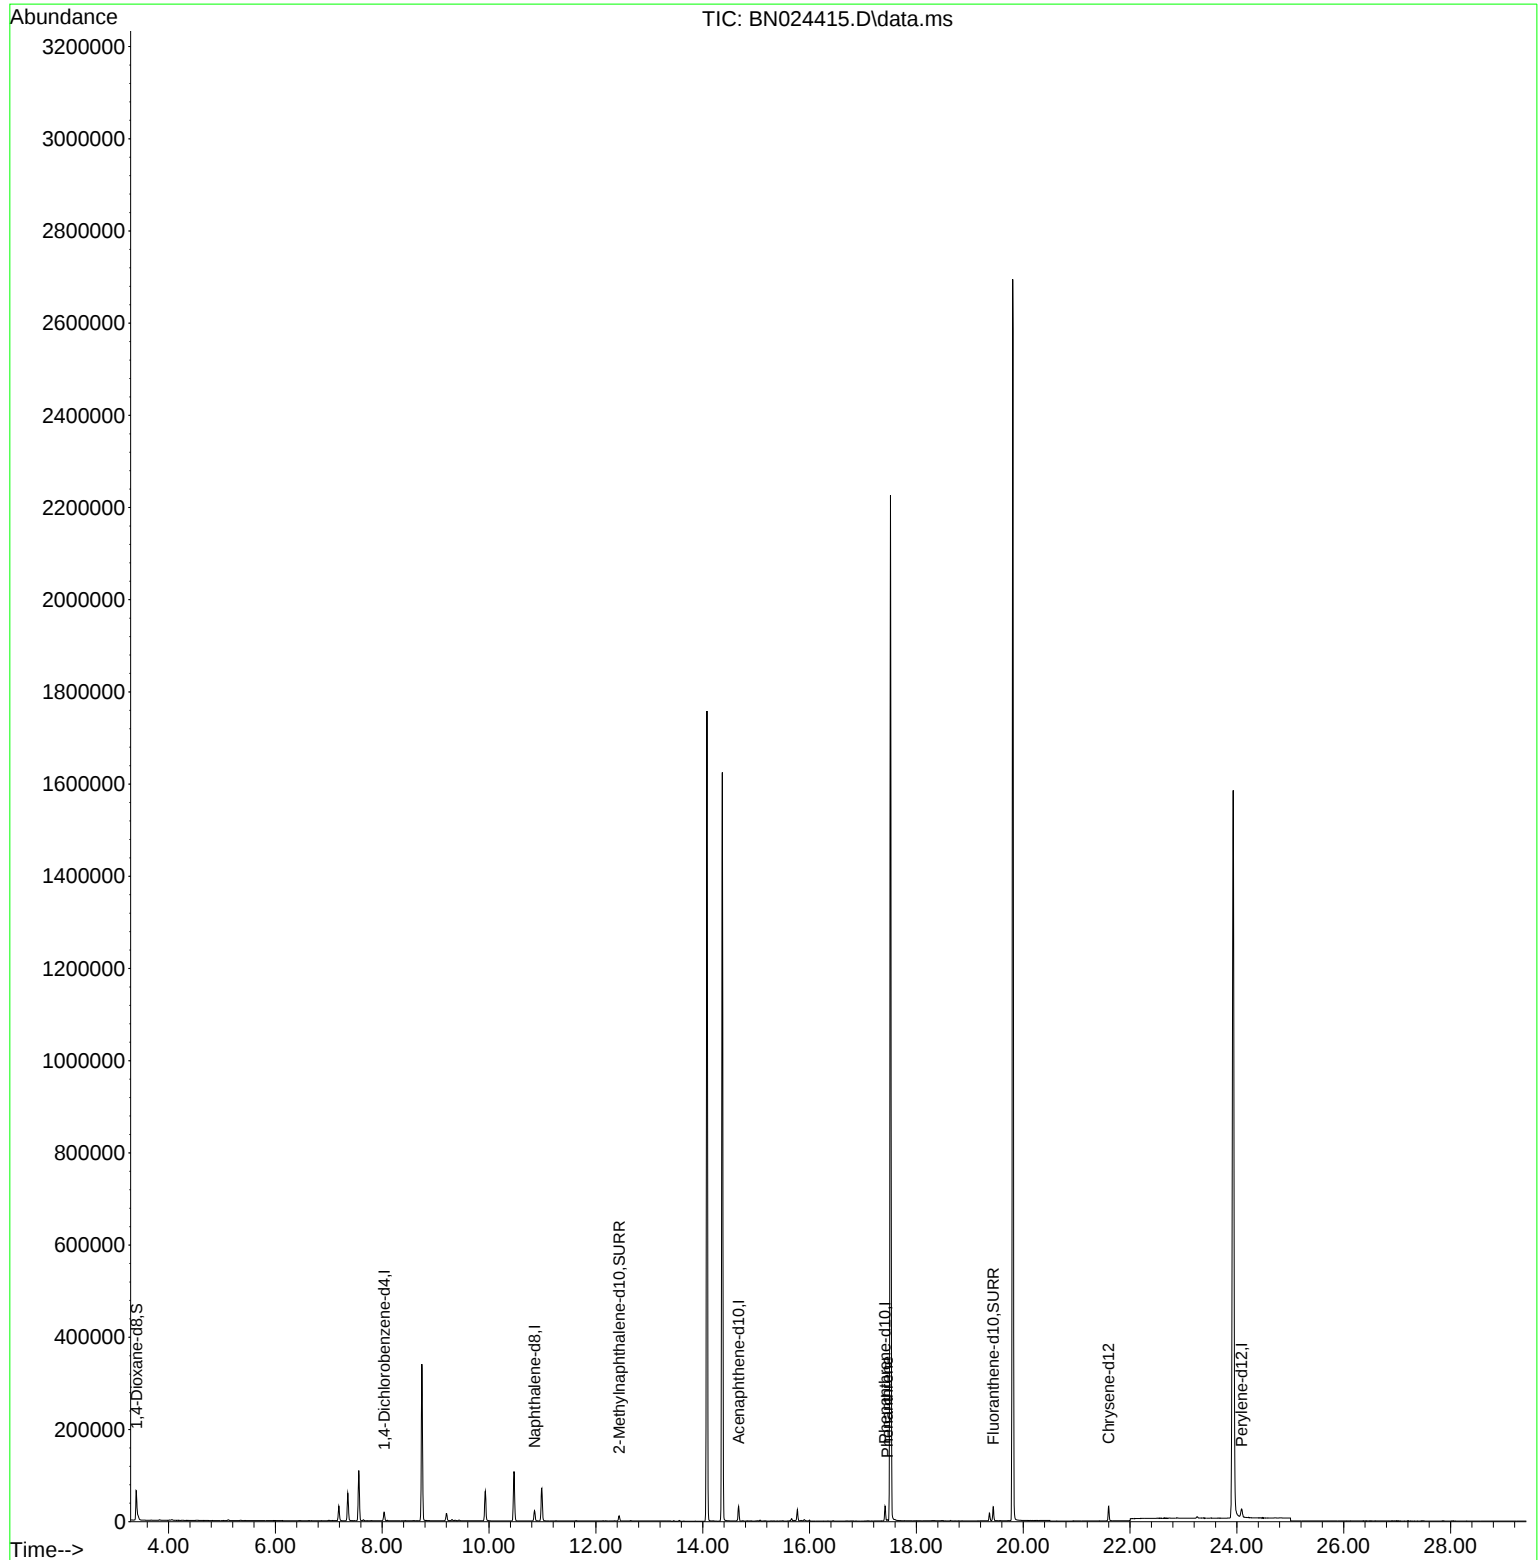

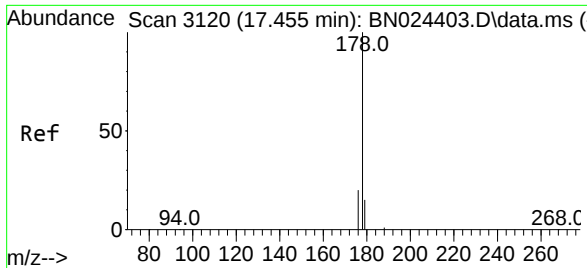

#15
 Phenanthrene
 Concen: 0.030 ng/ul
 RT: 17.456 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BN024415.D
 Acq: 20 Mar 2023 17:12

Instrument :
 BNA_N
 ClientSampleId :
 CB921

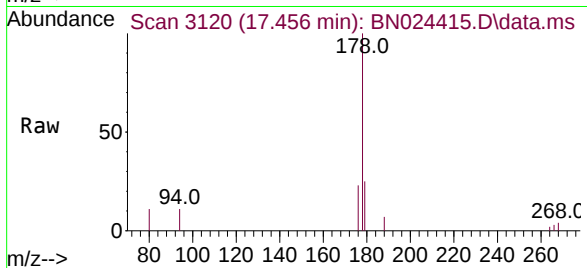

Tgt Ion	Ratio	Lower	Upper
178	100		
179	24.9	12.2	18.2#
176	23.2	15.7	23.5

