

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024427.D
 Acq On : 21 Mar 2023 01:09
 Operator : CG/JU
 Sample : 01885-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB921

Quant Time: Mar 21 02:45:20 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:42:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	13910	0.400	ng/ul	0.00
4) Naphthalene-d8	10.850	136	43209	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.670	164	25159	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	52060	0.400	ng/ul	0.00
17) Chrysene-d12	21.594	240	38922	0.400	ng/ul	0.00
23) Perylene-d12	24.100	264	33661	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.397	96	59267	3.872	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	18475	0.360	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	39471	0.381	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.435	88	3326	0.200	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024427.D
Acq On : 21 Mar 2023 01:09
Operator : CG/JU
Sample : 01885-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB921

Quant Time: Mar 21 02:45:20 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:42:36 2023
Response via : Initial Calibration

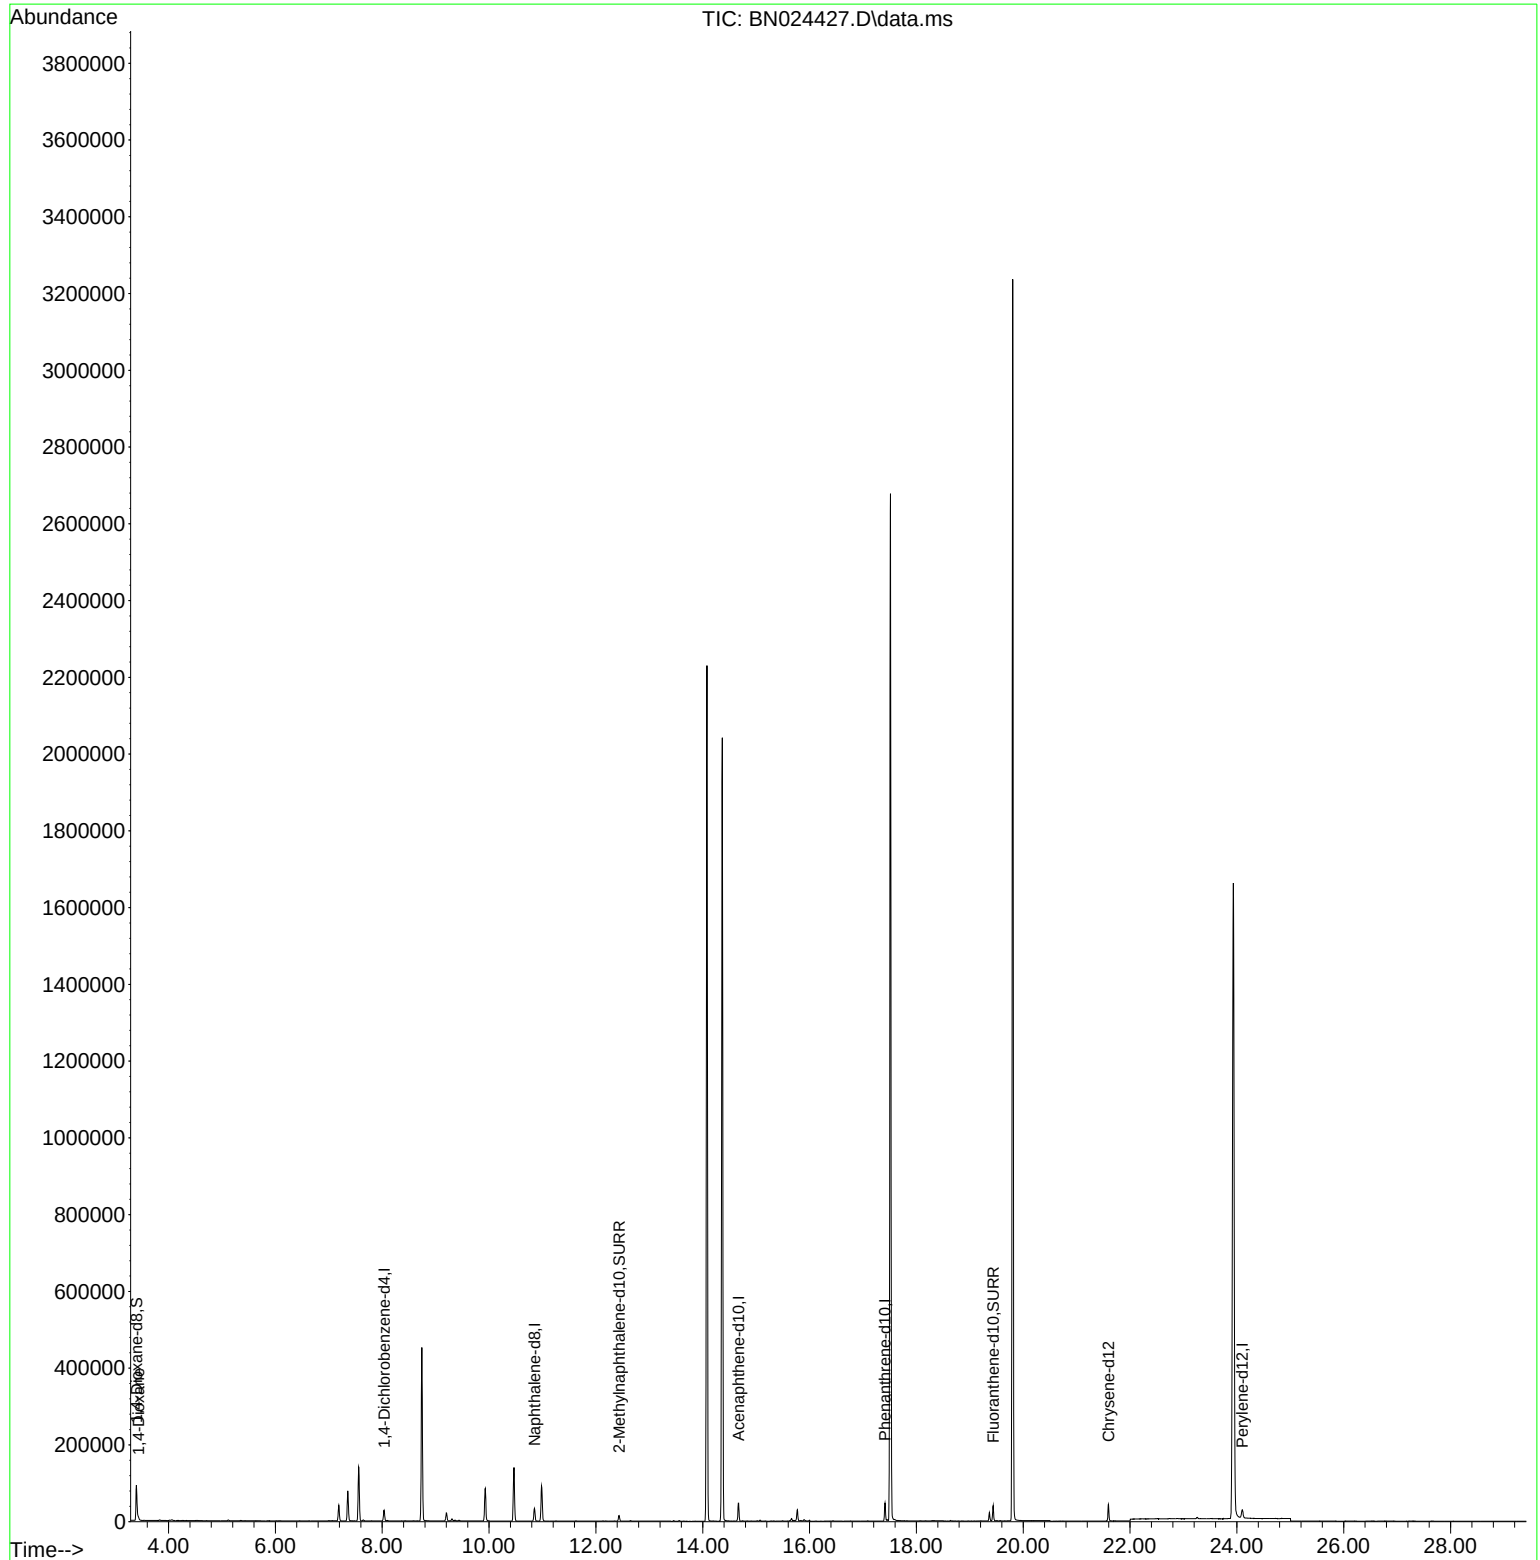

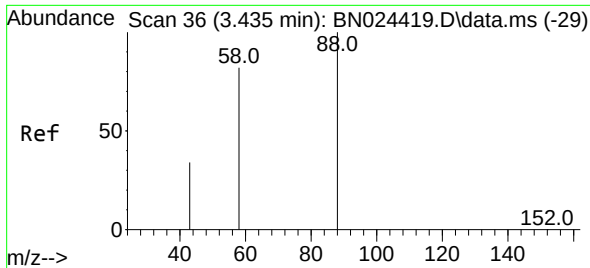

#2
 1,4-Dioxane
 Concen: 0.200 ng/ul
 RT: 3.435 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: BN024427.D
 Acq: 21 Mar 2023 01:09

Instrument :
 BNA_N
 ClientSampleId :
 CB921

Tgt Ion:	88	Resp:	3326
Ion	Ratio	Lower	Upper
88	100		
43	57.9	32.1	48.1#
58	68.6	55.1	82.7

