

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024429.D
 Acq On : 21 Mar 2023 02:22
 Operator : CG/JU
 Sample : 01996-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0A24

Quant Time: Mar 21 02:55:03 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:42:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	12895	0.400	ng/u1	0.00
4) Naphthalene-d8	10.850	136	39906	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.670	164	22927	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.413	188	46876	0.400	ng/u1	0.00
17) Chrysene-d12	21.600	240	34893	0.400	ng/u1	0.00
23) Perylene-d12	24.085	264	31902	0.400	ng/u1	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.397	96	54368	3.831	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.429	152	13941	0.294	ng/u1	0.00
18) Fluoranthene-d10	19.436	212	31495	0.339	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.431	88	108487	7.028	ng/u1	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\  
Data File : BN024429.D  
Acq On    : 21 Mar 2023   02:22  
Operator  : CG/JU  
Sample    : 01996-01  
Misc      :  
ALS Vial  : 28    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
H0A24


Quant Time: Mar 21 02:55:03 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Tue Mar 21 02:42:36 2023
Response via : Initial Calibration

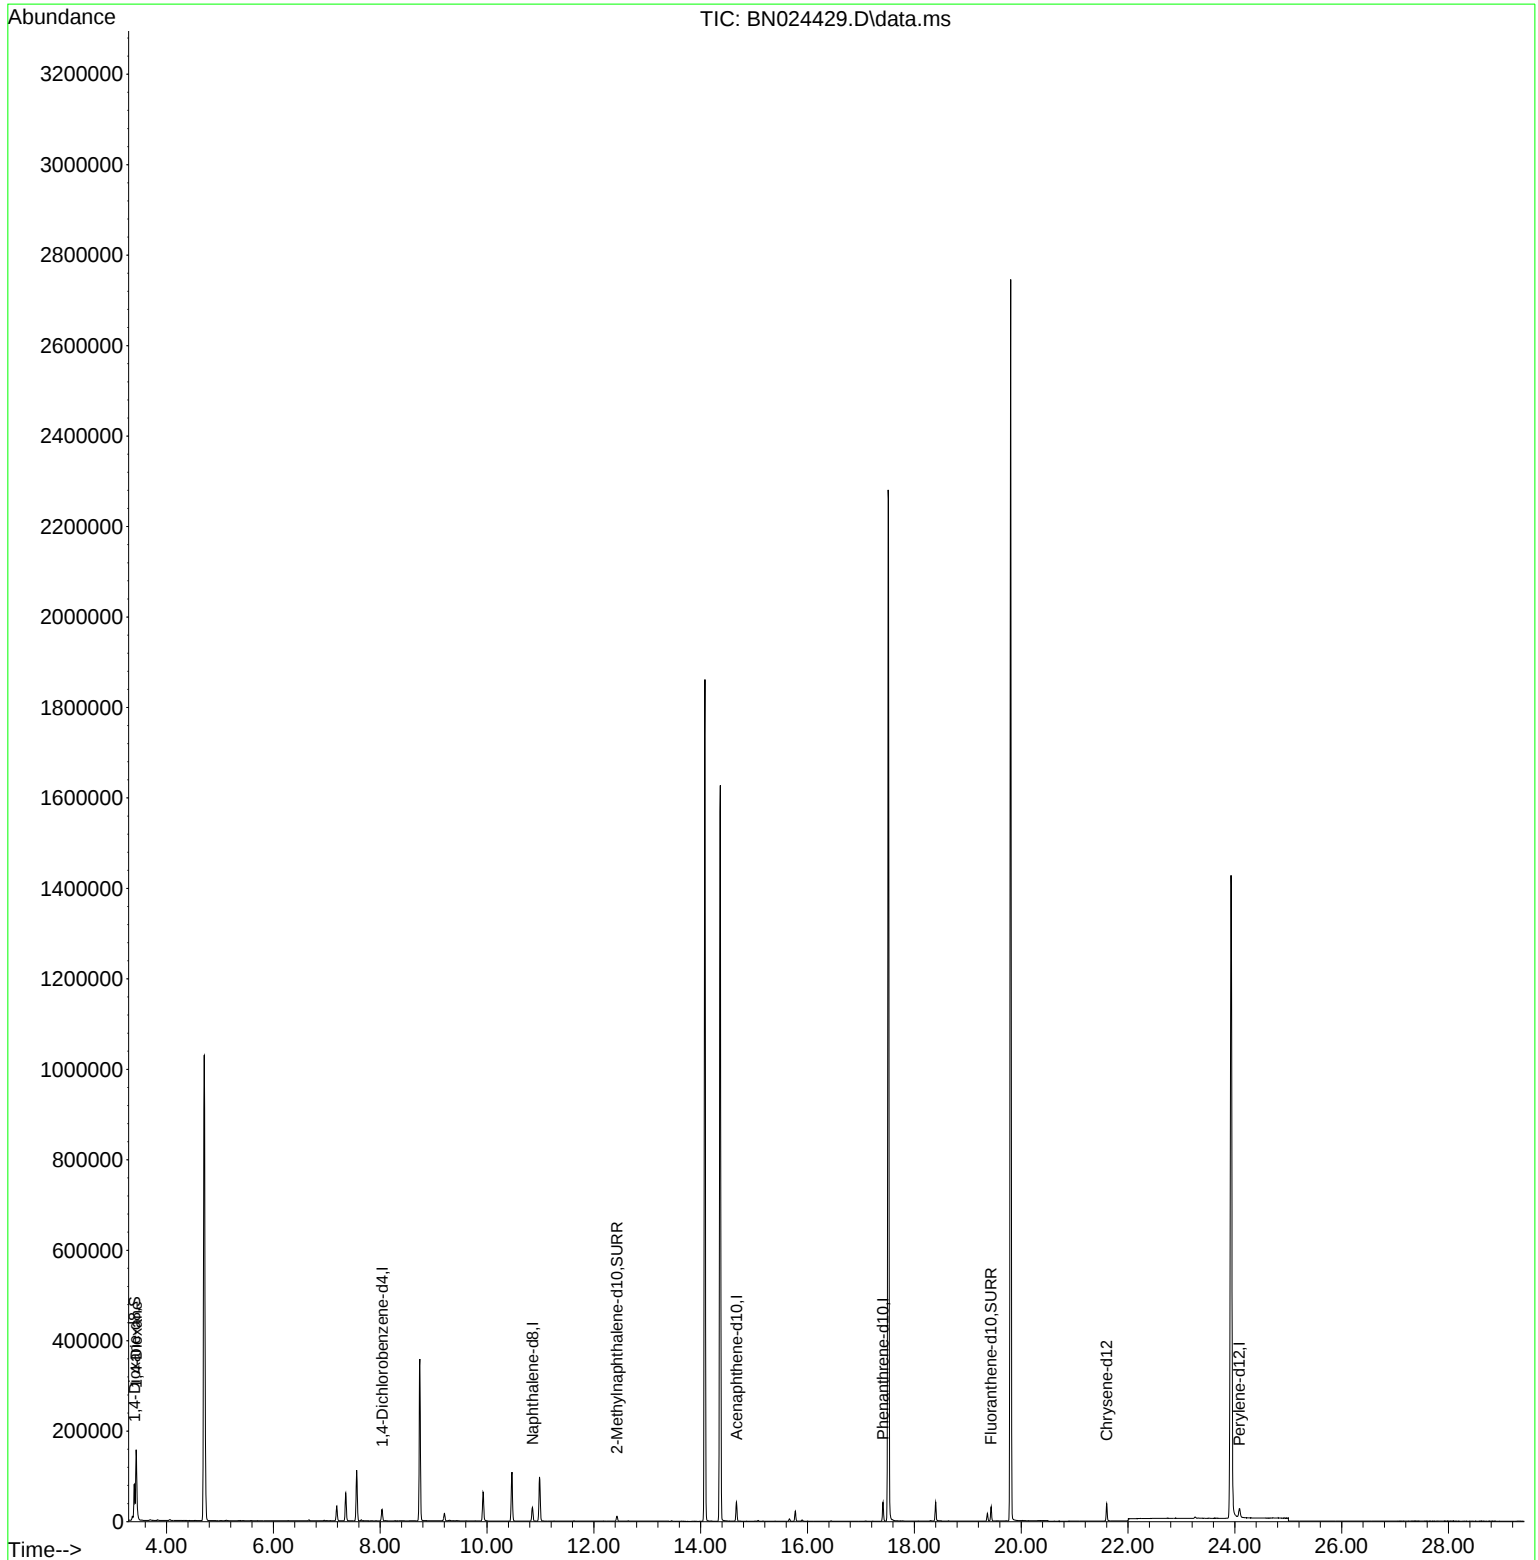

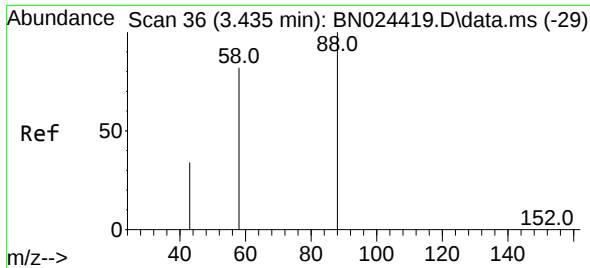

#2
 1,4-Dioxane
 Concen: 7.028 ng/ul
 RT: 3.431 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN024429.D
 Acq: 21 Mar 2023 02:22

Instrument :
 BNA_N
 ClientSampleId :
 H0A24

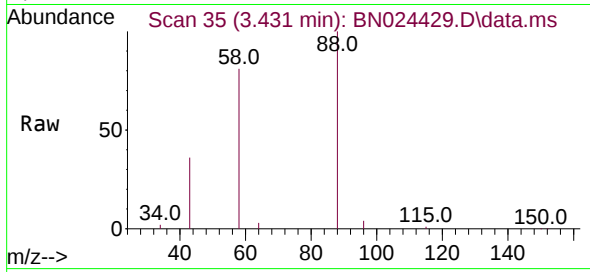

Tgt Ion: 88 Resp: 108487

Ion	Ratio	Lower	Upper
88	100		
43	35.8	32.1	48.1
58	81.3	55.1	82.7

