

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024435.D
 Acq On : 21 Mar 2023 06:00
 Operator : CG/JU
 Sample : 01996-05
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0A26

Quant Time: Mar 21 06:32:44 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:42:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	12355	0.400	ng/u1	0.00
4) Naphthalene-d8	10.850	136	38397	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.666	164	22125	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.413	188	44319	0.400	ng/u1	0.00
17) Chrysene-d12	21.600	240	33203	0.400	ng/u1	0.00
23) Perylene-d12	24.106	264	29666	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	75224	5.533	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.429	152	17267	0.378	ng/u1	0.00
18) Fluoranthene-d10	19.436	212	40101	0.454	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.431	88	1213575	82.056	ng/u1	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024435.D
Acq On : 21 Mar 2023 06:00
Operator : CG/JU
Sample : 01996-05
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0A26


Quant Time: Mar 21 06:32:44 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:42:36 2023
Response via : Initial Calibration

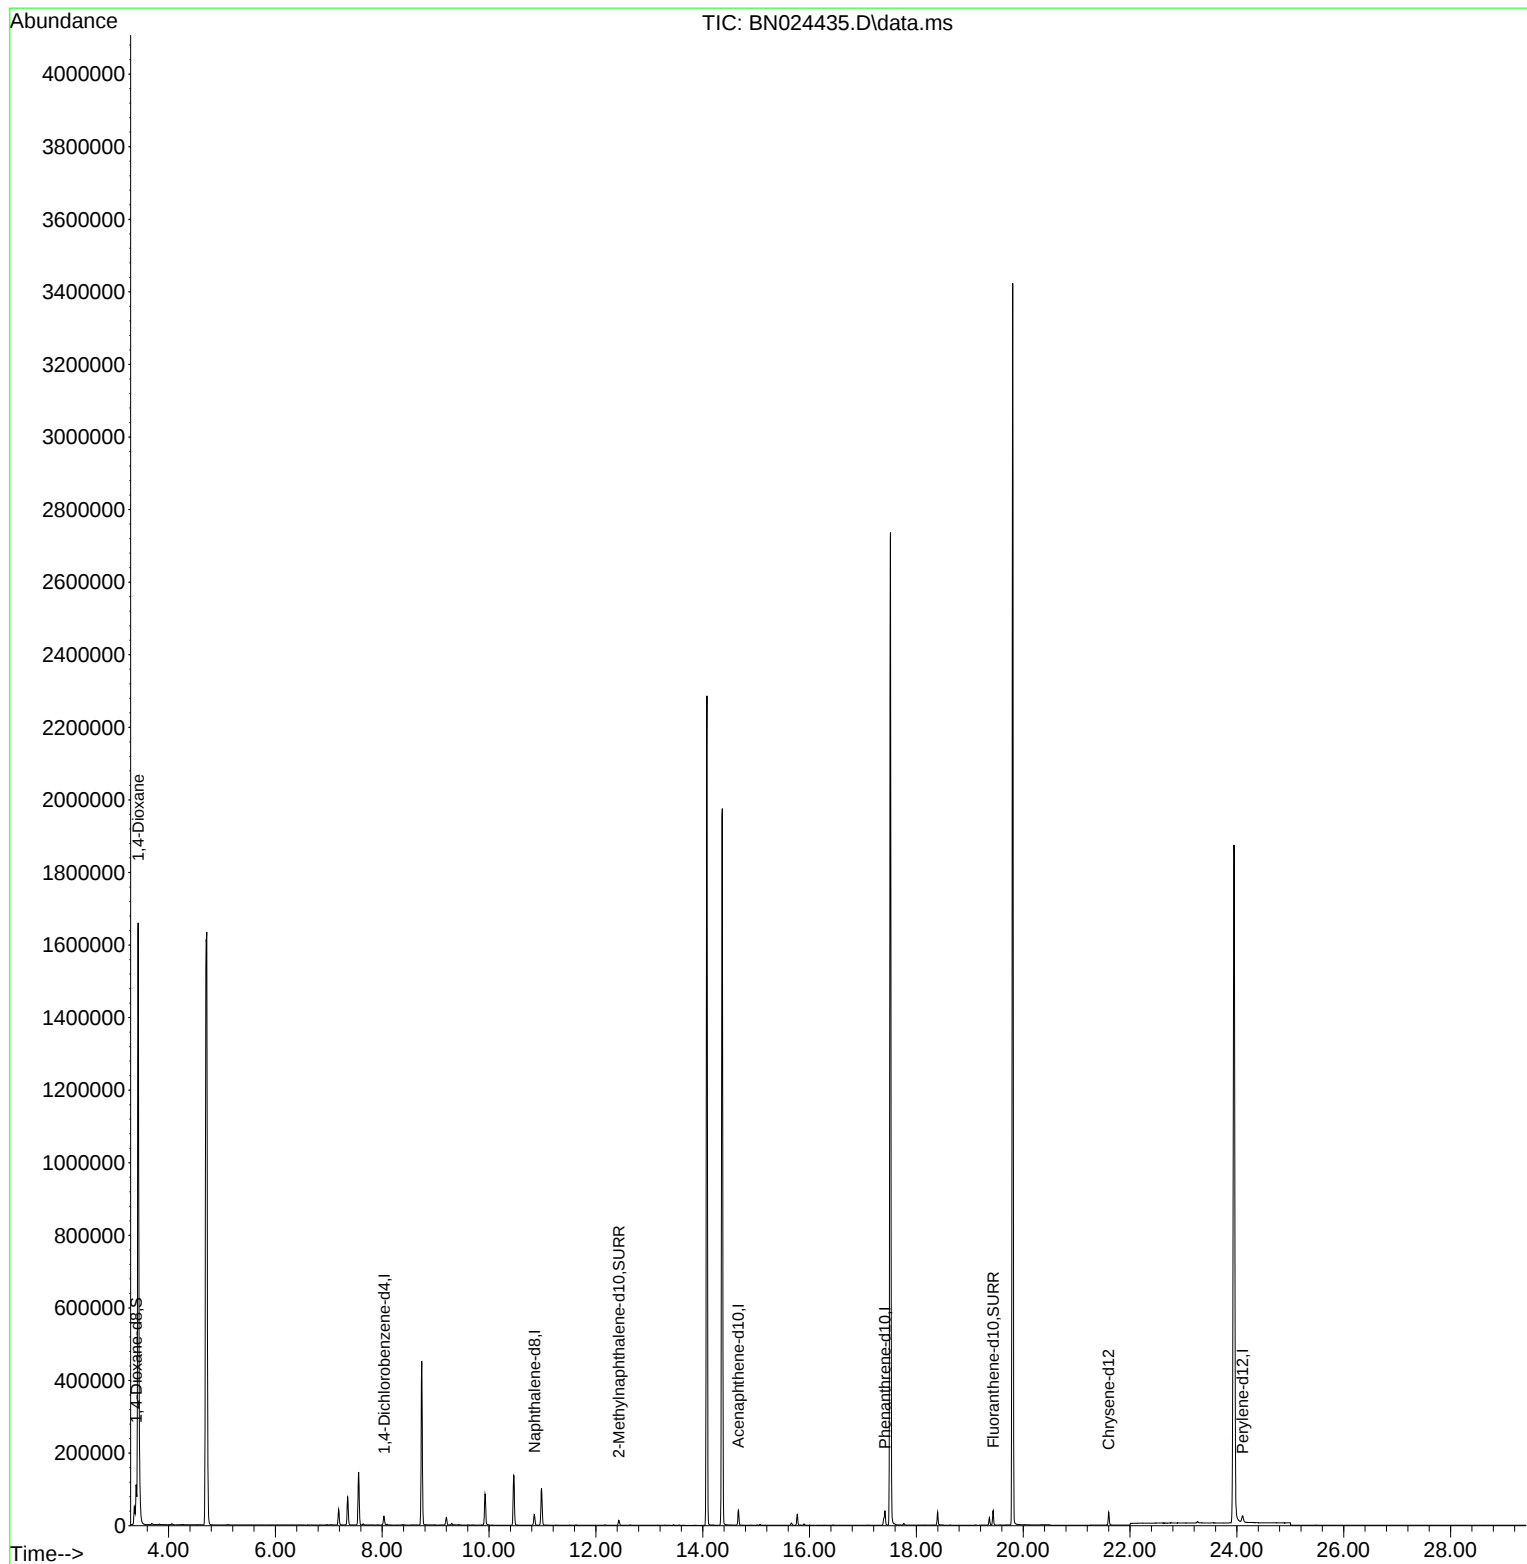

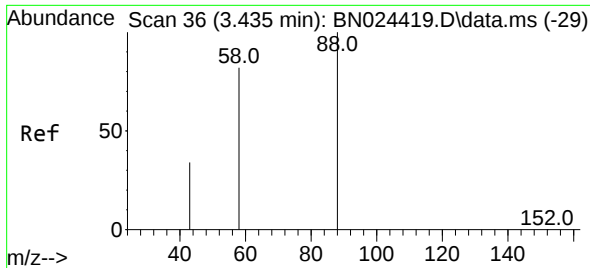

#2
 1,4-Dioxane
 Concen: 82.056 ng/ul
 RT: 3.431 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN024435.D
 Acq: 21 Mar 2023 06:00

Instrument :
 BNA_N
 ClientSampleId :
 H0A26

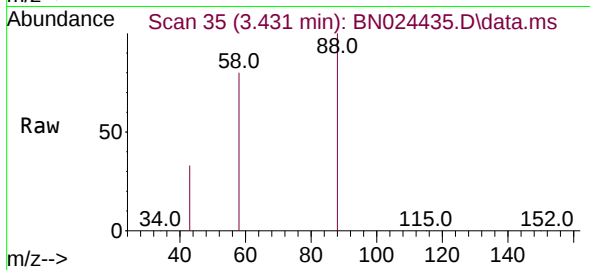

Tgt Ion: 88 Resp: 1213575

Ion	Ratio	Lower	Upper
88	100		
43	33.4	32.1	48.1
58	79.9	55.1	82.7

