

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024440.D
 Acq On : 21 Mar 2023 09:38
 Operator : CG/JU
 Sample : 01996-07
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0A28

Quant Time: Mar 21 17:37:45 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:42:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.030	152	9653	0.400	ng/ul	0.00
4) Naphthalene-d8	10.845	136	29595	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.666	164	16752	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.413	188	35237	0.400	ng/ul	0.00
17) Chrysene-d12	21.600	240	29218	0.400	ng/ul	0.00
23) Perylene-d12	24.106	264	28232	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	53883	5.072	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.429	152	11688	0.332	ng/ul	0.00
18) Fluoranthene-d10	19.436	212	28497	0.367	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.427	88	842927	72.948	ng/ul	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024440.D
Acq On : 21 Mar 2023 09:38
Operator : CG/JU
Sample : 01996-07
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0A28


Quant Time: Mar 21 17:37:45 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:42:36 2023
Response via : Initial Calibration

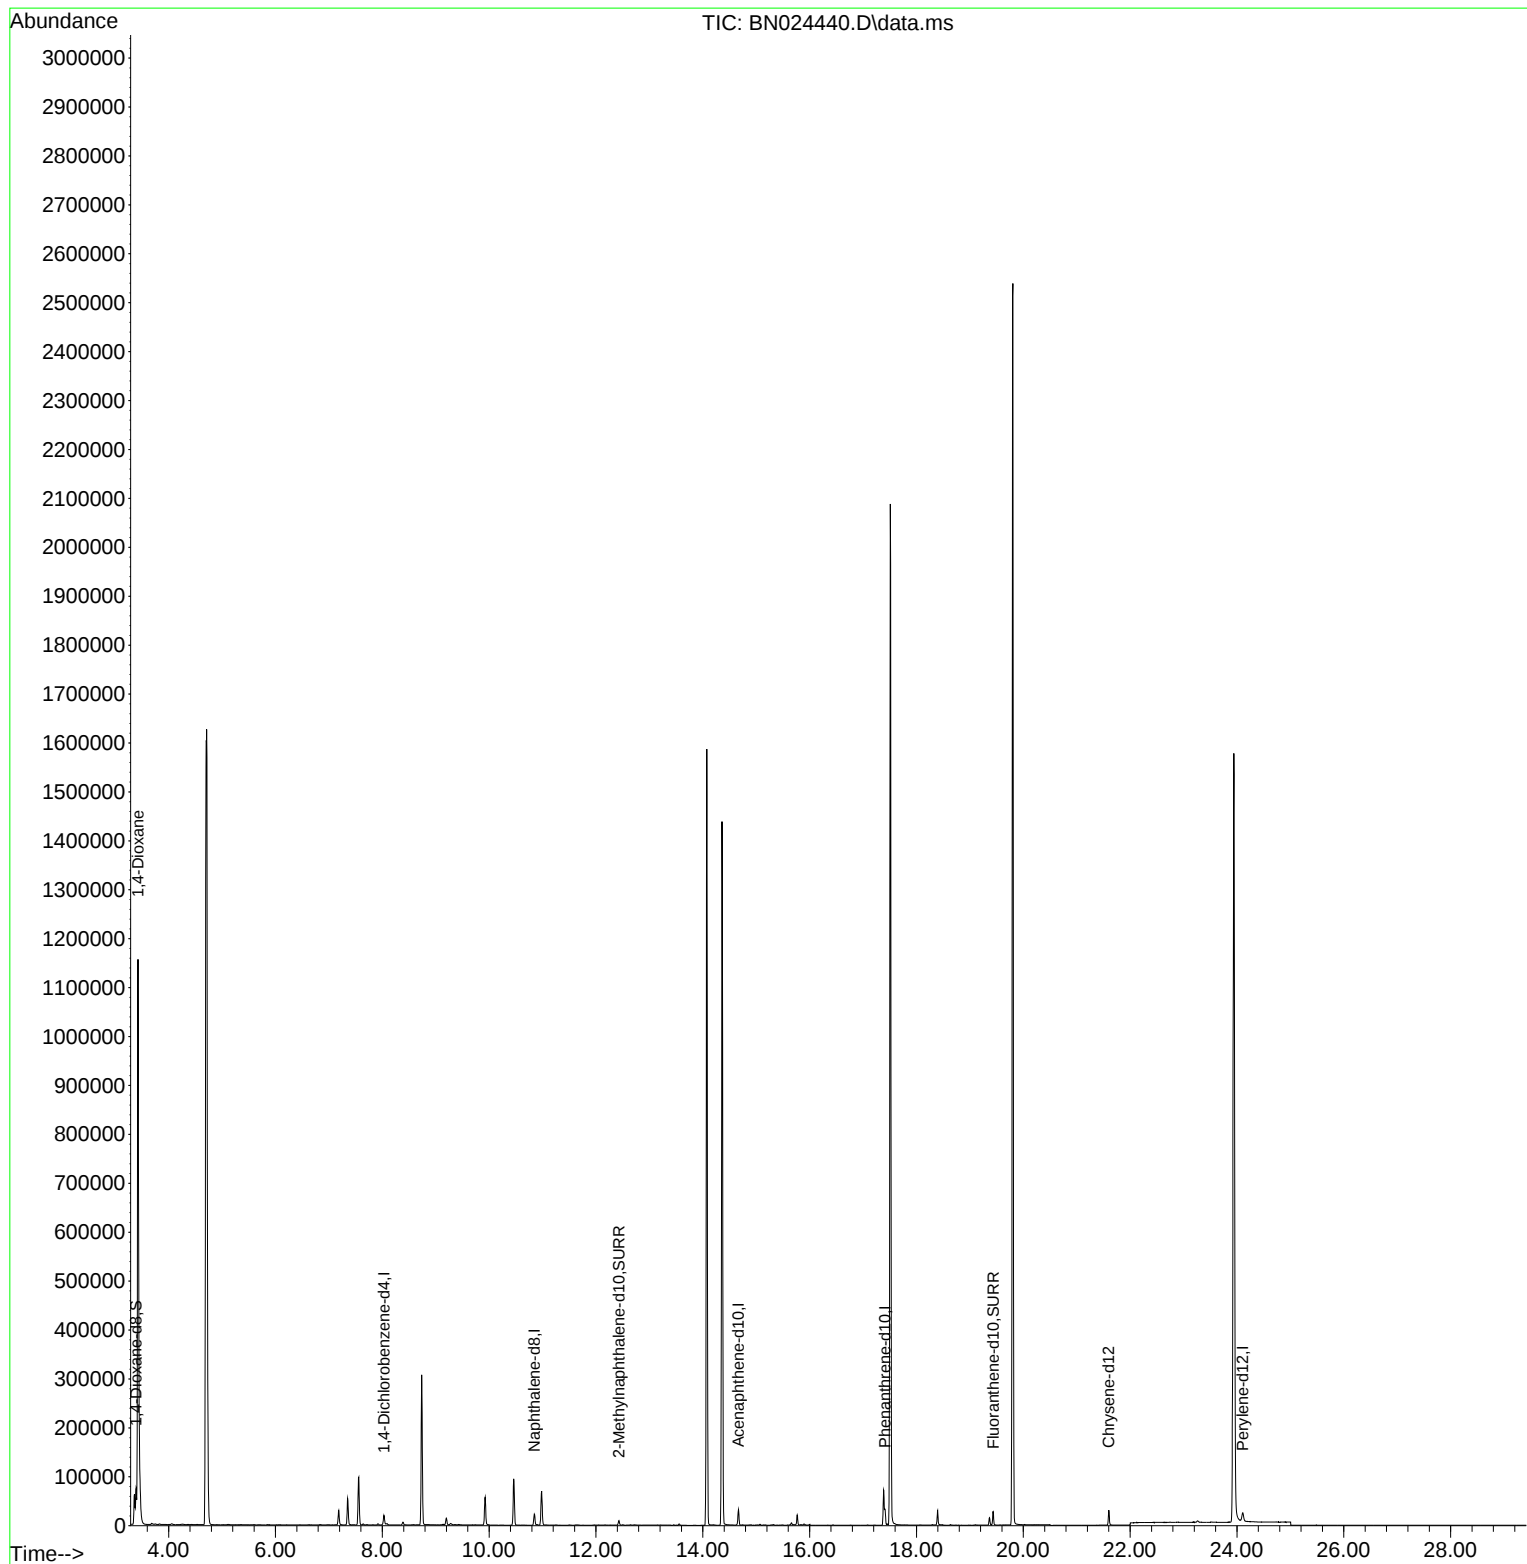

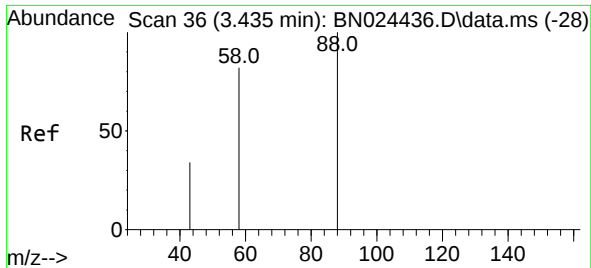

#2
 1,4-Dioxane
 Concen: 72.948 ng/ul
 RT: 3.427 min Scan# 34
 Delta R.T. -0.008 min
 Lab File: BN024440.D
 Acq: 21 Mar 2023 09:38

Instrument :
 BNA_N
 ClientSampleId :
 H0A28

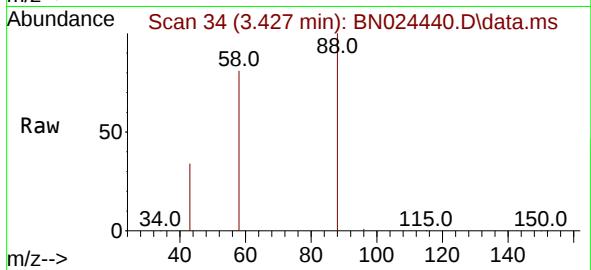

Tgt Ion: 88 Resp: 842927

Ion	Ratio	Lower	Upper
88	100		
43	34.0	32.1	48.1
58	80.7	55.1	82.7

