

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
 Data File : BN024441.D
 Acq On : 21 Mar 2023 10:14
 Operator : CG/JU
 Sample : 01996-08
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0A29

Quant Time: Mar 21 17:37:50 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 21 02:42:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.030	152	11734	0.400	ng/u1	0.00
4) Naphthalene-d8	10.845	136	36220	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.666	164	20450	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.409	188	41942	0.400	ng/u1	0.00
17) Chrysene-d12	21.597	240	35032	0.400	ng/u1	0.00
23) Perylene-d12	24.094	264	34820	0.400	ng/u1	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	81386	6.303	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.429	152	15907	0.370	ng/u1	0.00
18) Fluoranthene-d10	19.436	212	35214	0.378	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.431	88	623660	44.400	ng/u1	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032023\
Data File : BN024441.D
Acq On : 21 Mar 2023 10:14
Operator : CG/JU
Sample : 01996-08
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0A29

Quant Time: Mar 21 17:37:50 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN030923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 21 02:42:36 2023
Response via : Initial Calibration

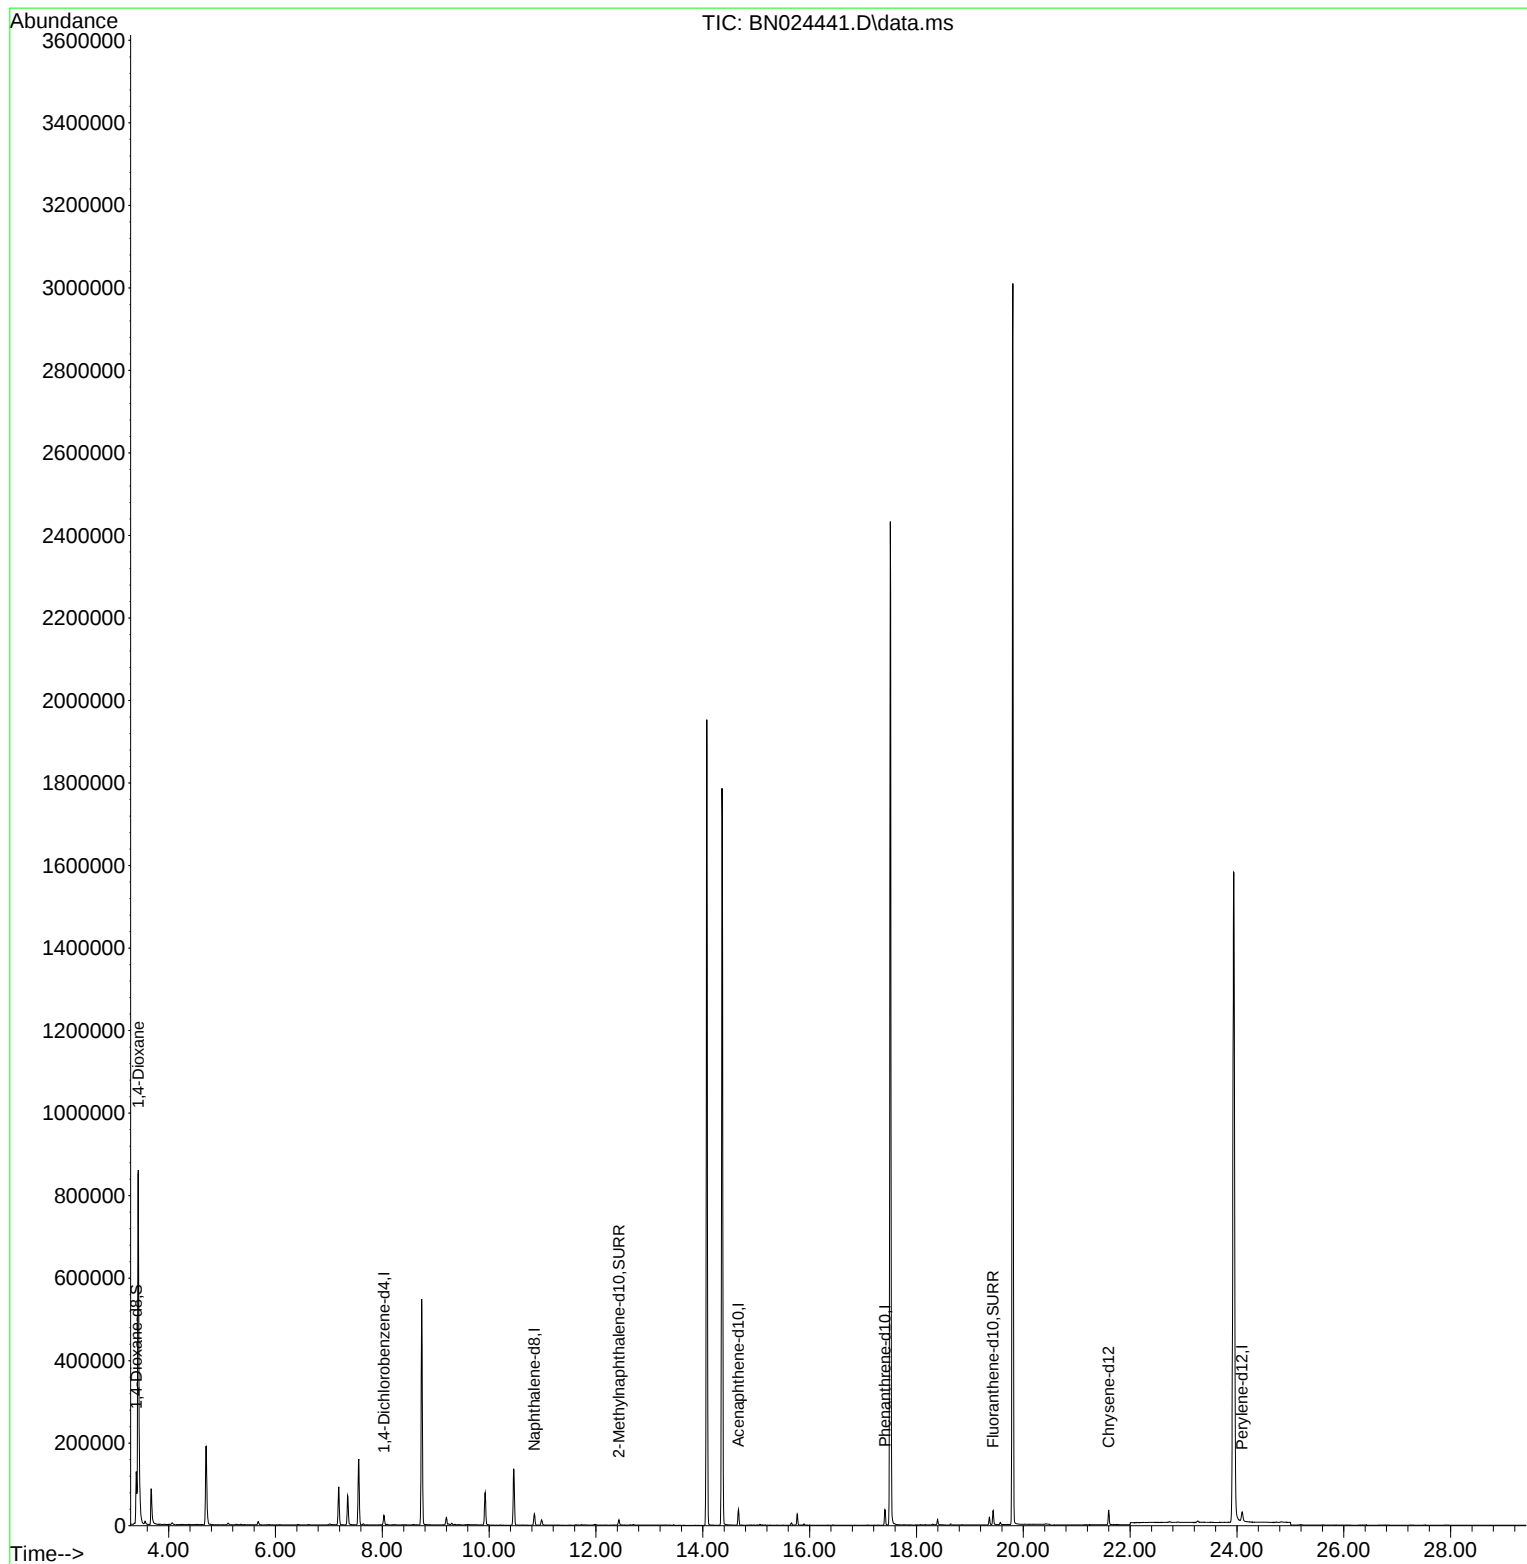

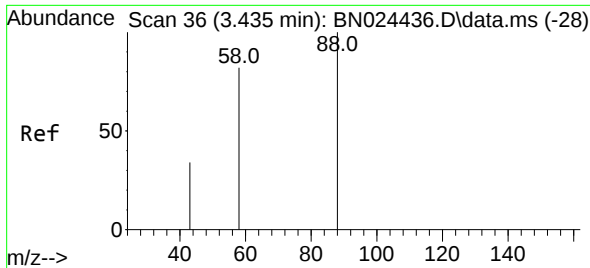

#2

1,4-Dioxane

Concen: 44.400 ng/ul

RT: 3.431 min Scan# 31

Delta R.T. -0.004 min

Lab File: BN024441.D


Acq: 21 Mar 2023 10:14

Instrument :

BNA_N

ClientSampleId :

H0A29

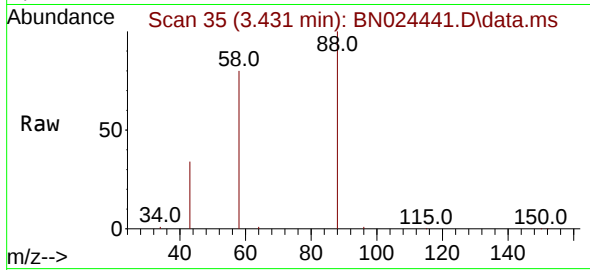

Tgt Ion: 88 Resp: 623660

Ion Ratio Lower Upper

88 100

43 34.0 32.1 48.1

58 80.4 55.1 82.7

